

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018559.D
 Acq On : 04 Dec 2023 12:04
 Operator : MA/JU
 Sample : 05439-21
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COAL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018559.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	36	rBV	73677	91466	0.93%	0.106%
2	3.552	76	79	87	rBV	56654	84337	0.86%	0.097%
3	3.687	99	102	118	rBV	508140	763564	7.79%	0.882%
4	3.922	140	142	149	rVB3	17512	25512	0.26%	0.029%
5	4.022	155	159	163	rVB2	22917	28473	0.29%	0.033%
6	7.022	662	669	677	rVB	319772	490950	5.01%	0.567%
7	7.193	691	698	709	rVB	1317827	2005795	20.46%	2.317%
8	7.387	724	731	739	rBV	1112291	1706737	17.41%	1.972%
9	7.475	741	746	752	rVB4	23065	42842	0.44%	0.049%
10	7.857	804	811	818	rVV	1237163	1944116	19.83%	2.246%
11	7.928	818	823	828	rVB3	9661	14590	0.15%	0.017%
12	8.563	924	931	944	rBV	929596	1468552	14.98%	1.697%
13	9.016	1000	1008	1016	rBV	1481837	2362213	24.10%	2.729%
14	9.446	1075	1081	1086	rVB2	22033	36844	0.38%	0.043%
15	9.740	1121	1131	1139	rBV	978947	1588425	16.21%	1.835%
16	10.275	1214	1222	1230	rBV	1642538	2683557	27.38%	3.100%
17	10.651	1279	1286	1296	rVB	1757291	2969702	30.30%	3.431%
18	10.793	1301	1310	1322	rBV	1643777	2738370	27.94%	3.164%
19	11.934	1498	1504	1511	rBV3	25960	48492	0.49%	0.056%
20	12.151	1536	1541	1545	rBV5	5596	10664	0.11%	0.012%
21	12.240	1552	1556	1564	rVB2	36746	57976	0.59%	0.067%
22	13.116	1699	1705	1708	rVB4	7651	14175	0.14%	0.016%
23	13.392	1745	1752	1757	rBV	99745	157609	1.61%	0.182%
24	13.457	1759	1763	1766	rBV2	7194	10947	0.11%	0.013%
25	13.716	1803	1807	1812	rBV4	6394	13365	0.14%	0.015%
26	13.904	1832	1839	1849	rBV	3869322	5275376	53.82%	6.095%
27	14.181	1878	1886	1896	rBV	4171662	6048621	61.71%	6.988%
28	14.392	1919	1922	1925	rVB2	8109	11062	0.11%	0.013%
29	14.487	1931	1938	1946	rBV	2913385	4332337	44.20%	5.005%
30	14.681	1965	1971	1976	rBV	250944	366991	3.74%	0.424%
31	14.904	2005	2009	2013	rVB5	14529	21003	0.21%	0.024%
32	15.481	2098	2107	2116	rBV	5497791	8176305	83.42%	9.447%
33	15.592	2120	2126	2140	rVV	1319592	1817451	18.54%	2.100%
34	15.716	2143	2147	2152	rVB2	27126	41869	0.43%	0.048%
35	16.263	2237	2240	2243	rVB5	11061	11003	0.11%	0.013%
36	16.722	2312	2318	2321	rBV4	7043	13317	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018559.D
 Acq On : 04 Dec 2023 12:04
 Operator : MA/JU
 Sample : 05439-21
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	16.910	2346	2350	2355	rVB2	10841	18724	0.19%	0.022%
38	17.233	2398	2405	2412	rBV	3554737	5056496	51.59%	5.842%
39	17.333	2415	2422	2432	rVV	6097098	8969055	91.50%	10.362%
40	17.910	2517	2520	2524	rVB2	16196	16090	0.16%	0.019%
41	18.122	2551	2556	2562	rBV2	149474	201275	2.05%	0.233%
42	19.145	2726	2730	2734	rVB3	75254	98752	1.01%	0.114%
43	19.210	2737	2741	2745	rBV	80349	112801	1.15%	0.130%
44	19.357	2762	2766	2770	rBV3	67165	91397	0.93%	0.106%
45	19.569	2796	2802	2809	rBV	7389818	9801926	100.00%	11.325%
46	21.033	3048	3051	3061	rBV5	110368	213193	2.18%	0.246%
47	21.316	3094	3099	3105	rBV	3398064	4133673	42.17%	4.776%
48	23.539	3470	3477	3485	rBV2	3467370	6767808	69.05%	7.819%
49	23.692	3497	3503	3513	rVB	1816898	3597879	36.71%	4.157%




Sum of corrected areas: 86553677

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018559.D
Acq On : 04 Dec 2023 12:04
Operator : MA/JU
Sample : 05439-21
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COAL9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

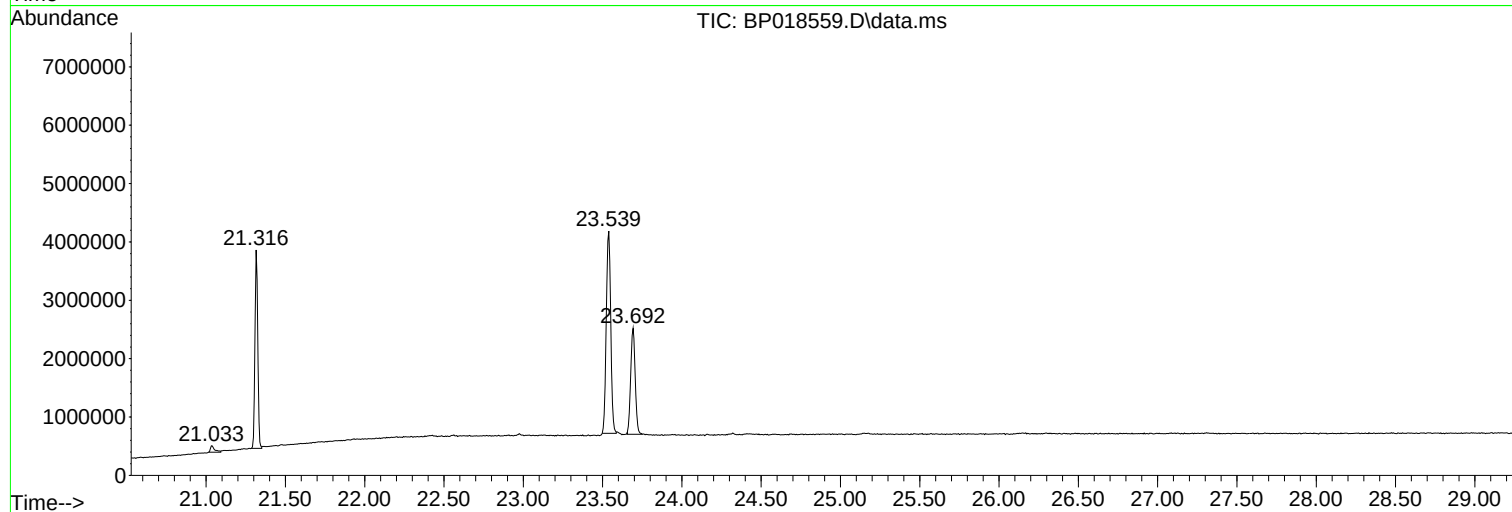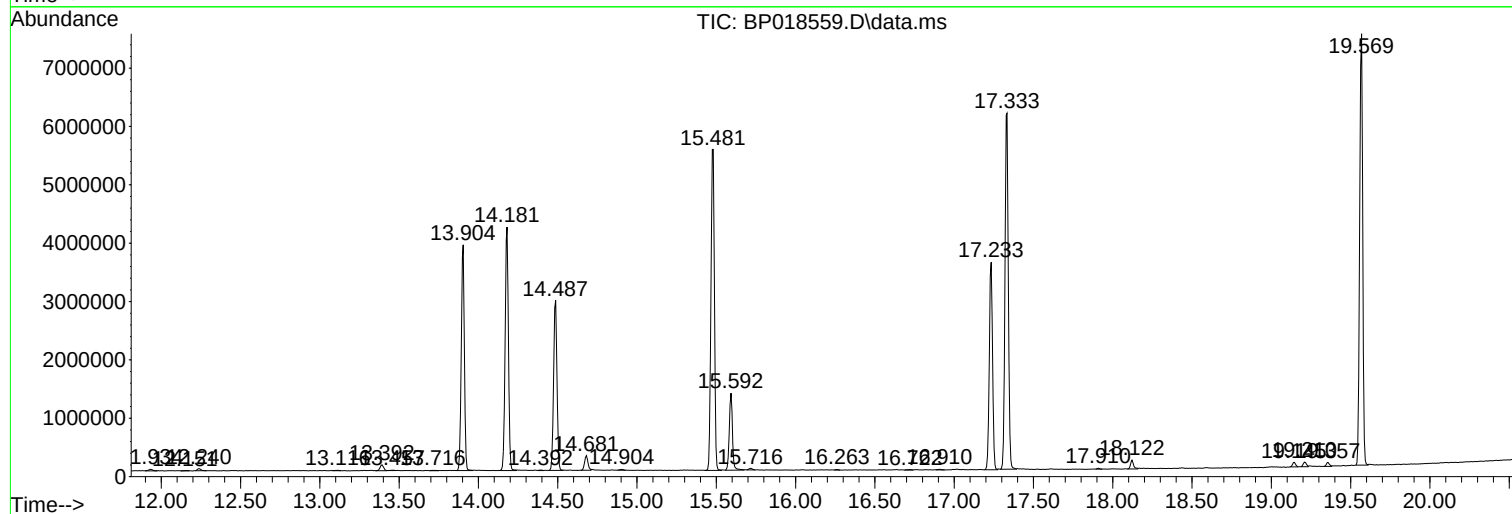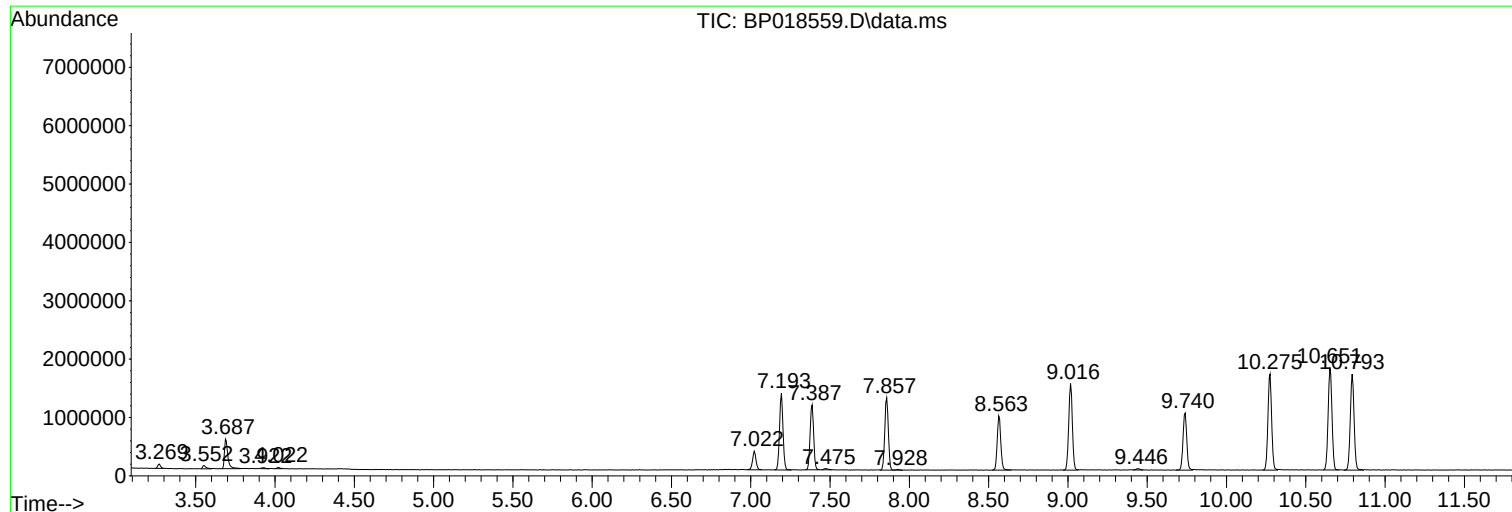

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018559.D
Acq On : 04 Dec 2023 12:04
Operator : MA/JU
Sample : 05439-21
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AL9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018559.D
Acq On : 04 Dec 2023 12:04
Operator : MA/JU
Sample : 05439-21
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AL9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc