

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018560.D
 Acq On : 04 Dec 2023 12:38
 Operator : MA/JU
 Sample : 05439-22
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COAMO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018560.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	38	rVB	81509	103439	1.02%	0.114%
2	3.687	98	102	117	rBV	466022	693028	6.86%	0.764%
3	3.922	138	142	148	rBV3	20102	34131	0.34%	0.038%
4	4.022	154	159	162	rBV2	24912	35324	0.35%	0.039%
5	6.852	634	640	642	rBV2	9117	14167	0.14%	0.016%
6	7.022	660	669	678	rVB	359685	545801	5.40%	0.602%
7	7.193	691	698	708	rVB	1458910	2239590	22.17%	2.468%
8	7.387	723	731	740	rBV	1297967	1960347	19.40%	2.161%
9	7.481	743	747	751	rBV4	13052	17990	0.18%	0.020%
10	7.858	804	811	820	rBV	1243146	1932923	19.13%	2.130%
11	8.563	923	931	942	rBV	1061574	1665186	16.48%	1.835%
12	9.016	1001	1008	1018	rBV	1685724	2676439	26.49%	2.950%
13	9.440	1076	1080	1082	rBV2	7223	10955	0.11%	0.012%
14	9.740	1123	1131	1141	rBV	1157924	1900373	18.81%	2.094%
15	10.275	1214	1222	1233	rBV	1898324	3120738	30.89%	3.439%
16	10.652	1278	1286	1295	rBV	1785773	3012286	29.82%	3.320%
17	10.793	1302	1310	1319	rBV	1804711	2956793	29.27%	3.259%
18	11.940	1500	1505	1510	rVB3	8543	15978	0.16%	0.018%
19	12.240	1550	1556	1563	rVB3	40814	69219	0.69%	0.076%
20	12.669	1624	1629	1634	rBV5	4937	10347	0.10%	0.011%
21	13.393	1747	1752	1758	rVV2	37684	57982	0.57%	0.064%
22	13.457	1759	1763	1768	rVB4	8805	13063	0.13%	0.014%
23	13.904	1832	1839	1850	rBV	4083920	5673337	56.16%	6.253%
24	14.181	1879	1886	1900	rBV	4705984	6750953	66.82%	7.441%
25	14.487	1931	1938	1945	rBV	3072207	4354432	43.10%	4.799%
26	14.681	1965	1971	1979	rBV	249559	383440	3.80%	0.423%
27	14.898	2004	2008	2014	rVB5	12411	26054	0.26%	0.029%
28	15.475	2099	2106	2113	rBV	6098711	8791954	87.02%	9.690%
29	15.592	2120	2126	2140	rBV	1405693	1912045	18.93%	2.107%
30	15.716	2143	2147	2153	rVB2	30691	49223	0.49%	0.054%
31	16.263	2236	2240	2244	rVB7	7557	13076	0.13%	0.014%
32	16.910	2347	2350	2354	rBV3	8890	12167	0.12%	0.013%
33	17.016	2366	2368	2373	rVB3	8307	11984	0.12%	0.013%
34	17.234	2398	2405	2412	rBV	3582505	5058821	50.07%	5.576%
35	17.334	2415	2422	2433	rBV	6646659	9474351	93.78%	10.442%
36	17.610	2466	2469	2475	rVB3	11059	17519	0.17%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018560.D
Acq On : 04 Dec 2023 12:38
Operator : MA/JU
Sample : 05439-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COAM0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	18.122	2552	2556	2563	rBV5	38522	58070	0.57%	0.064%
38	19.145	2726	2730	2736	rBV2	79304	104508	1.03%	0.115%
39	19.210	2737	2741	2748	rBV	75561	112014	1.11%	0.123%
40	19.357	2763	2766	2770	rBV6	29995	38360	0.38%	0.042%
41	19.569	2796	2802	2812	rBV	7586208	10102835	100.00%	11.135%
42	21.316	3095	3099	3105	rBV	3120348	3940297	39.00%	4.343%
43	23.539	3470	3477	3495	rVB	3785001	7153975	70.81%	7.885%
44	23.692	3496	3503	3517	rVB	1831710	3606838	35.70%	3.975%




Sum of corrected areas: 90732352

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018560.D
Acq On : 04 Dec 2023 12:38
Operator : MA/JU
Sample : 05439-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COAM0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

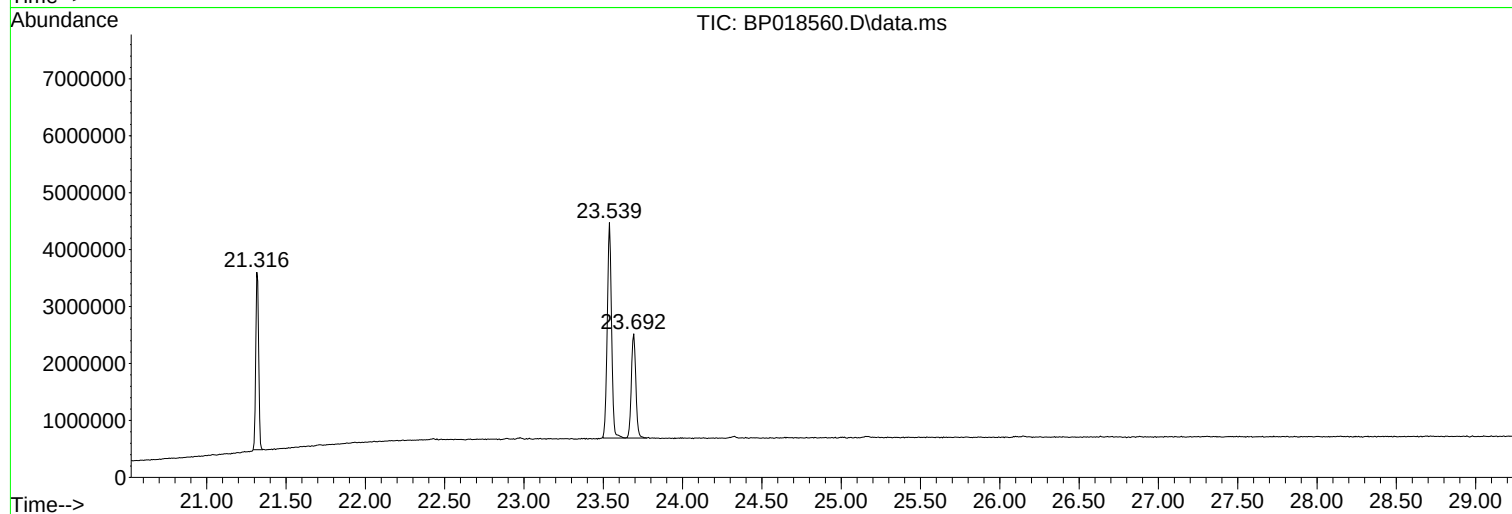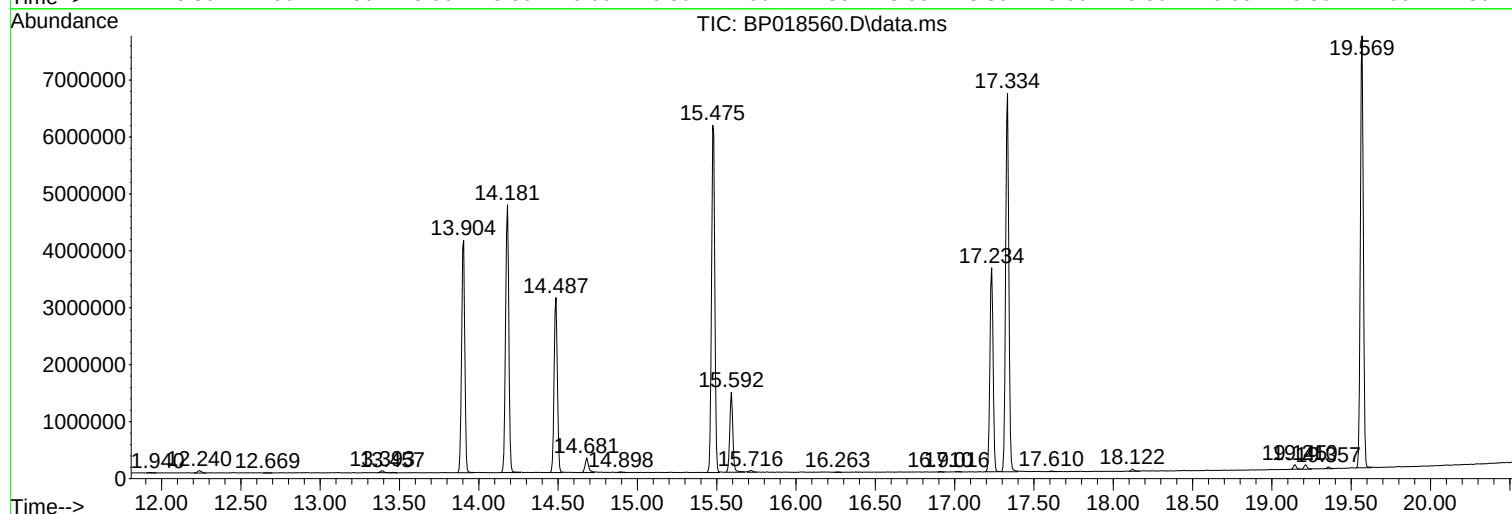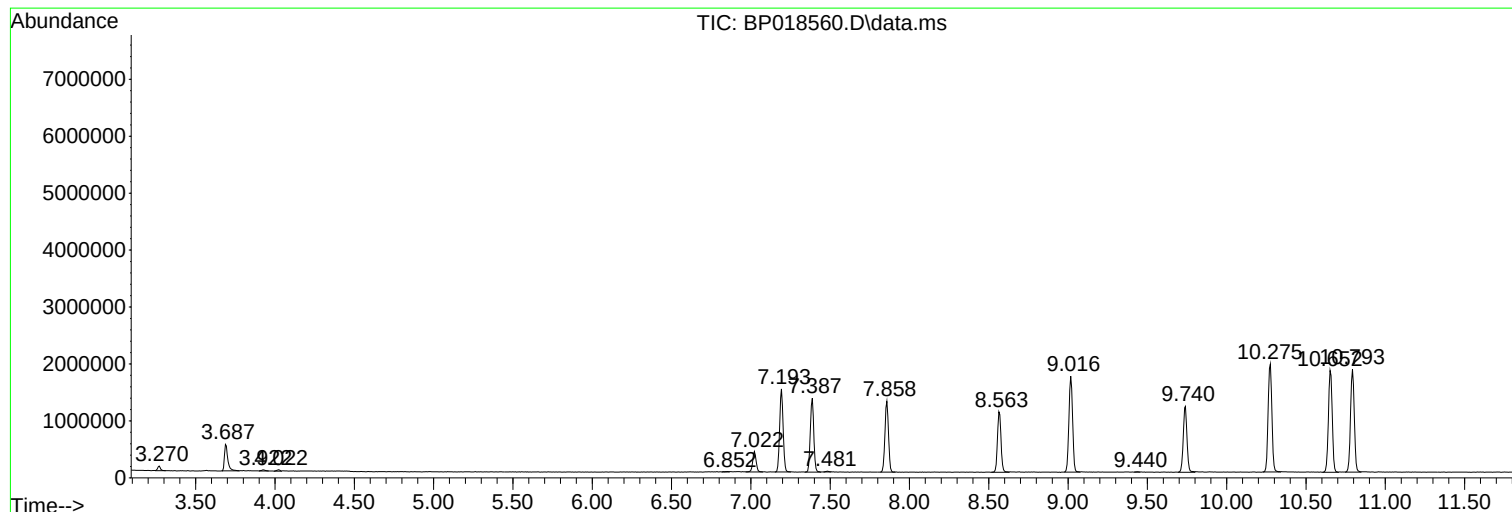

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018560.D
Acq On : 04 Dec 2023 12:38
Operator : MA/JU
Sample : 05439-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AM0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018560.D
Acq On : 04 Dec 2023 12:38
Operator : MA/JU
Sample : 05439-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AM0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------