

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018561.D
 Acq On : 04 Dec 2023 13:12
 Operator : MA/JU
 Sample : 05416-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AK4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018561.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	36	rVB	79346	96315	1.31%	0.134%
2	3.693	99	103	112	rBV	434388	635028	8.66%	0.885%
3	3.928	139	143	149	rVB2	24656	36669	0.50%	0.051%
4	4.022	155	159	166	rBV2	27065	38259	0.52%	0.053%
5	5.787	453	459	464	rBV4	9372	16438	0.22%	0.023%
6	5.899	476	478	484	rVB	5224	10031	0.14%	0.014%
7	5.958	484	488	489	rBV4	5677	8642	0.12%	0.012%
8	6.752	618	623	625	rBV4	5751	7586	0.10%	0.011%
9	7.022	661	669	677	rVB	283462	434955	5.93%	0.606%
10	7.193	688	698	709	rVB	1208349	1857518	25.32%	2.588%
11	7.387	724	731	738	rBV	1041748	1615447	22.02%	2.251%
12	7.481	743	747	749	rVV5	7274	10481	0.14%	0.015%
13	7.858	804	811	819	rVB	1310746	2043633	27.86%	2.848%
14	7.922	819	822	825	rBV4	6844	9176	0.13%	0.013%
15	8.563	925	931	940	rBV	824712	1263847	17.23%	1.761%
16	9.016	1000	1008	1019	rBV	1301636	2090734	28.50%	2.913%
17	9.440	1075	1080	1084	rBV5	17870	27030	0.37%	0.038%
18	9.740	1122	1131	1141	rBV	824731	1368351	18.65%	1.907%
19	10.269	1211	1221	1231	rBV	1422090	2349779	32.03%	3.274%
20	10.652	1278	1286	1293	rBV	1782951	2925182	39.88%	4.076%
21	10.716	1293	1297	1302	rVB8	7232	11549	0.16%	0.016%
22	10.793	1302	1310	1319	rBV	1412194	2369256	32.30%	3.301%
23	11.216	1377	1382	1387	rBV3	5665	11294	0.15%	0.016%
24	11.457	1421	1423	1431	rVB2	5572	9770	0.13%	0.014%
25	11.940	1499	1505	1512	rBV4	39738	78024	1.06%	0.109%
26	12.240	1550	1556	1562	rBV	32620	51996	0.71%	0.072%
27	13.098	1698	1702	1703	rBV3	7651	7680	0.10%	0.011%
28	13.387	1745	1751	1756	rBV4	18669	37617	0.51%	0.052%
29	13.457	1761	1763	1769	rVB7	8373	11086	0.15%	0.015%
30	13.728	1806	1809	1812	rBV2	5410	7942	0.11%	0.011%
31	13.898	1832	1838	1845	rBV	2786551	3836051	52.30%	5.345%
32	14.181	1875	1886	1896	rBV	3091933	4651545	63.41%	6.481%
33	14.487	1931	1938	1948	rBV	2569959	3798461	51.78%	5.293%
34	14.569	1948	1952	1957	rVB2	36853	52538	0.72%	0.073%
35	14.681	1964	1971	1981	rBV2	150093	254418	3.47%	0.354%
36	14.904	2004	2009	2016	rVB8	12330	24231	0.33%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018561.D
 Acq On : 04 Dec 2023 13:12
 Operator : MA/JU
 Sample : 05416-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AK4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.157	2049	2052	2058	rBV	16557	25312	0.35%	0.035%
38	15.292	2071	2075	2077	rBV3	8092	11153	0.15%	0.016%
39	15.475	2100	2106	2114	rBV	4299177	6012366	81.96%	8.377%
40	15.592	2120	2126	2137	rBV	829211	1140735	15.55%	1.589%
41	15.716	2143	2147	2152	rVB3	19717	28210	0.38%	0.039%
42	16.551	2287	2289	2292	rVB4	7332	7544	0.10%	0.011%
43	16.910	2347	2350	2354	rVB2	8079	11541	0.16%	0.016%
44	17.233	2398	2405	2412	rVB	2577292	3741850	51.01%	5.214%
45	17.334	2415	2422	2434	rBV	4387308	6350962	86.58%	8.849%
46	17.533	2452	2456	2459	rVB3	8158	8314	0.11%	0.012%
47	17.904	2514	2519	2524	rBV	167913	207112	2.82%	0.289%
48	18.122	2551	2556	2562	rBV3	46939	77909	1.06%	0.109%
49	18.198	2566	2569	2574	rVB2	12542	17493	0.24%	0.024%
50	19.145	2726	2730	2736	rBV2	54492	78523	1.07%	0.109%
51	19.210	2738	2741	2745	rVV	50329	62736	0.86%	0.087%
52	19.357	2763	2766	2769	rBV5	27997	29533	0.40%	0.041%
53	19.569	2796	2802	2809	rBV	5253973	6741176	91.90%	9.393%
54	21.316	3095	3099	3107	rBV	2914211	3620014	49.35%	5.044%
55	23.539	3470	3477	3486	rBV2	3928775	7335389	100.00%	10.221%
56	23.692	3496	3503	3515	rVB	2036507	4202291	57.29%	5.855%




Sum of corrected areas: 71768722

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018561.D
Acq On : 04 Dec 2023 13:12
Operator : MA/JU
Sample : 05416-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AK4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

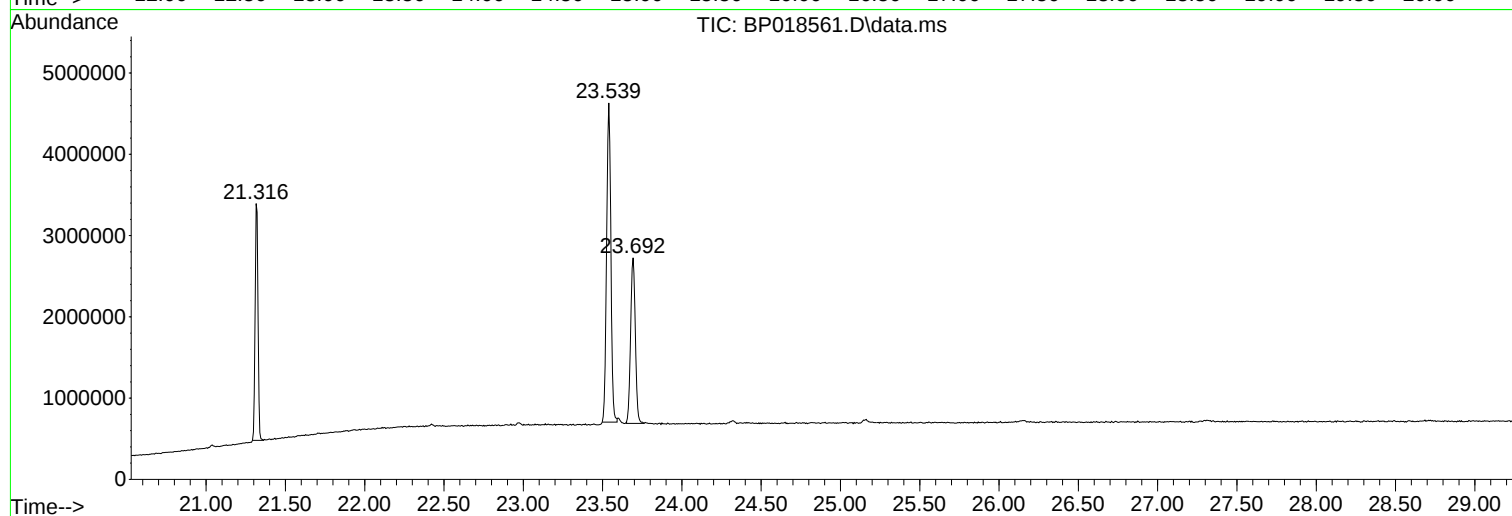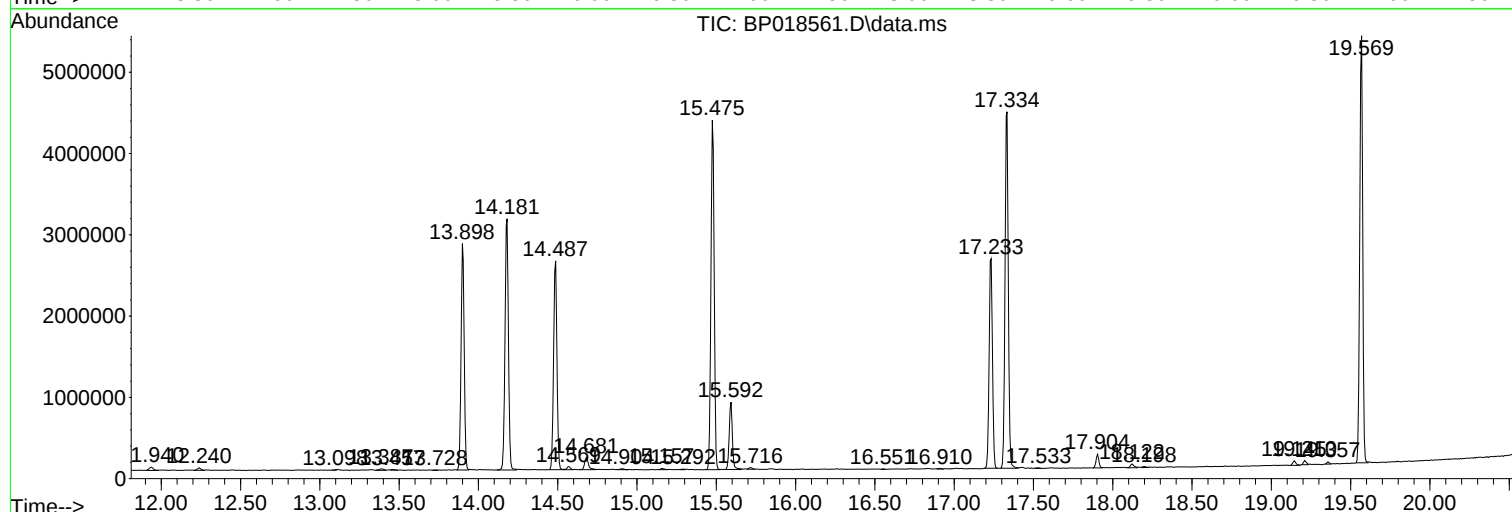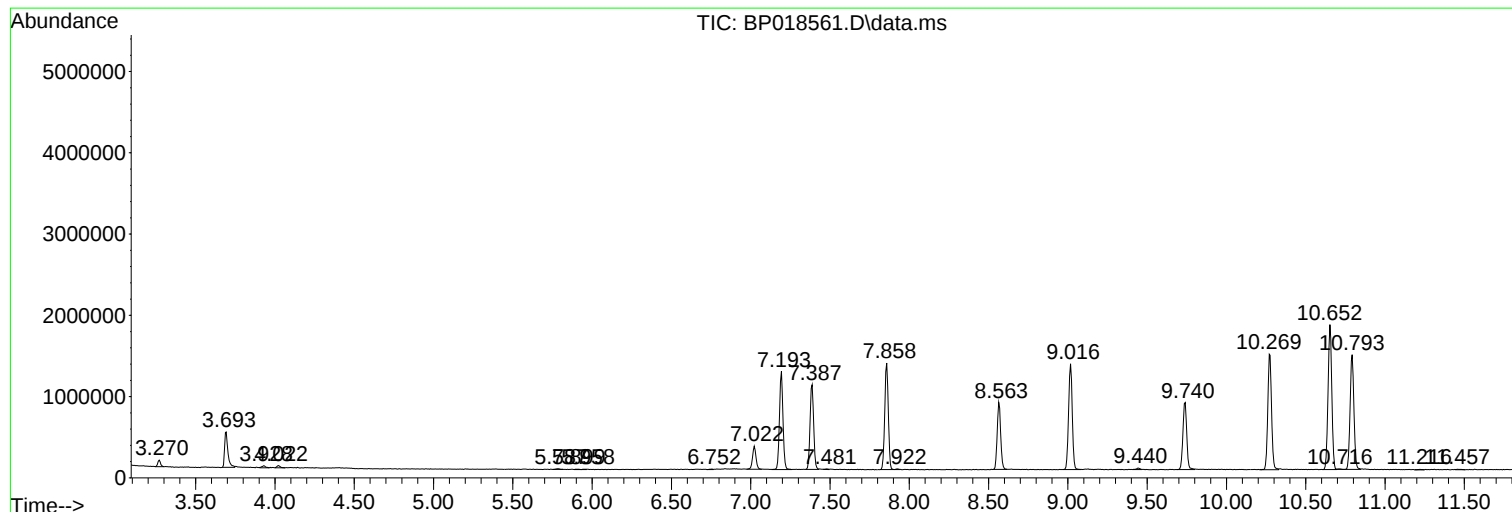

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018561.D
Acq On : 04 Dec 2023 13:12
Operator : MA/JU
Sample : 05416-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AK4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018561.D
Acq On : 04 Dec 2023 13:12
Operator : MA/JU
Sample : 05416-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AK4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc