

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018563.D
 Acq On : 04 Dec 2023 14:20
 Operator : MA/JU
 Sample : 05441-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018563.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	28	rBV2	55022	75452	0.63%	0.077%
2	3.269	28	31	36	rVB	74524	95176	0.79%	0.097%
3	3.564	77	81	84	rVB2	10783	13137	0.11%	0.013%
4	3.687	98	102	116	rBV	430165	668384	5.54%	0.679%
5	3.928	138	143	149	rVB2	20102	32388	0.27%	0.033%
6	4.022	155	159	166	rVB2	19660	27040	0.22%	0.027%
7	7.022	663	669	678	rVB	375660	569127	4.72%	0.578%
8	7.193	691	698	710	rVB	1408307	2146725	17.79%	2.180%
9	7.387	723	731	742	rBV	1250187	1972079	16.34%	2.002%
10	7.481	744	747	752	rVB3	9591	16868	0.14%	0.017%
11	7.857	804	811	818	rBV	1139205	1796071	14.88%	1.824%
12	8.563	924	931	941	rBV	1121477	1723250	14.28%	1.750%
13	8.681	949	951	957	rVB3	9393	12676	0.11%	0.013%
14	9.016	1001	1008	1021	rBV	1678533	2615830	21.67%	2.656%
15	9.440	1076	1080	1086	rVB3	21541	36852	0.31%	0.037%
16	9.740	1121	1131	1146	rBV	1196544	1967070	16.30%	1.997%
17	10.275	1214	1222	1231	rBV	1954216	3196657	26.49%	3.246%
18	10.651	1279	1286	1295	rBV	1741576	2826566	23.42%	2.870%
19	10.793	1301	1310	1318	rBV	1897457	3087074	25.58%	3.134%
20	11.934	1498	1504	1509	rVB3	18070	32305	0.27%	0.033%
21	12.240	1549	1556	1562	rBV2	39153	67628	0.56%	0.069%
22	13.392	1744	1752	1758	rBV2	48771	81597	0.68%	0.083%
23	13.457	1759	1763	1767	rVB4	9497	14709	0.12%	0.015%
24	13.904	1832	1839	1846	rBV	4281389	5971216	49.48%	6.063%
25	14.181	1875	1886	1895	rBV	4708902	6840223	56.68%	6.945%
26	14.487	1931	1938	1948	rBV	2950268	4280682	35.47%	4.346%
27	14.569	1948	1952	1957	rVB3	7813	15516	0.13%	0.016%
28	14.681	1965	1971	1984	rBV2	345239	532735	4.41%	0.541%
29	14.839	1993	1998	2003	rBV5	6439	13161	0.11%	0.013%
30	14.904	2005	2009	2016	rVB5	20708	36650	0.30%	0.037%
31	15.481	2100	2107	2115	rBV	6240252	9198729	76.22%	9.340%
32	15.592	2120	2126	2139	rVV	1786338	2384256	19.76%	2.421%
33	15.716	2143	2147	2153	rVB2	29459	48620	0.40%	0.049%
34	17.233	2398	2405	2413	rBV	3715598	5219275	43.25%	5.299%
35	17.333	2415	2422	2434	rVV	7476729	10595202	87.79%	10.758%
36	17.610	2465	2469	2473	rVB3	9915	14763	0.12%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018563.D
Acq On : 04 Dec 2023 14:20
Operator : MA/JU
Sample : 05441-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	18.122	2552	2556	2563	rBV2	133266	174151	1.44%	0.177%
38	18.198	2566	2569	2573	rVB3	12716	16462	0.14%	0.017%
39	19.145	2726	2730	2735	rBV	93033	119156	0.99%	0.121%
40	19.210	2737	2741	2745	rBV	97184	137454	1.14%	0.140%
41	19.357	2762	2766	2772	rBV4	107952	141761	1.17%	0.144%
42	19.569	2796	2802	2809	rBV	9373907	12068851	100.00%	12.254%
43	21.321	3095	3100	3107	rBV	3742887	4719076	39.10%	4.791%
44	23.539	3470	3477	3485	rBV2	4558976	8887479	73.64%	9.024%
45	23.692	3497	3503	3512	rVB	2085103	4000614	33.15%	4.062%




Sum of corrected areas: 98490693

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018563.D
Acq On : 04 Dec 2023 14:20
Operator : MA/JU
Sample : 05441-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

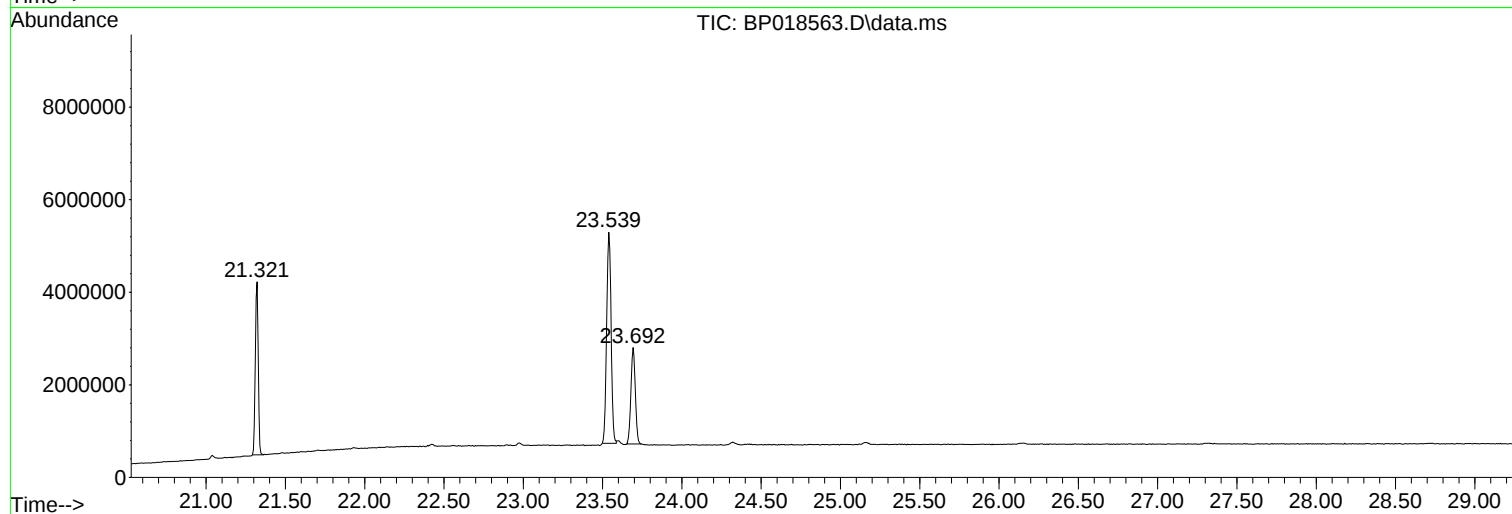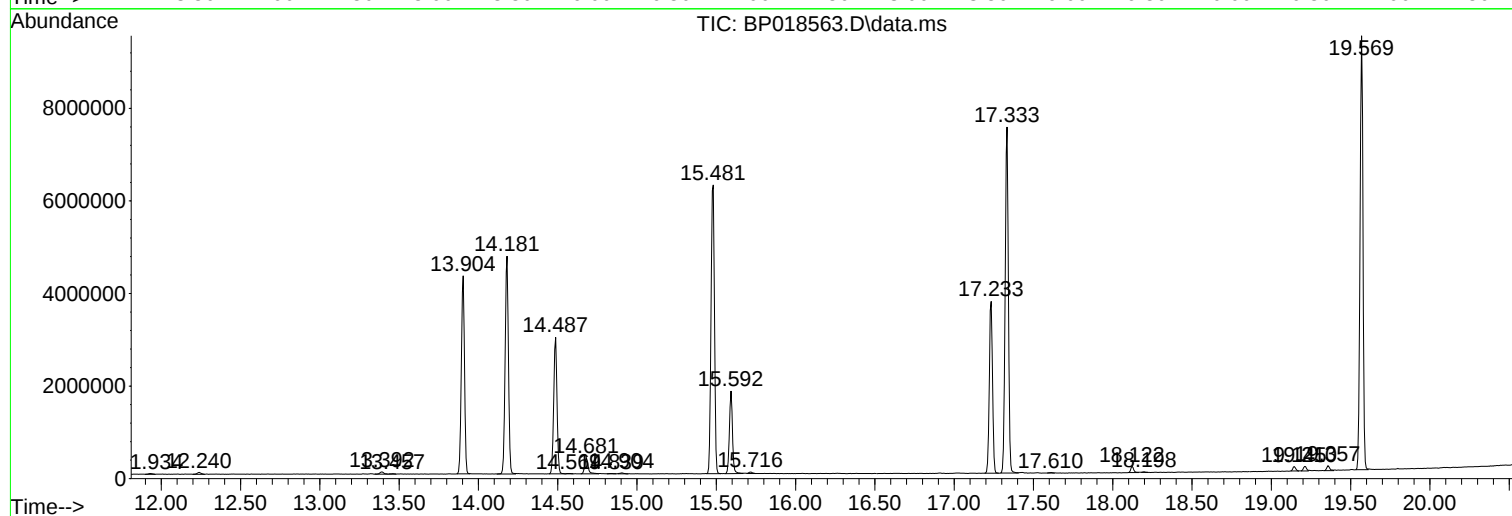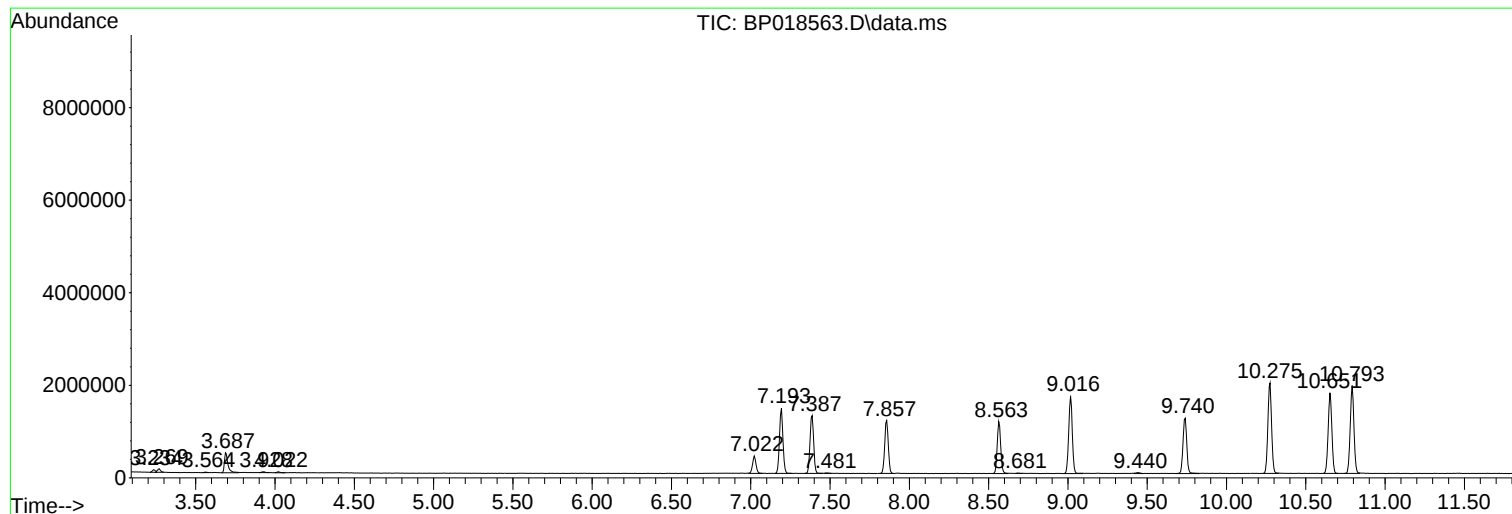

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018563.D
Acq On : 04 Dec 2023 14:20
Operator : MA/JU
Sample : 05441-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018563.D
Acq On : 04 Dec 2023 14:20
Operator : MA/JU
Sample : 05441-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------