

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018566.D
 Acq On : 04 Dec 2023 16:36
 Operator : MA/JU
 Sample : 05441-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018566.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	22	26	28	rBV2	35619	48967	0.59%	0.064%
2	3.269	28	31	35	rVV	65307	82525	0.99%	0.108%
3	3.305	35	37	44	rVB5	15504	22646	0.27%	0.030%
4	3.687	98	102	113	rBV	367703	539615	6.49%	0.708%
5	3.928	137	143	147	rBV2	20264	31060	0.37%	0.041%
6	4.016	155	158	164	rVB2	21683	31962	0.38%	0.042%
7	5.134	344	348	351	rVB2	7779	10045	0.12%	0.013%
8	5.287	371	374	380	rVB4	5725	11171	0.13%	0.015%
9	6.269	535	541	547	rVB2	10771	23065	0.28%	0.030%
10	7.022	663	669	677	rVB	249971	380417	4.57%	0.499%
11	7.193	689	698	708	rBV	1243564	1937559	23.29%	2.542%
12	7.387	724	731	742	rBV	1047833	1600234	19.23%	2.099%
13	7.487	744	748	751	rBV4	7628	10841	0.13%	0.014%
14	7.857	804	811	820	rBV	1151916	1797850	21.61%	2.359%
15	8.563	923	931	939	rBV	763054	1165853	14.01%	1.529%
16	9.016	1001	1008	1017	rBV	1434011	2282893	27.44%	2.995%
17	9.440	1075	1080	1086	rVB5	11308	15459	0.19%	0.020%
18	9.740	1122	1131	1140	rBV	970118	1600864	19.24%	2.100%
19	10.269	1213	1221	1231	rBV	1578121	2622837	31.52%	3.441%
20	10.651	1278	1286	1294	rBV	1664490	2766435	33.25%	3.629%
21	10.793	1302	1310	1320	rBV	1158644	1894263	22.77%	2.485%
22	11.469	1418	1425	1435	rVB3	39909	78158	0.94%	0.103%
23	12.240	1549	1556	1562	rVB2	34281	67431	0.81%	0.088%
24	13.110	1699	1704	1707	rBV2	6058	8414	0.10%	0.011%
25	13.392	1747	1752	1757	rVB4	23452	35956	0.43%	0.047%
26	13.457	1759	1763	1765	rBV4	7966	11406	0.14%	0.015%
27	13.904	1832	1839	1850	rBV	3517535	4951931	59.51%	6.496%
28	14.181	1876	1886	1897	rBV2	3668311	5629499	67.66%	7.385%
29	14.486	1930	1938	1947	rBV	2701795	3956424	47.55%	5.190%
30	14.569	1949	1952	1955	rBV4	7424	11267	0.14%	0.015%
31	14.681	1963	1971	1979	rBV2	170914	281583	3.38%	0.369%
32	14.839	1996	1998	2003	rBV2	6740	8539	0.10%	0.011%
33	14.904	2005	2009	2013	rVB4	10036	15804	0.19%	0.021%
34	15.475	2098	2106	2112	rBV	5068947	7554304	90.79%	9.910%
35	15.592	2120	2126	2136	rBV	1258367	1695040	20.37%	2.224%
36	15.716	2143	2147	2152	rVB2	23339	35293	0.42%	0.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018566.D
 Acq On : 04 Dec 2023 16:36
 Operator : MA/JU
 Sample : 05441-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	16.263	2237	2240	2244	rVB3	7683	11698	0.14%	0.015%
38	16.910	2346	2350	2356	rVB5	8695	13575	0.16%	0.018%
39	17.227	2398	2404	2412	rBV	3093697	4450944	53.49%	5.839%
40	17.333	2415	2422	2432	rBV	5332754	7742791	93.05%	10.157%
41	17.610	2464	2469	2472	rBV2	6799	11623	0.14%	0.015%
42	17.704	2483	2485	2489	rVB3	10687	12171	0.15%	0.016%
43	18.122	2552	2556	2562	rBV3	55992	73425	0.88%	0.096%
44	18.586	2632	2635	2638	rBV4	10914	14914	0.18%	0.020%
45	19.145	2726	2730	2736	rBV3	67763	93543	1.12%	0.123%
46	19.210	2737	2741	2747	rVV	71841	99911	1.20%	0.131%
47	19.357	2763	2766	2772	rBV6	31824	44896	0.54%	0.059%
48	19.569	2796	2802	2810	rBV	6596920	8320747	100.00%	10.916%
49	21.316	3095	3099	3108	rBV	2648607	3243478	38.98%	4.255%
50	23.539	3470	3477	3485	rBV2	3039654	5840665	70.19%	7.662%
51	23.692	3497	3503	3515	rVB	1547737	3035737	36.48%	3.982%




Sum of corrected areas: 76227728

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018566.D
Acq On : 04 Dec 2023 16:36
Operator : MA/JU
Sample : 05441-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

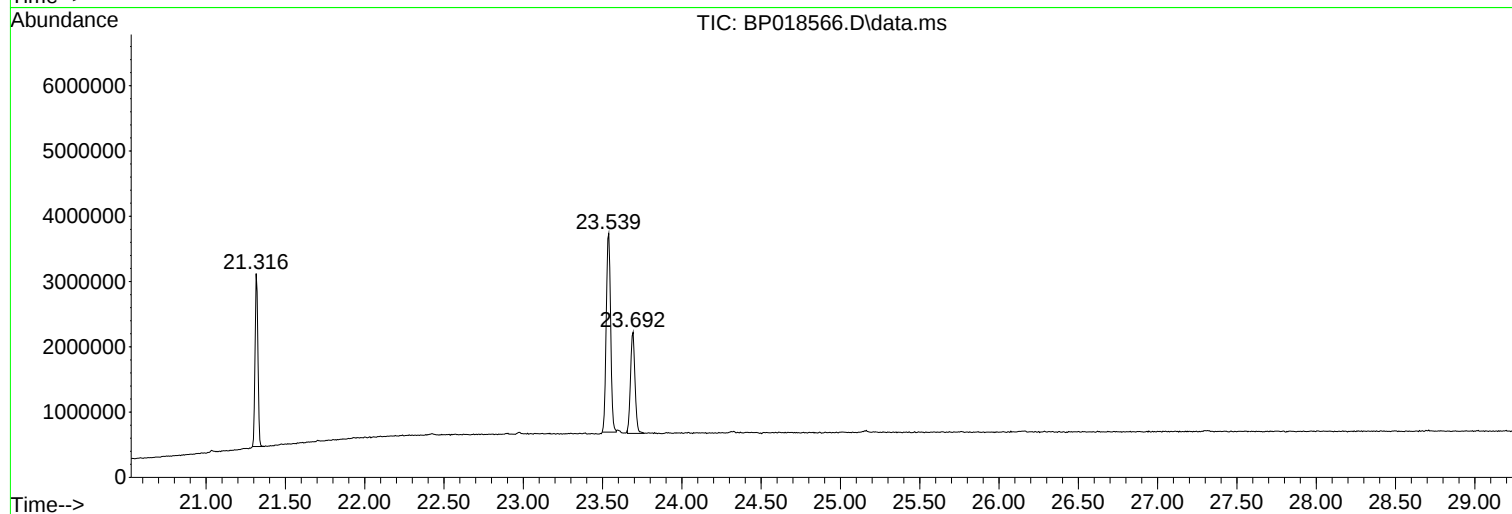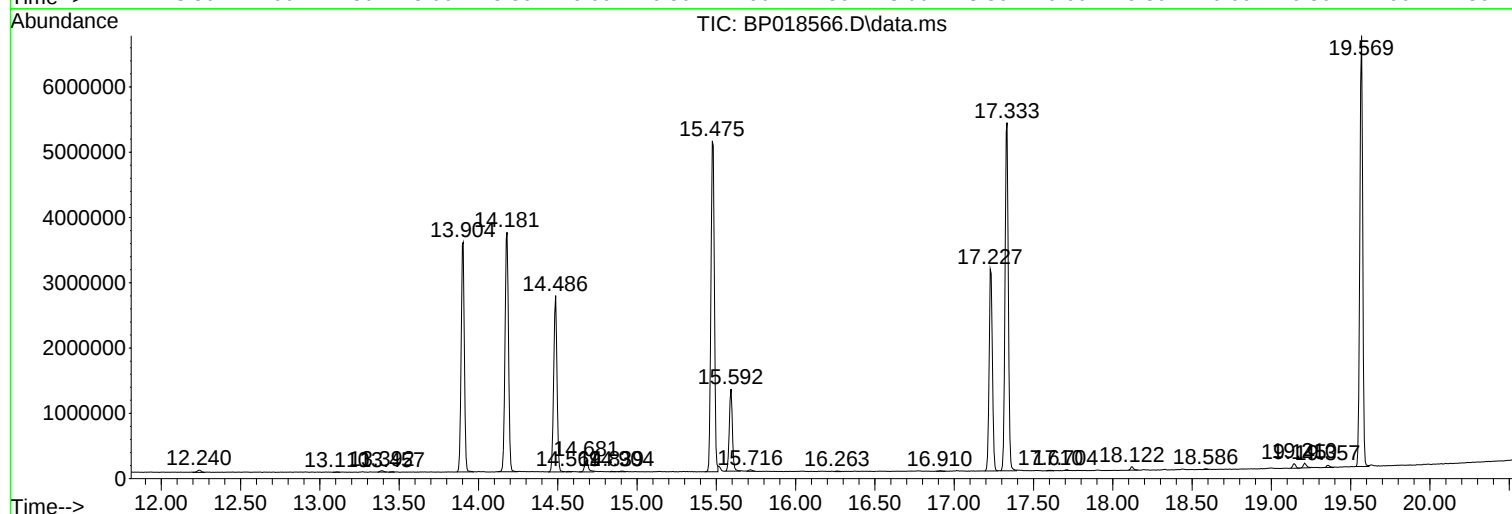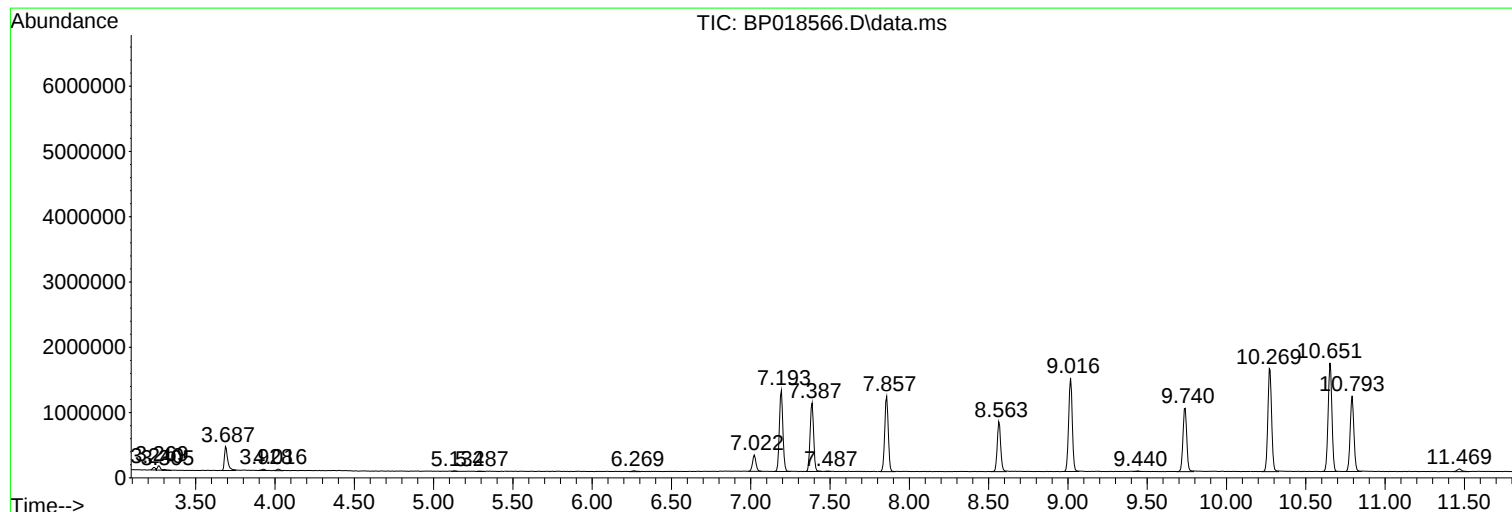

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018566.D
Acq On : 04 Dec 2023 16:36
Operator : MA/JU
Sample : 05441-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018566.D
Acq On : 04 Dec 2023 16:36
Operator : MA/JU
Sample : 05441-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc