

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018571.D
 Acq On : 04 Dec 2023 19:26
 Operator : MA/JU
 Sample : 05441-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG2

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018571.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	38	rVB	101733	129803	1.01%	0.121%
2	3.687	99	102	115	rBV	562208	842705	6.56%	0.786%
3	4.022	155	159	167	rVB	30333	46089	0.36%	0.043%
4	4.105	171	173	178	rVB2	21859	25971	0.20%	0.024%
5	5.128	345	347	354	rVB2	10838	13575	0.11%	0.013%
6	7.022	663	669	677	rVB	427079	652699	5.08%	0.609%
7	7.193	691	698	708	rBV	1566194	2478790	19.28%	2.312%
8	7.387	719	731	739	rBV	1459447	2323842	18.08%	2.167%
9	7.481	742	747	754	rVB3	15306	35980	0.28%	0.034%
10	7.857	804	811	818	rBV	1719194	2713312	21.11%	2.531%
11	8.563	924	931	944	rBV	1269442	1966048	15.29%	1.834%
12	9.016	1001	1008	1019	rVB	2002727	3171871	24.67%	2.958%
13	9.440	1076	1080	1085	rVB2	22095	31933	0.25%	0.030%
14	9.734	1123	1130	1139	rBV	1408424	2305578	17.93%	2.150%
15	10.269	1214	1221	1236	rBV	2288279	3771940	29.34%	3.518%
16	10.651	1278	1286	1294	rBV	2568376	4197635	32.65%	3.915%
17	10.793	1302	1310	1320	rBV	2173452	3600134	28.00%	3.358%
18	11.463	1419	1424	1429	rBV6	13587	28699	0.22%	0.027%
19	12.240	1552	1556	1561	rVB2	37782	62183	0.48%	0.058%
20	12.587	1610	1615	1619	rBV7	8690	18604	0.14%	0.017%
21	13.387	1744	1751	1758	rVB3	25022	41202	0.32%	0.038%
22	13.457	1758	1763	1766	rBV5	8286	13821	0.11%	0.013%
23	13.898	1831	1838	1854	rBV	3970737	5617234	43.69%	5.239%
24	14.175	1876	1885	1892	rBV	4059412	6174165	48.03%	5.759%
25	14.481	1930	1937	1947	rVV	3012420	4469139	34.76%	4.168%
26	14.569	1949	1952	1959	rVB5	7941	13300	0.10%	0.012%
27	14.681	1962	1971	1982	rBV	317797	506768	3.94%	0.473%
28	14.904	2004	2009	2013	rBV5	17233	26691	0.21%	0.025%
29	15.145	2043	2050	2052	rBV5	12801	21842	0.17%	0.020%
30	15.339	2080	2083	2089	rVB5	8582	15283	0.12%	0.014%
31	15.475	2099	2106	2113	rBV	5931300	8319970	64.72%	7.760%
32	15.592	2119	2126	2136	rBV	1621517	2221673	17.28%	2.072%
33	15.716	2142	2147	2157	rVB2	32573	59540	0.46%	0.056%
34	15.981	2189	2192	2197	rVB2	14799	19860	0.15%	0.019%
35	16.263	2236	2240	2243	rVB3	10394	16117	0.13%	0.015%
36	16.910	2347	2350	2355	rVB6	10776	13284	0.10%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018571.D
 Acq On : 04 Dec 2023 19:26
 Operator : MA/JU
 Sample : 05441-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.233	2398	2405	2411	rBV	3734185	5290739	41.15%	4.935%
38	17.333	2415	2422	2433	rBV	6344528	9236950	71.85%	8.615%
39	17.704	2481	2485	2490	rBV2	35926	56487	0.44%	0.053%
40	17.910	2518	2520	2524	rVB4	12582	13282	0.10%	0.012%
41	18.122	2551	2556	2565	rBV	201122	276858	2.15%	0.258%
42	19.145	2725	2730	2734	rBV2	91364	125592	0.98%	0.117%
43	19.210	2737	2741	2745	rBV	95370	128574	1.00%	0.120%
44	19.357	2762	2766	2771	rBV	136614	171745	1.34%	0.160%
45	19.451	2780	2782	2783	rBV	25599	20991	0.16%	0.020%
46	19.569	2796	2802	2814	rBV	9893852	12855879	100.00%	11.991%
47	21.039	3049	3052	3056	rBV3	78424	96214	0.75%	0.090%
48	21.316	3094	3099	3108	rBV	4562193	5810018	45.19%	5.419%
49	23.539	3469	3477	3484	rBV2	5864180	11190299	87.04%	10.437%
50	23.692	3496	3503	3517	rVB	2850549	5974469	46.47%	5.572%




Sum of corrected areas: 107215377

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018571.D
Acq On : 04 Dec 2023 19:26
Operator : MA/JU
Sample : 05441-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

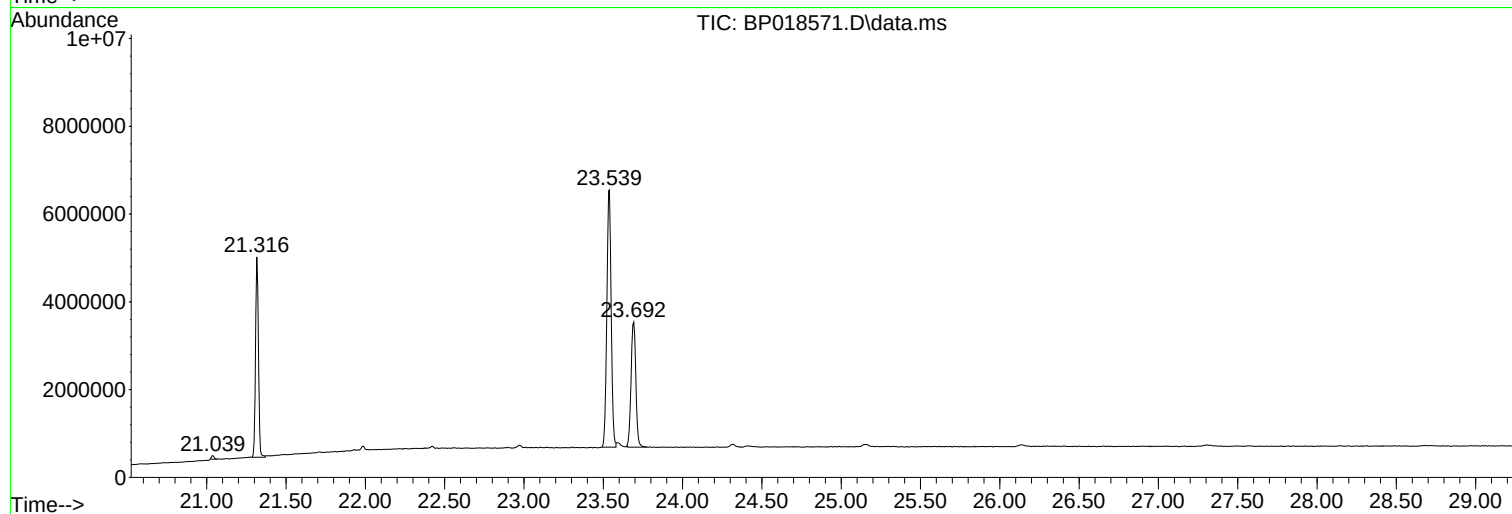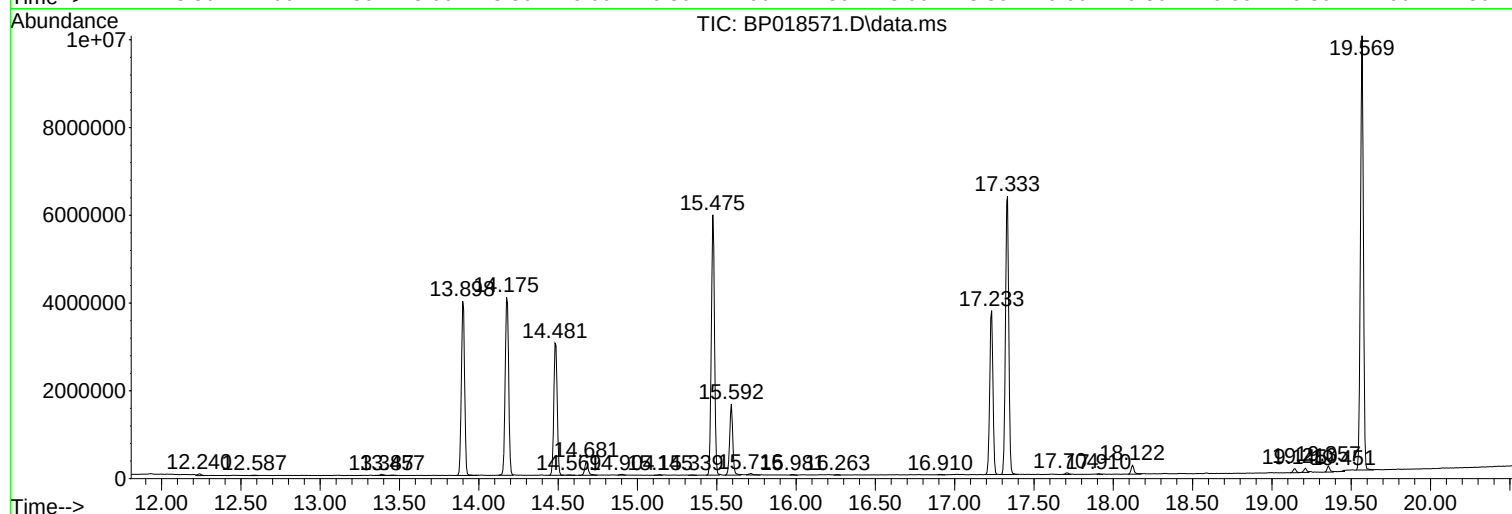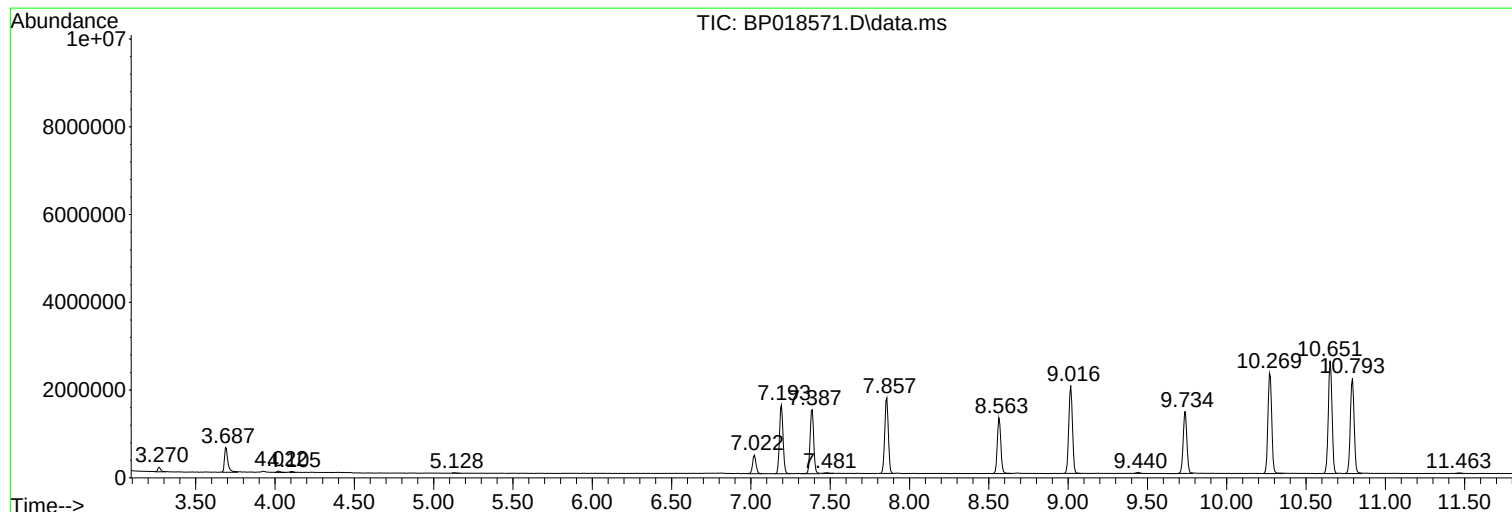

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018571.D
Acq On : 04 Dec 2023 19:26
Operator : MA/JU
Sample : 05441-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018571.D
Acq On : 04 Dec 2023 19:26
Operator : MA/JU
Sample : 05441-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc