

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018572.D
 Acq On : 04 Dec 2023 20:00
 Operator : MA/JU
 Sample : 05441-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018572.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	41	rVB	92603	122822	0.87%	0.106%
2	3.687	98	102	119	rBV	533140	814832	5.79%	0.701%
3	3.928	138	143	147	rVB2	25443	38035	0.27%	0.033%
4	4.023	155	159	164	rVB2	25431	37427	0.27%	0.032%
5	7.022	663	669	678	rVB	396932	600900	4.27%	0.517%
6	7.193	690	698	707	rBV	1635595	2571686	18.28%	2.214%
7	7.381	723	730	741	rBV	1394810	2246198	15.97%	1.934%
8	7.481	743	747	753	rBV7	11871	20736	0.15%	0.018%
9	7.858	801	811	818	rBV	1500045	2392880	17.01%	2.060%
10	8.563	923	931	941	rBV	1221864	1915961	13.62%	1.649%
11	8.681	948	951	957	rVB4	9290	15403	0.11%	0.013%
12	9.016	1000	1008	1018	rBV	1967760	3096681	22.01%	2.666%
13	9.440	1075	1080	1089	rVB2	22493	42428	0.30%	0.037%
14	9.734	1123	1130	1138	rBV	1385892	2224642	15.81%	1.915%
15	10.269	1211	1221	1236	rBV	2163422	3673517	26.11%	3.163%
16	10.652	1276	1286	1296	rVB	2244051	3697617	26.28%	3.183%
17	10.793	1300	1310	1320	rBV	2193536	3642612	25.89%	3.136%
18	11.928	1496	1503	1508	rBV5	16526	25922	0.18%	0.022%
19	12.240	1550	1556	1563	rBV2	45992	81070	0.58%	0.070%
20	13.393	1745	1752	1757	rBV2	27472	51515	0.37%	0.044%
21	13.451	1760	1762	1767	rBV2	10242	15131	0.11%	0.013%
22	13.898	1832	1838	1848	rBV	4696061	6623686	47.08%	5.702%
23	14.181	1876	1886	1896	rBV	5139027	7817548	55.57%	6.730%
24	14.487	1931	1938	1948	rVV	3564334	5368100	38.16%	4.621%
25	14.681	1965	1971	1984	rBV	348793	538140	3.83%	0.463%
26	14.904	2004	2009	2015	rVB6	18831	30667	0.22%	0.026%
27	15.475	2099	2106	2118	rBV	7343738	10507581	74.69%	9.046%
28	15.593	2118	2126	2140	rBV	2087025	2848878	20.25%	2.453%
29	15.716	2143	2147	2155	rVB2	38593	59991	0.43%	0.052%
30	16.704	2311	2315	2322	rBV3	6760	21511	0.15%	0.019%
31	17.228	2398	2404	2411	rBV	4504257	6411349	45.57%	5.520%
32	17.334	2415	2422	2433	rVV	8849475	12628367	89.76%	10.872%
33	17.422	2435	2437	2442	rVB4	15104	20426	0.15%	0.018%
34	17.610	2465	2469	2473	rBV2	15090	23877	0.17%	0.021%
35	18.122	2551	2556	2562	rBV2	91713	120946	0.86%	0.104%
36	19.139	2726	2729	2735	rVB2	103870	135679	0.96%	0.117%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018572.D
Acq On : 04 Dec 2023 20:00
Operator : MA/JU
Sample : 05441-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.210	2737	2741	2745	rBV	108553	141608	1.01%	0.122%
38	19.357	2762	2766	2772	rBV4	66766	80914	0.58%	0.070%
39	19.569	2796	2802	2813	rBV	10605548	14068927	100.00%	12.112%
40	21.316	3094	3099	3105	rBV	4372735	5692898	40.46%	4.901%
41	23.539	3469	3477	3485	rBV2	5495305	10634178	75.59%	9.155%
42	23.692	3496	3503	3515	rVB	2509803	5053487	35.92%	4.351%




Sum of corrected areas: 116156773

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018572.D
Acq On : 04 Dec 2023 20:00
Operator : MA/JU
Sample : 05441-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

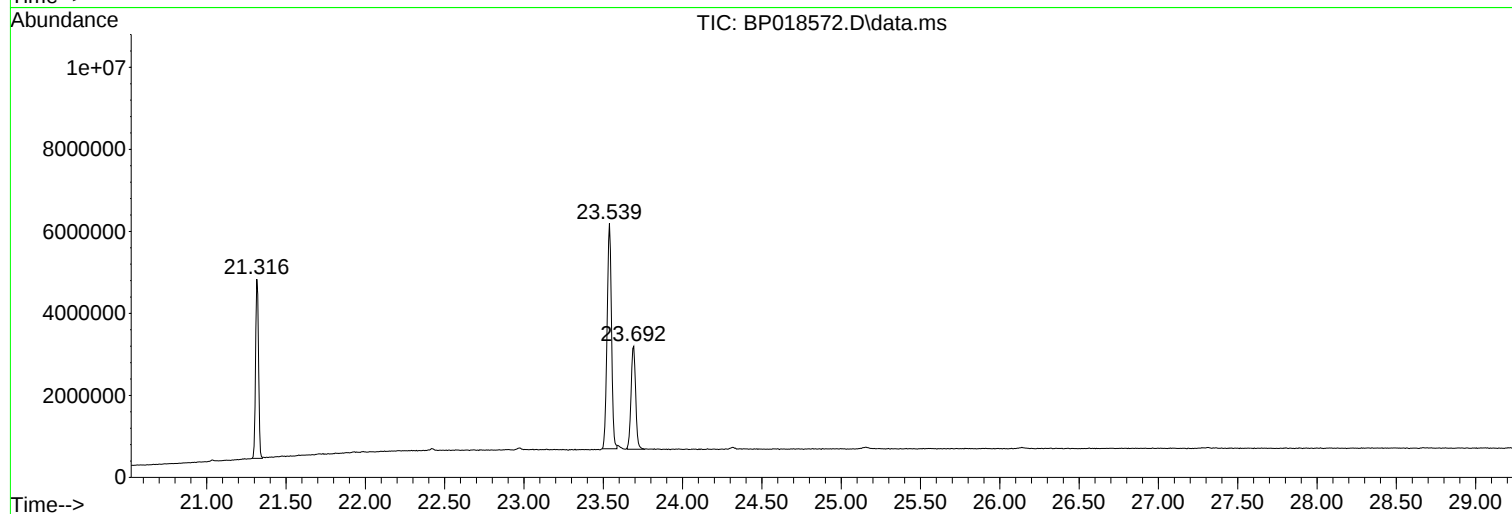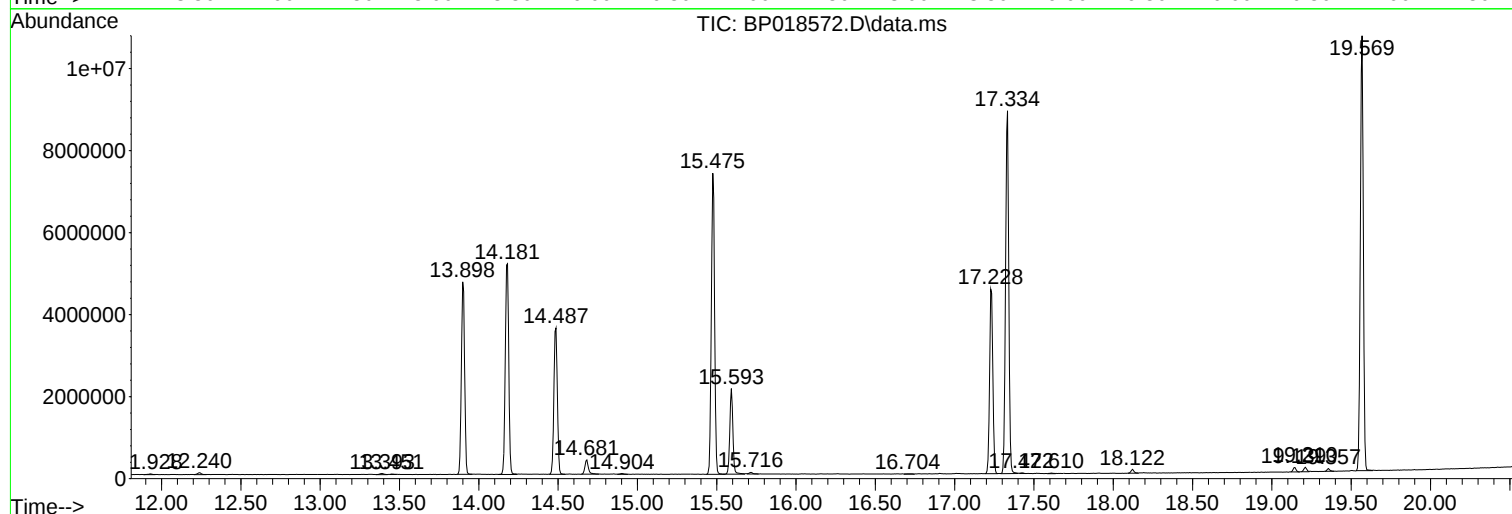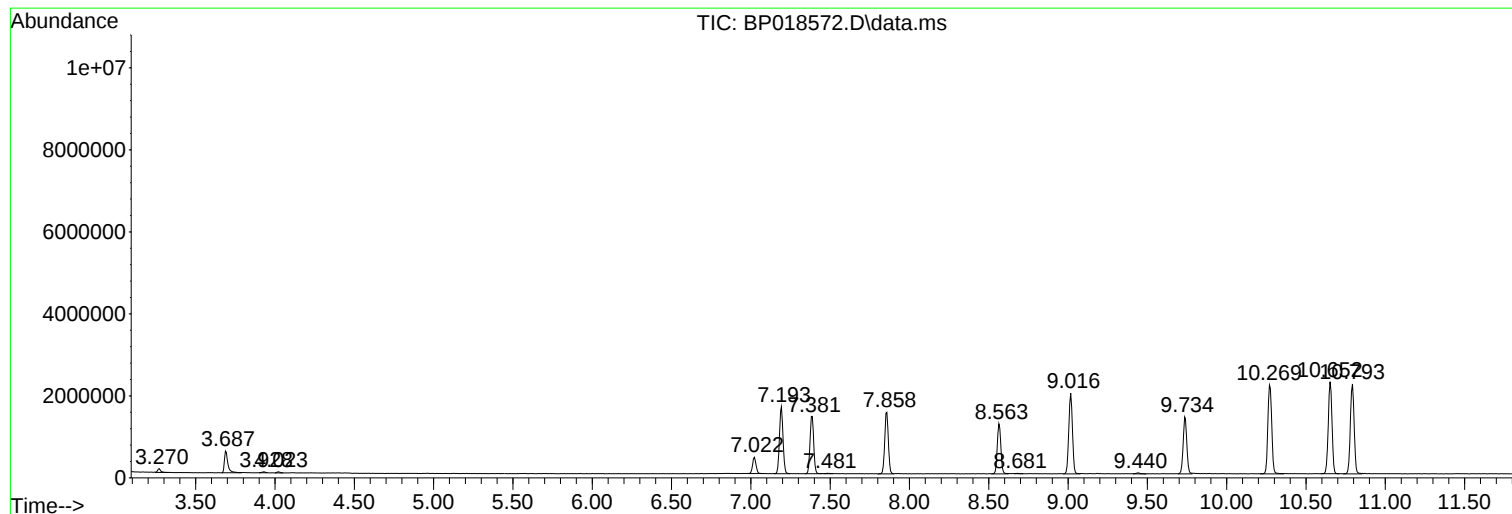

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018572.D
Acq On : 04 Dec 2023 20:00
Operator : MA/JU
Sample : 05441-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018572.D
Acq On : 04 Dec 2023 20:00
Operator : MA/JU
Sample : 05441-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
