

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018573.D
 Acq On : 04 Dec 2023 20:34
 Operator : MA/JU
 Sample : 05441-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018573.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	29	rBV	402142	554759	4.42%	0.519%
2	3.687	99	102	117	rBV	445948	692667	5.52%	0.649%
3	3.934	139	144	146	rVB2	17034	24579	0.20%	0.023%
4	4.017	156	158	165	rVB2	25907	39235	0.31%	0.037%
5	7.022	663	669	678	rVB	318711	489103	3.90%	0.458%
6	7.193	691	698	707	rBV	1501885	2331771	18.58%	2.183%
7	7.381	724	730	743	rBV	1226766	1949565	15.54%	1.826%
8	7.481	743	747	751	rVV5	8555	14627	0.12%	0.014%
9	7.858	802	811	818	rBV	1417929	2297958	18.32%	2.152%
10	7.928	818	823	826	rBV3	9696	14238	0.11%	0.013%
11	8.563	925	931	940	rBV	1054914	1613687	12.86%	1.511%
12	9.016	999	1008	1015	rBV	1741206	2820517	22.48%	2.641%
13	9.440	1076	1080	1086	rVB2	21142	38779	0.31%	0.036%
14	9.734	1121	1130	1142	rBV	1238569	1986494	15.83%	1.860%
15	10.269	1214	1221	1234	rBV	1980541	3269069	26.06%	3.061%
16	10.651	1277	1286	1297	rBV	2176005	3595994	28.66%	3.367%
17	10.793	1302	1310	1324	rVV	1900751	3179325	25.34%	2.977%
18	11.387	1405	1411	1416	rBV3	10395	21295	0.17%	0.020%
19	11.463	1419	1424	1431	rVV4	18740	33495	0.27%	0.031%
20	12.240	1549	1556	1563	rBV3	40859	69594	0.55%	0.065%
21	12.451	1590	1592	1599	rVB2	7578	14334	0.11%	0.013%
22	13.322	1737	1740	1743	rBV4	9509	13319	0.11%	0.012%
23	13.393	1746	1752	1756	rBV2	39777	66541	0.53%	0.062%
24	13.451	1758	1762	1766	rBV4	8382	12836	0.10%	0.012%
25	13.898	1832	1838	1851	rBV	4565852	6321605	50.38%	5.920%
26	14.175	1877	1885	1900	rBV2	4870970	7303854	58.21%	6.839%
27	14.481	1927	1937	1947	rBV	3489775	5250101	41.84%	4.916%
28	14.681	1965	1971	1982	rBV	262066	428215	3.41%	0.401%
29	14.898	2004	2008	2013	rBV6	15651	27286	0.22%	0.026%
30	15.475	2099	2106	2119	rBV	6841484	9852628	78.53%	9.226%
31	15.592	2119	2126	2138	rBV	1805301	2439981	19.45%	2.285%
32	15.710	2143	2146	2156	rVB3	36751	68794	0.55%	0.064%
33	16.263	2234	2240	2244	rBV9	10178	16837	0.13%	0.016%
34	16.904	2347	2349	2355	rVB3	12501	16501	0.13%	0.015%
35	17.016	2364	2368	2374	rVB4	11167	19674	0.16%	0.018%
36	17.228	2398	2404	2412	rBV	4222329	6174223	49.21%	5.781%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018573.D
Acq On : 04 Dec 2023 20:34
Operator : MA/JU
Sample : 05441-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	17.333	2415	2422	2434	rVV	7834563	11284558	89.94%	10.567%
38	18.122	2551	2556	2562	rBV2	122318	164562	1.31%	0.154%
39	19.145	2725	2730	2736	rBV2	96159	128668	1.03%	0.120%
40	19.210	2737	2741	2749	rVV	97589	137607	1.10%	0.129%
41	19.357	2762	2766	2774	rBV3	76521	102726	0.82%	0.096%
42	19.569	2796	2802	2810	rBV	9557822	12546666	100.00%	11.749%
43	21.316	3094	3099	3105	rBV	4567258	5443041	43.38%	5.097%
44	23.533	3469	3476	3483	rBV2	4697279	9172022	73.10%	8.589%
45	23.686	3496	3502	3514	rVB	2419197	4749423	37.85%	4.447%




Sum of corrected areas: 106792753

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018573.D
Acq On : 04 Dec 2023 20:34
Operator : MA/JU
Sample : 05441-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

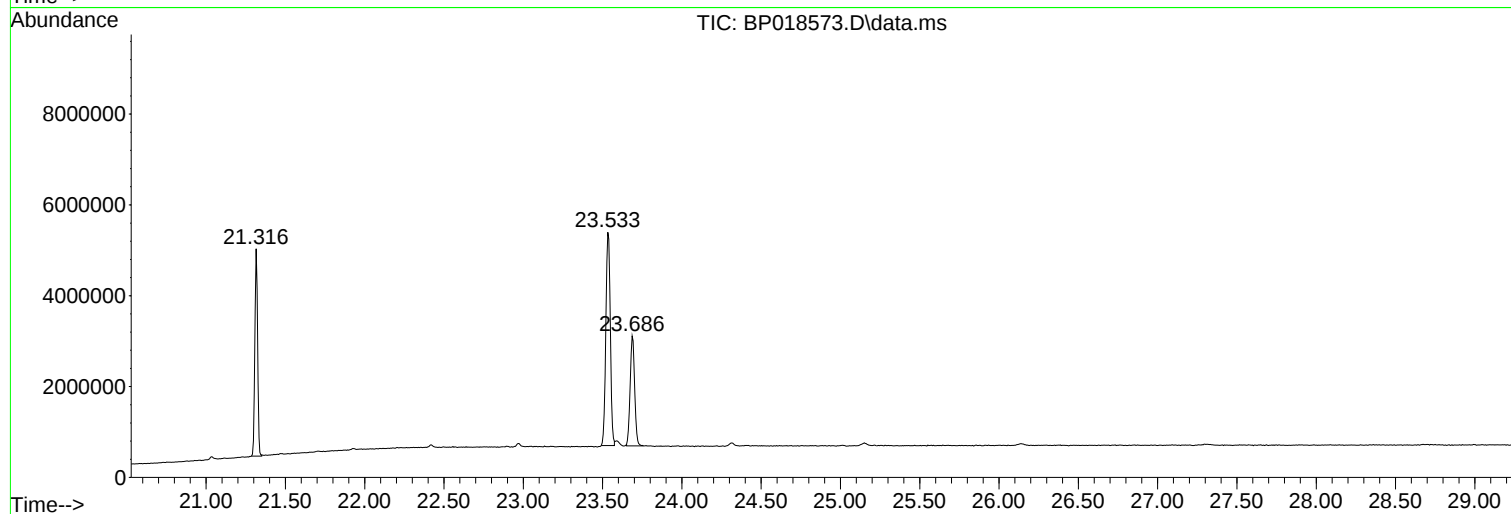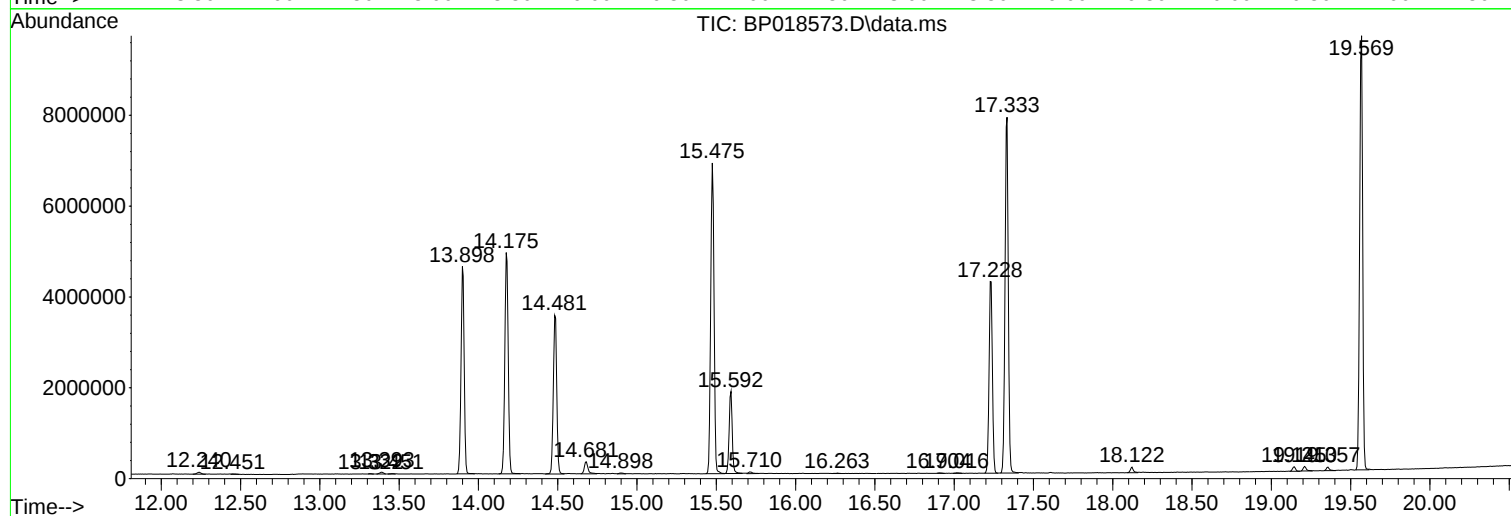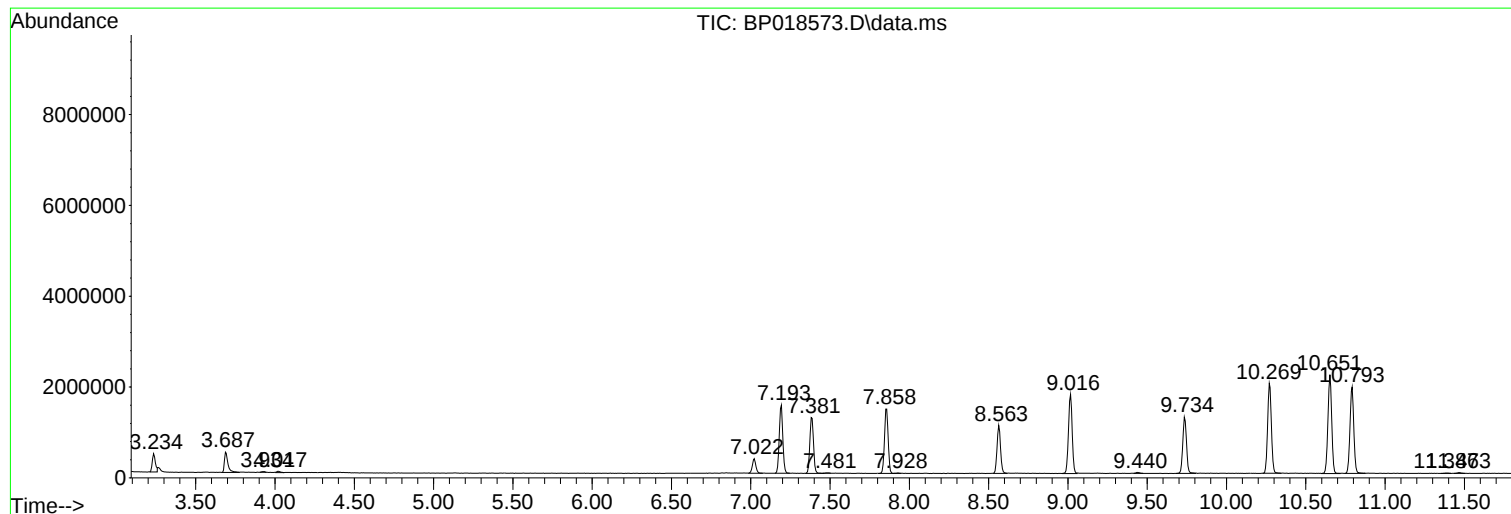

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018573.D
Acq On : 04 Dec 2023 20:34
Operator : MA/JU
Sample : 05441-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018573.D
Acq On : 04 Dec 2023 20:34
Operator : MA/JU
Sample : 05441-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc