

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018574.D
 Acq On : 04 Dec 2023 21:08
 Operator : MA/JU
 Sample : 05441-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018574.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	28	rBV	66751	87986	0.68%	0.081%
2	3.269	28	31	37	rVB2	79847	108373	0.83%	0.099%
3	3.687	99	102	116	rBV	514272	780840	6.00%	0.716%
4	3.928	139	143	149	rVB3	20791	31829	0.24%	0.029%
5	4.022	155	159	166	rVB	37122	54131	0.42%	0.050%
6	4.551	246	249	253	rVB3	11280	16453	0.13%	0.015%
7	7.022	663	669	677	rVV	337849	527040	4.05%	0.483%
8	7.092	677	681	686	rVB	10358	19470	0.15%	0.018%
9	7.192	691	698	708	rVV	1461726	2274853	17.49%	2.085%
10	7.387	724	731	742	rBV	1326644	2083266	16.02%	1.909%
11	7.857	803	811	819	rBV	1434317	2264349	17.41%	2.075%
12	8.563	924	931	941	rBV	1138021	1776734	13.66%	1.628%
13	9.016	1000	1008	1020	rBV	1858390	2922662	22.47%	2.679%
14	9.439	1074	1080	1088	rVB2	25414	37560	0.29%	0.034%
15	9.734	1123	1130	1143	rBV	1243455	2064745	15.88%	1.892%
16	10.269	1214	1221	1234	rBV	2121482	3431794	26.39%	3.145%
17	10.651	1278	1286	1293	rBV	2122872	3524148	27.10%	3.230%
18	10.792	1302	1310	1323	rBV	2082889	3448306	26.52%	3.161%
19	11.928	1495	1503	1509	rBV5	13282	29894	0.23%	0.027%
20	12.239	1549	1556	1561	rBV2	44198	76922	0.59%	0.071%
21	13.386	1746	1751	1756	rBV2	41987	68797	0.53%	0.063%
22	13.463	1760	1764	1768	rVB2	10108	15468	0.12%	0.014%
23	13.898	1830	1838	1845	rBV	4723801	6539100	50.28%	5.993%
24	14.174	1878	1885	1896	rBV	4973448	7545310	58.02%	6.916%
25	14.480	1931	1937	1947	rBV	3524732	5190455	39.91%	4.757%
26	14.680	1964	1971	1986	rBV	324760	523657	4.03%	0.480%
27	14.904	2005	2009	2015	rVB4	27148	50023	0.38%	0.046%
28	15.274	2066	2072	2073	rBV	8259	15607	0.12%	0.014%
29	15.474	2099	2106	2119	rBV	7295086	10062457	77.38%	9.223%
30	15.592	2119	2126	2140	rVV	1890701	2578795	19.83%	2.364%
31	15.716	2143	2147	2154	rVB2	38489	61549	0.47%	0.056%
32	16.916	2345	2351	2352	rBV3	9415	14655	0.11%	0.013%
33	17.015	2364	2368	2373	rVB4	8129	14719	0.11%	0.013%
34	17.227	2398	2404	2412	rBV	4304115	6131491	47.15%	5.620%
35	17.327	2415	2421	2433	rBV	8111933	11644839	89.54%	10.673%
36	18.121	2552	2556	2562	rVB2	66515	84548	0.65%	0.077%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018574.D
Acq On : 04 Dec 2023 21:08
Operator : MA/JU
Sample : 05441-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	18.198	2566	2569	2575	rVB6	13995	20114	0.15%	0.018%
38	19.139	2725	2729	2734	rBV	99049	127506	0.98%	0.117%
39	19.210	2737	2741	2749	rVV	92893	134273	1.03%	0.123%
40	19.351	2762	2765	2771	rBV3	46337	64964	0.50%	0.060%
41	19.568	2796	2802	2811	rBV	9758415	13004488	100.00%	11.919%
42	21.315	3094	3099	3107	rBV	4496258	5468509	42.05%	5.012%
43	23.533	3469	3476	3484	rBV2	4956760	9515509	73.17%	8.721%
44	23.686	3496	3502	3511	rVB	2396786	4666463	35.88%	4.277%




Sum of corrected areas: 109104651

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018574.D
Acq On : 04 Dec 2023 21:08
Operator : MA/JU
Sample : 05441-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

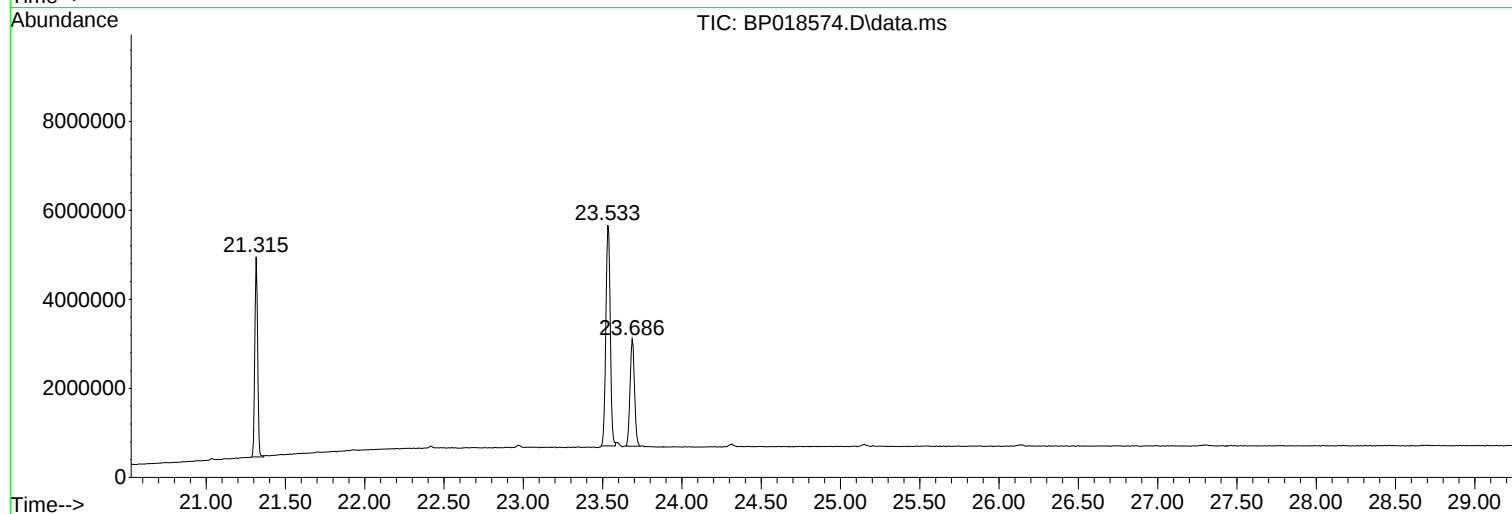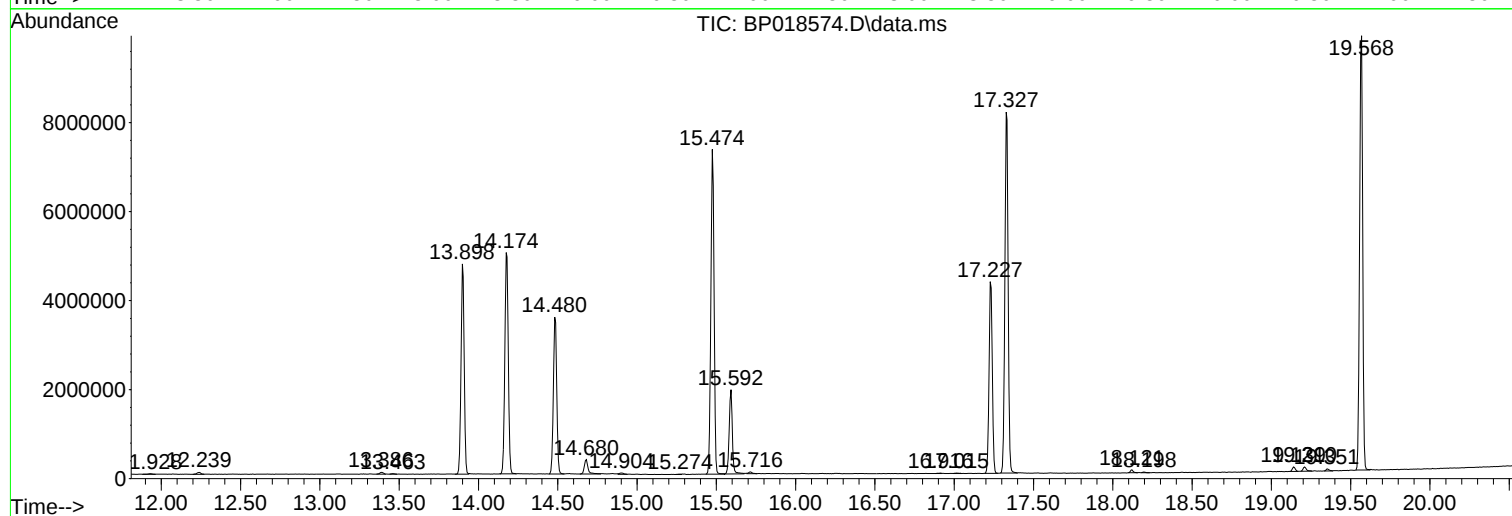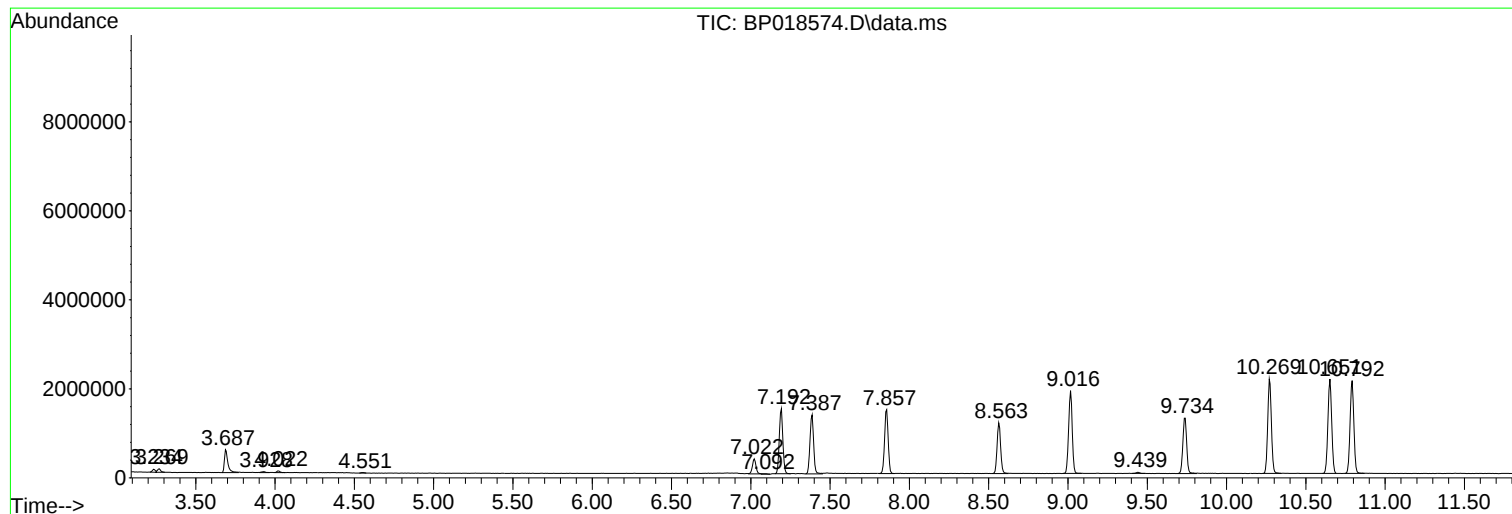

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018574.D
Acq On : 04 Dec 2023 21:08
Operator : MA/JU
Sample : 05441-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018574.D
Acq On : 04 Dec 2023 21:08
Operator : MA/JU
Sample : 05441-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
