

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018575.D
 Acq On : 04 Dec 2023 21:42
 Operator : MA/JU
 Sample : 05441-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018575.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	39	rVB	74324	95897	0.74%	0.104%
2	3.687	98	102	119	rBV	452977	706240	5.48%	0.765%
3	4.022	154	159	163	rBV	49057	69721	0.54%	0.075%
4	5.128	344	347	351	rBV3	11719	16051	0.12%	0.017%
5	7.022	663	669	678	rVB	321928	490933	3.81%	0.531%
6	7.193	691	698	712	rVB	1457893	2322740	18.03%	2.514%
7	7.381	724	730	739	rBV	1111151	1752553	13.60%	1.897%
8	7.481	745	747	752	rVB3	13766	18585	0.14%	0.020%
9	7.852	804	810	819	rVB	1151203	1874056	14.54%	2.029%
10	8.563	924	931	940	rBV	770681	1180692	9.16%	1.278%
11	9.016	997	1008	1016	rBV	1267233	2028627	15.74%	2.196%
12	9.434	1073	1079	1087	rVB2	16301	32223	0.25%	0.035%
13	9.734	1123	1130	1142	rBV	906025	1457552	11.31%	1.578%
14	10.269	1214	1221	1230	rBV	1496392	2395551	18.59%	2.593%
15	10.651	1277	1286	1294	rBV	1705957	2853633	22.15%	3.089%
16	10.793	1301	1310	1321	rBV	1409642	2382981	18.49%	2.580%
17	12.240	1549	1556	1562	rBV2	31887	50200	0.39%	0.054%
18	12.516	1598	1603	1609	rBV3	36572	59083	0.46%	0.064%
19	13.387	1745	1751	1758	rBV2	33431	57410	0.45%	0.062%
20	13.898	1830	1838	1849	rBV	3358129	4658621	36.16%	5.043%
21	14.175	1878	1885	1894	rBV2	3610344	5263060	40.85%	5.697%
22	14.481	1930	1937	1946	rBV	2806996	4261670	33.07%	4.613%
23	14.681	1964	1971	1985	rBV	224338	374201	2.90%	0.405%
24	14.904	2004	2009	2017	rVB	11416	21048	0.16%	0.023%
25	15.475	2099	2106	2116	rBV	5129043	7249615	56.26%	7.848%
26	15.592	2120	2126	2139	rVV	1432138	1936170	15.03%	2.096%
27	15.716	2142	2147	2152	rVB2	24643	37865	0.29%	0.041%
28	16.904	2346	2349	2354	rBV4	8776	14189	0.11%	0.015%
29	17.016	2366	2368	2372	rVB4	11273	13029	0.10%	0.014%
30	17.233	2398	2405	2411	rBV	3782435	5286175	41.03%	5.722%
31	17.328	2415	2421	2433	rVV2	5927082	8664537	67.24%	9.380%
32	18.122	2551	2556	2560	rBV	82056	108872	0.84%	0.118%
33	19.145	2725	2730	2735	rBV	86812	117609	0.91%	0.127%
34	19.210	2737	2741	2745	rVV	88761	111956	0.87%	0.121%
35	19.357	2762	2766	2769	rBV3	54774	73051	0.57%	0.079%
36	19.392	2771	2772	2776	rBV2	21923	37716	0.29%	0.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018575.D
Acq On : 04 Dec 2023 21:42
Operator : MA/JU
Sample : 05441-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.569	2796	2802	2815	rBV	9681853	12885057	100.00%	13.948%
38	21.316	3094	3099	3105	rBV	5138469	6285369	48.78%	6.804%
39	23.539	3469	3477	3485	rBV2	5014584	9660155	74.97%	10.457%
40	23.692	3496	3503	3515	rVB	2801807	5471590	42.46%	5.923%




Sum of corrected areas: 92376283

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018575.D
Acq On : 04 Dec 2023 21:42
Operator : MA/JU
Sample : 05441-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

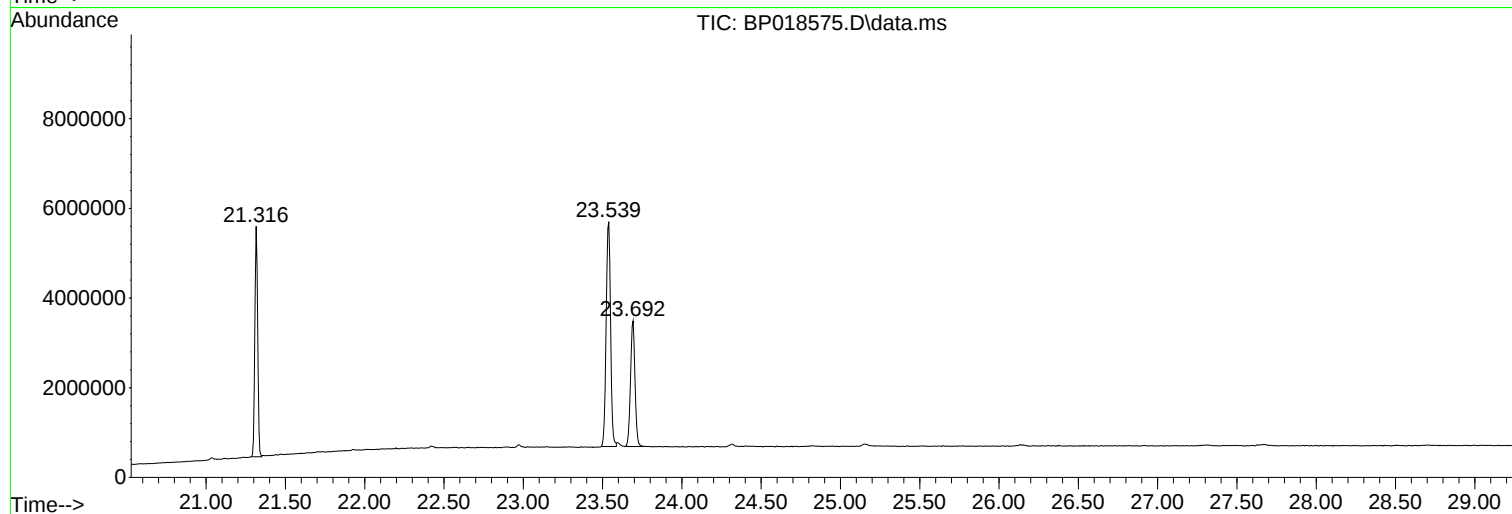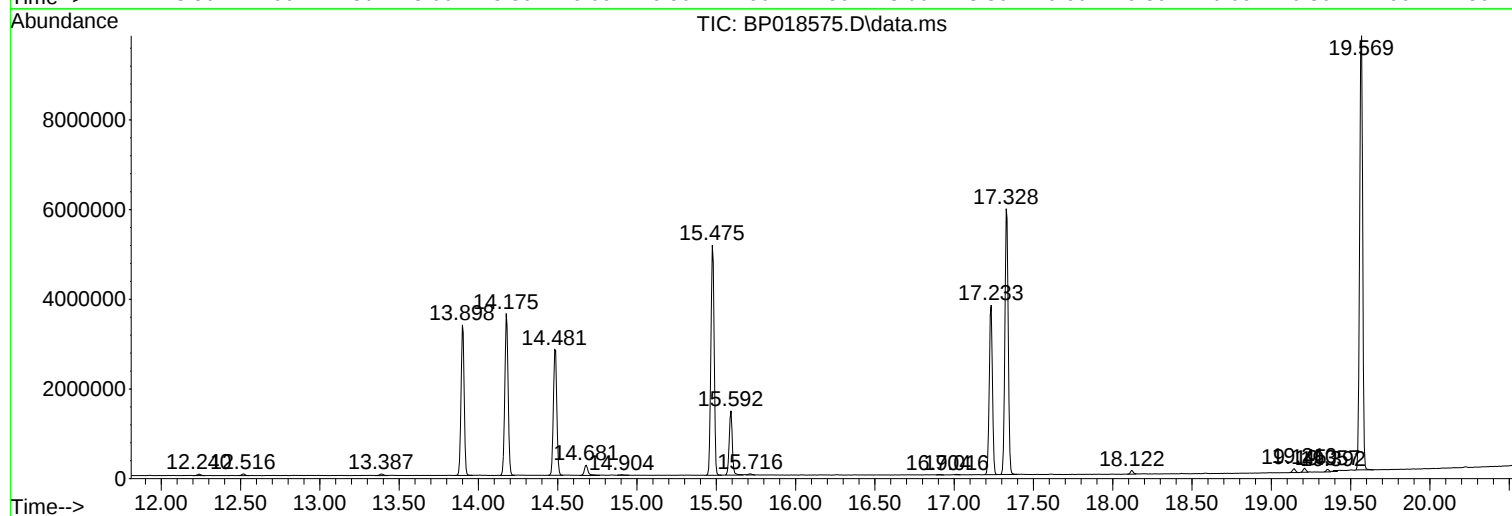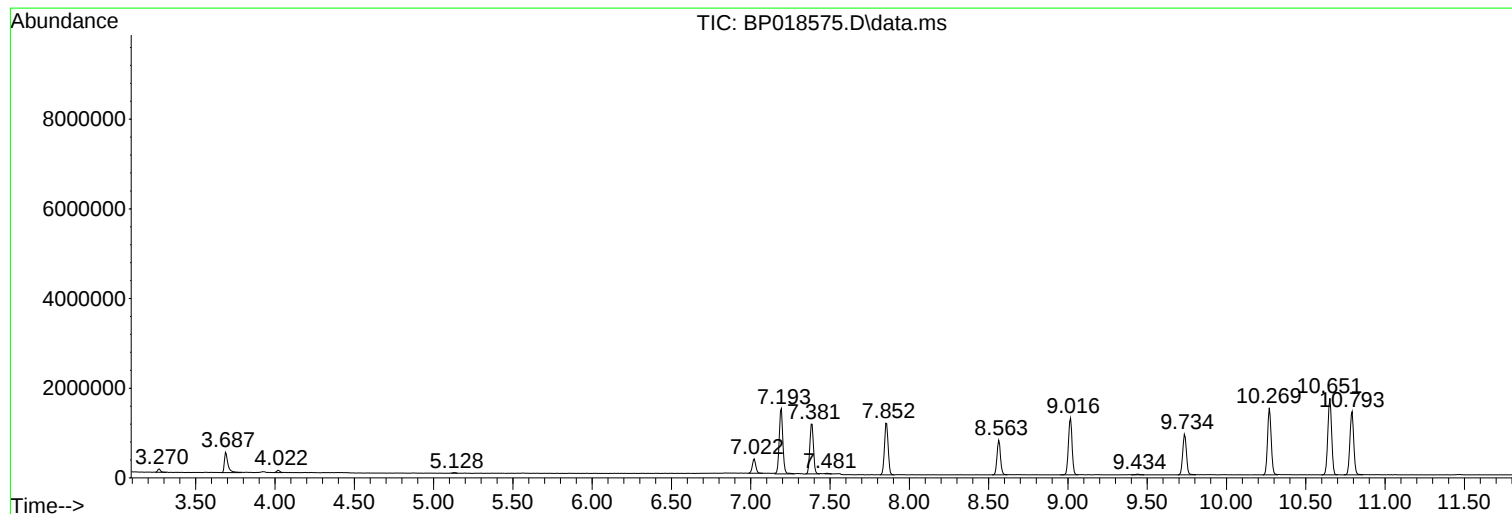

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018575.D
Acq On : 04 Dec 2023 21:42
Operator : MA/JU
Sample : 05441-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018575.D
Acq On : 04 Dec 2023 21:42
Operator : MA/JU
Sample : 05441-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
