

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018576.D
 Acq On : 04 Dec 2023 22:16
 Operator : MA/JU
 Sample : 05441-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018576.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	37	rVB	85941	107470	0.98%	0.103%
2	3.558	77	80	86	rVB2	17395	25227	0.23%	0.024%
3	3.687	98	102	112	rBV	517899	739394	6.74%	0.708%
4	3.928	139	143	147	rVB2	21085	30297	0.28%	0.029%
5	4.017	155	158	164	rVB2	26063	39719	0.36%	0.038%
6	5.558	412	420	422	rBV4	6955	11013	0.10%	0.011%
7	7.022	662	669	678	rVB	416097	640798	5.84%	0.613%
8	7.193	691	698	709	rVB	1649772	2590599	23.62%	2.479%
9	7.387	721	731	738	rBV	1415922	2282966	20.82%	2.185%
10	7.487	743	748	750	rBV2	10344	14236	0.13%	0.014%
11	7.858	803	811	819	rVB	1407046	2241532	20.44%	2.145%
12	8.563	924	931	940	rBV	1260253	1938626	17.68%	1.855%
13	9.016	1000	1008	1015	rBV	1913309	3062375	27.92%	2.930%
14	9.440	1073	1080	1087	rVB2	25842	46133	0.42%	0.044%
15	9.734	1122	1130	1144	rBV	1353025	2204273	20.10%	2.109%
16	10.269	1212	1221	1235	rBV	2214149	3562684	32.48%	3.409%
17	10.651	1278	1286	1293	rBV	2055497	3426509	31.24%	3.279%
18	10.787	1302	1309	1318	rBV	2058527	3494702	31.87%	3.344%
19	11.928	1500	1503	1507	rVB3	15738	22459	0.20%	0.021%
20	12.234	1548	1555	1562	rVB3	47406	89170	0.81%	0.085%
21	13.387	1747	1751	1756	rBV2	28936	44115	0.40%	0.042%
22	13.457	1759	1763	1766	rBV4	9160	11967	0.11%	0.011%
23	13.898	1832	1838	1849	rBV	4423806	6276921	57.23%	6.007%
24	14.175	1875	1885	1898	rBV	5132023	7436166	67.80%	7.116%
25	14.481	1930	1937	1948	rBV	3139941	4770343	43.50%	4.565%
26	14.681	1965	1971	1983	rBV	292247	493000	4.50%	0.472%
27	14.840	1995	1998	2003	rVB4	7460	12150	0.11%	0.012%
28	14.898	2003	2008	2014	rBV6	15647	28116	0.26%	0.027%
29	15.475	2099	2106	2113	rBV	6959339	9612404	87.65%	9.198%
30	15.592	2118	2126	2138	rBV	1667536	2268590	20.69%	2.171%
31	15.716	2143	2147	2152	rVV3	35861	62797	0.57%	0.060%
32	16.263	2237	2240	2245	rVB7	9470	15447	0.14%	0.015%
33	16.316	2245	2249	2254	rBV5	8380	15385	0.14%	0.015%
34	16.375	2257	2259	2264	rVV3	9993	12912	0.12%	0.012%
35	16.434	2264	2269	2274	rVV7	7077	14639	0.13%	0.014%
36	16.710	2312	2316	2320	rBV5	8244	15137	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018576.D
 Acq On : 04 Dec 2023 22:16
 Operator : MA/JU
 Sample : 05441-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QH1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	16.910	2346	2350	2353	rVB2	9476	15749	0.14%	0.015%
38	17.228	2398	2404	2414	rVB	3568190	5198711	47.40%	4.975%
39	17.328	2414	2421	2436	rBV	7269033	10450921	95.29%	10.001%
40	17.710	2482	2486	2491	rBV4	14377	19116	0.17%	0.018%
41	18.122	2551	2556	2562	rBV3	63630	91769	0.84%	0.088%
42	18.322	2586	2590	2596	rBV2	58285	74814	0.68%	0.072%
43	19.139	2725	2729	2735	rBV3	83066	116359	1.06%	0.111%
44	19.210	2737	2741	2745	rVV	78042	100509	0.92%	0.096%
45	19.357	2762	2766	2772	rBV7	31716	48046	0.44%	0.046%
46	19.569	2796	2802	2809	rBV	7954074	10967198	100.00%	10.495%
47	21.316	3094	3099	3106	rBV	3643273	4478228	40.83%	4.285%
48	23.533	3469	3476	3493	rBV2	5443412	10443852	95.23%	9.994%
49	23.686	3496	3502	3512	rVB	2436413	4835709	44.09%	4.627%




Sum of corrected areas: 104501252

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018576.D
Acq On : 04 Dec 2023 22:16
Operator : MA/JU
Sample : 05441-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

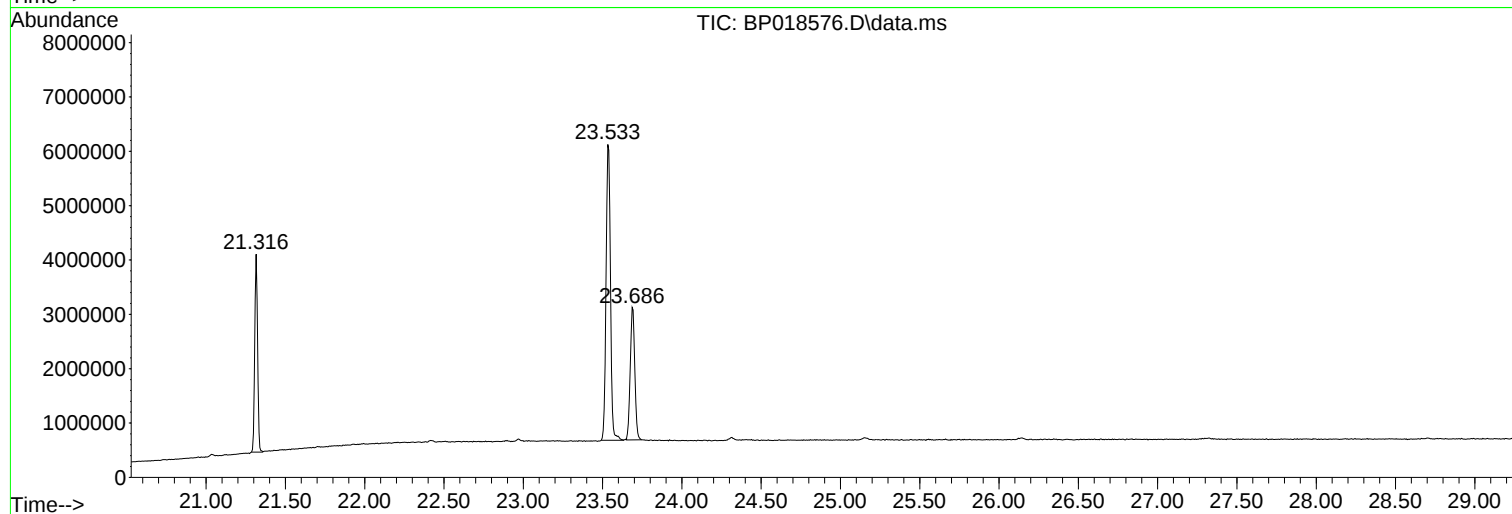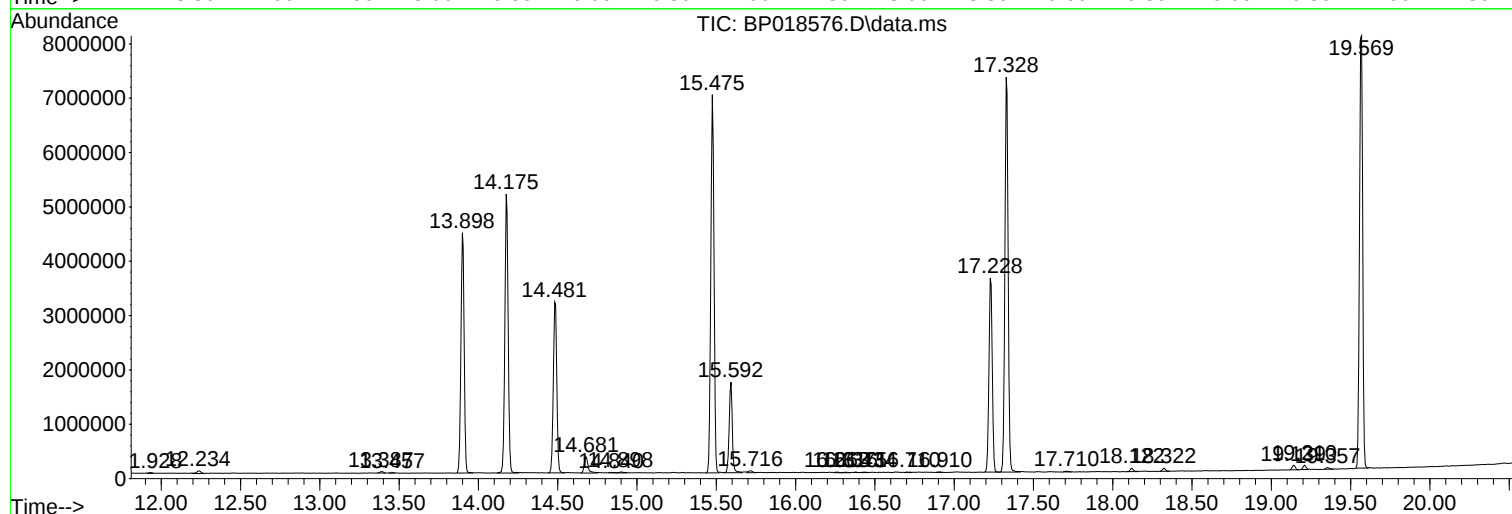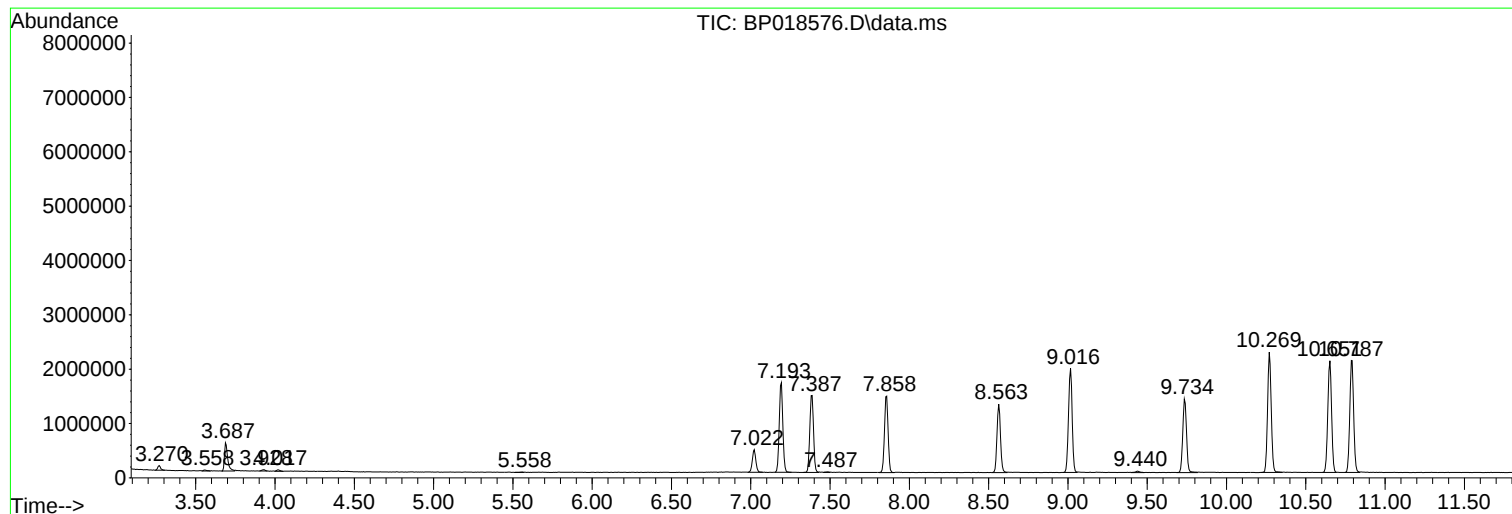

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018576.D
Acq On : 04 Dec 2023 22:16
Operator : MA/JU
Sample : 05441-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018576.D
Acq On : 04 Dec 2023 22:16
Operator : MA/JU
Sample : 05441-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc