

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018579.D
 Acq On : 04 Dec 2023 23:58
 Operator : MA/JU
 Sample : 05439-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018579.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	41	rVB	89912	124708	0.97%	0.118%
2	3.687	99	102	114	rBV	373624	564499	4.38%	0.534%
3	4.022	155	159	162	rVB2	22762	30231	0.23%	0.029%
4	7.022	656	669	678	rVB	261199	424701	3.30%	0.401%
5	7.193	691	698	706	rVB	1136781	1759167	13.65%	1.663%
6	7.381	721	730	738	rBV	1009656	1584265	12.29%	1.497%
7	7.463	740	744	752	rVB	43894	77573	0.60%	0.073%
8	7.640	769	774	775	rBV	19506	29237	0.23%	0.028%
9	7.852	802	810	818	rBV	1345572	2161131	16.77%	2.042%
10	8.563	924	931	939	rBV	1093309	1661702	12.90%	1.570%
11	9.016	1000	1008	1017	rBV	1714476	2791949	21.67%	2.639%
12	9.734	1123	1130	1140	rBV	1217980	1977970	15.35%	1.869%
13	10.269	1214	1221	1235	rBV	2054068	3351738	26.01%	3.168%
14	10.651	1278	1286	1296	rVB	1992500	3323613	25.79%	3.141%
15	10.793	1302	1310	1318	rBV	1758721	2972666	23.07%	2.809%
16	11.934	1500	1504	1509	rVB5	8885	14015	0.11%	0.013%
17	12.240	1550	1556	1562	rBV2	41233	71106	0.55%	0.067%
18	13.110	1700	1704	1708	rBV3	9745	16908	0.13%	0.016%
19	13.392	1745	1752	1759	rBV	622002	945530	7.34%	0.894%
20	13.710	1801	1806	1811	rBV6	10132	21113	0.16%	0.020%
21	13.898	1832	1838	1845	rBV	4465182	6278001	48.72%	5.933%
22	14.175	1879	1885	1897	rBV	5016566	7138439	55.40%	6.747%
23	14.481	1931	1937	1945	rVB	3252539	4844093	37.59%	4.578%
24	14.681	1965	1971	1981	rBV	296584	473244	3.67%	0.447%
25	14.839	1993	1998	2000	rBV6	12366	18051	0.14%	0.017%
26	15.475	2099	2106	2114	rBV	6990752	9781455	75.91%	9.244%
27	15.592	2119	2126	2140	rVV	1884283	2563968	19.90%	2.423%
28	15.716	2143	2147	2157	rVB3	38273	73545	0.57%	0.070%
29	16.269	2236	2241	2242	rBV4	11212	18644	0.14%	0.018%
30	16.492	2275	2279	2283	rVB	20780	29029	0.23%	0.027%
31	16.598	2294	2297	2300	rBV2	17218	19853	0.15%	0.019%
32	17.228	2398	2404	2411	rBV	4149133	5845221	45.36%	5.524%
33	17.328	2415	2421	2433	rVV	7765015	11127572	86.36%	10.517%
34	17.910	2516	2520	2523	rVB2	24979	30513	0.24%	0.029%
35	18.122	2551	2556	2564	rBV	251948	351528	2.73%	0.332%
36	18.580	2632	2634	2641	rVB4	16215	22064	0.17%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018579.D
Acq On : 04 Dec 2023 23:58
Operator : MA/JU
Sample : 05439-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.039	2709	2712	2716	rVB2	122520	128152	0.99%	0.121%
38	19.139	2725	2729	2736	rBV2	103222	154710	1.20%	0.146%
39	19.210	2737	2741	2745	rBV	111821	147622	1.15%	0.140%
40	19.351	2762	2765	2772	rVB2	115722	141824	1.10%	0.134%
41	19.563	2795	2801	2815	rBV	9528763	12885475	100.00%	12.178%
42	19.792	2837	2840	2845	rVB	65023	78995	0.61%	0.075%
43	21.033	3049	3051	3059	rVB3	86963	111441	0.86%	0.105%
44	21.316	3094	3099	3105	rBV	4284480	5228990	40.58%	4.942%
45	23.533	3469	3476	3484	rBV2	4925529	9704455	75.31%	9.172%
46	23.686	3496	3502	3518	rVB	2417125	4708777	36.54%	4.450%




Sum of corrected areas: 105809483

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018579.D
Acq On : 04 Dec 2023 23:58
Operator : MA/JU
Sample : 05439-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

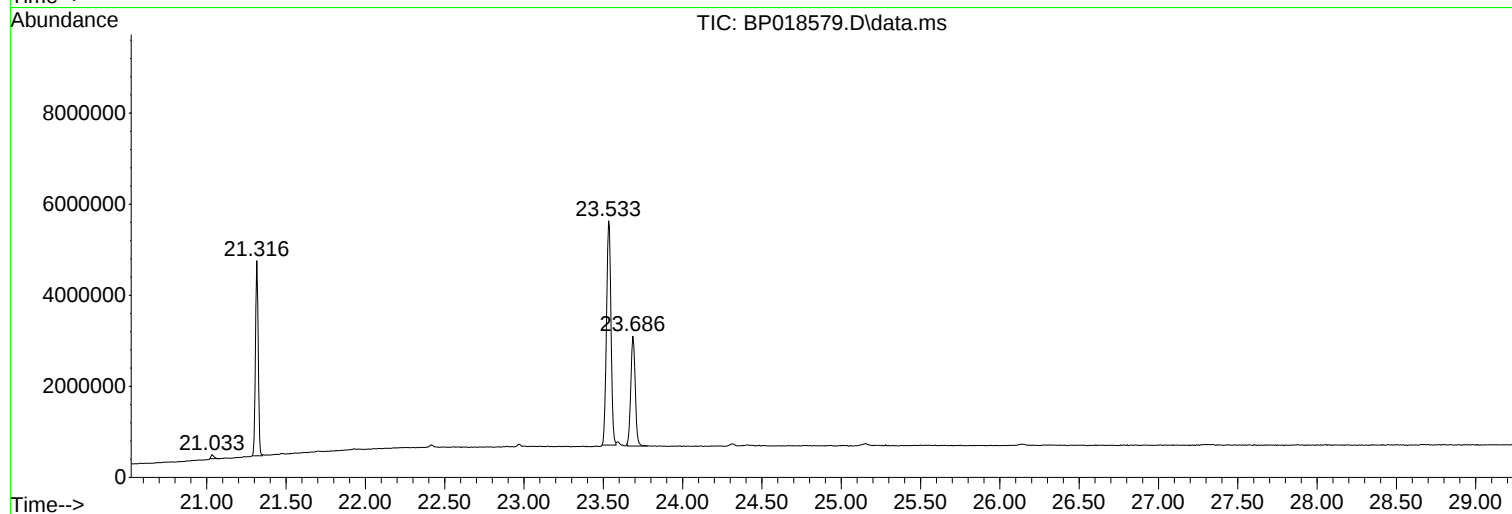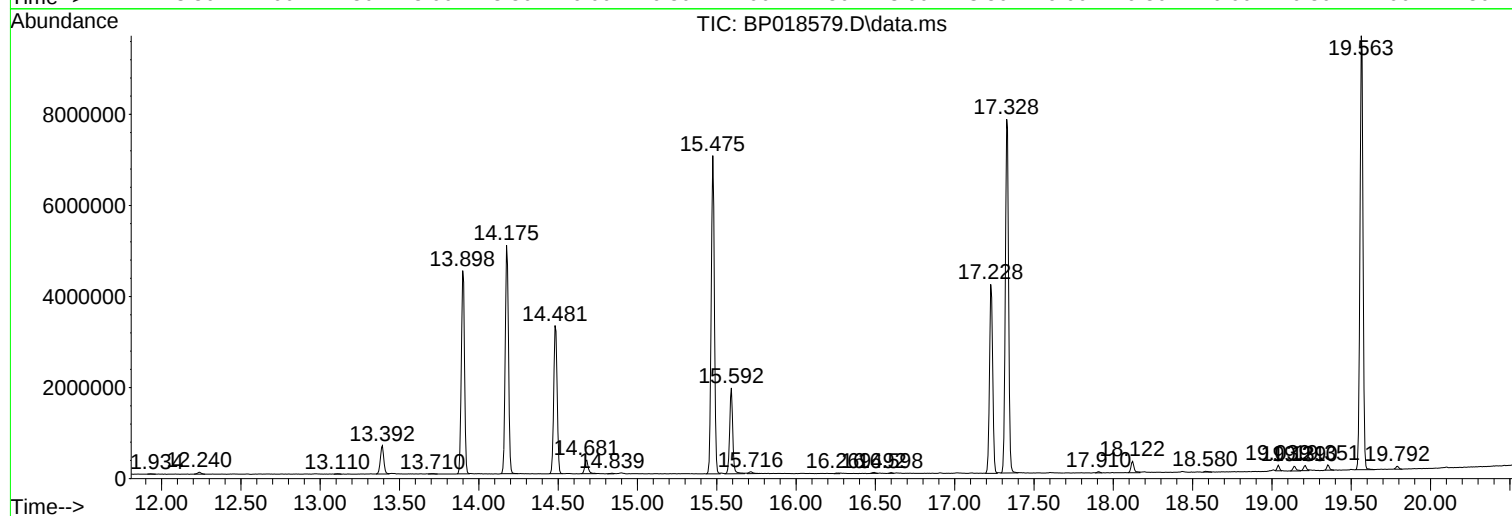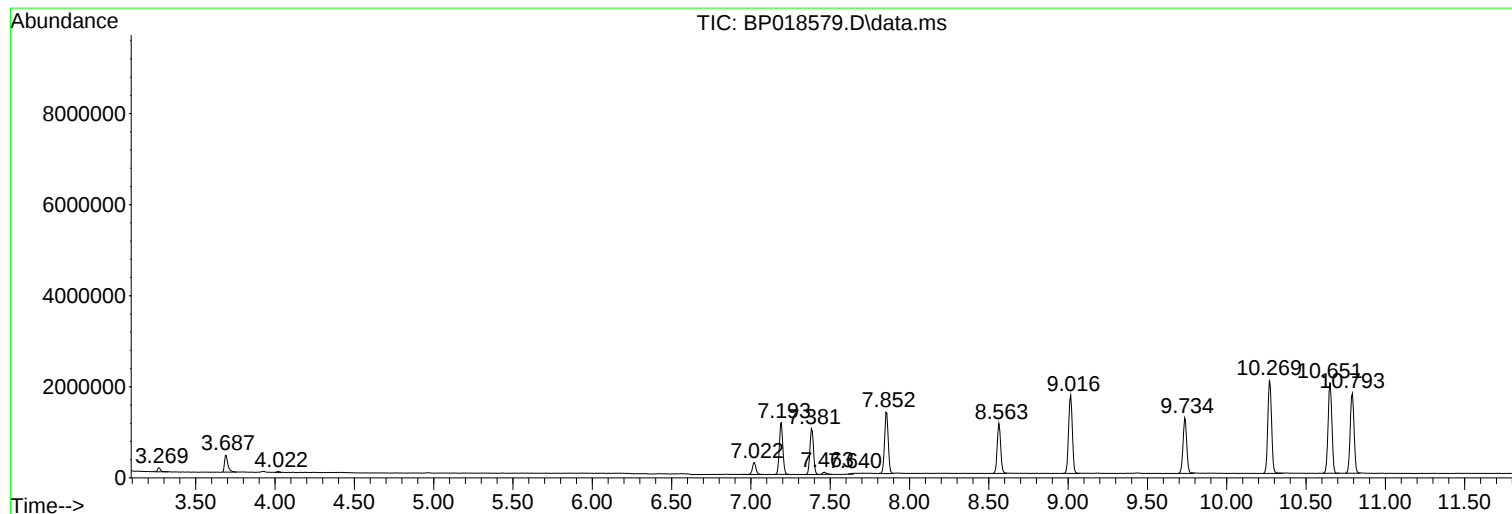

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018579.D
Acq On : 04 Dec 2023 23:58
Operator : MA/JU
Sample : 05439-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2,4,7,9-Tetramethyl-5-decyn... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.392	3.90 ng/ul	945530	Acenaphthene-d10	14.481

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2,4,7,9-Tetramethyl-5-decyn-4,7-...	226	C14H26O2	000126-86-3	91		
2	2,4,7,9-Tetramethyl-5-decyn-4,7-...	226	C14H26O2	000126-86-3	90		
3	Acetaminophen	151	C8H9NO2	000103-90-2	59		
4	Metacetamol	151	C8H9NO2	000621-42-1	59		
5	N-(4-tert-Butoxyphenyl)acetamide...	249	C14H19NO3	1000504-17-4	59		

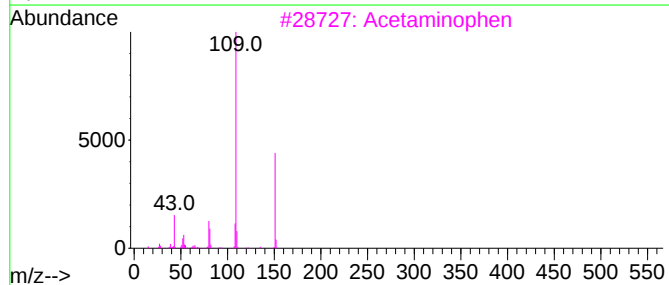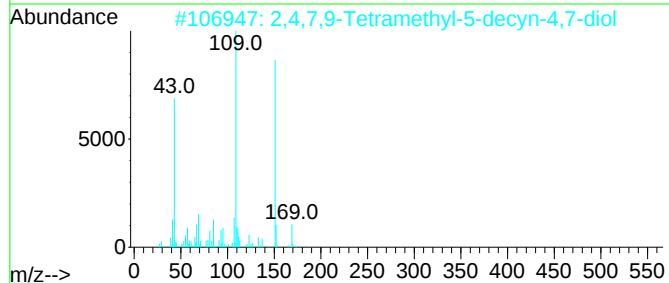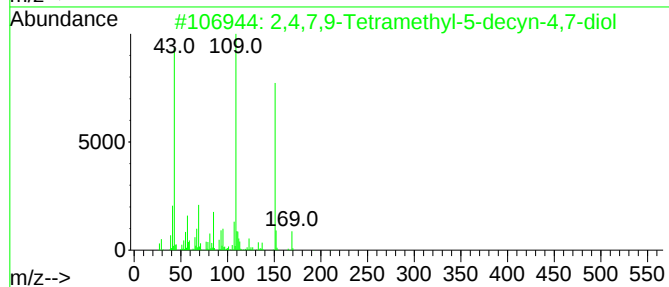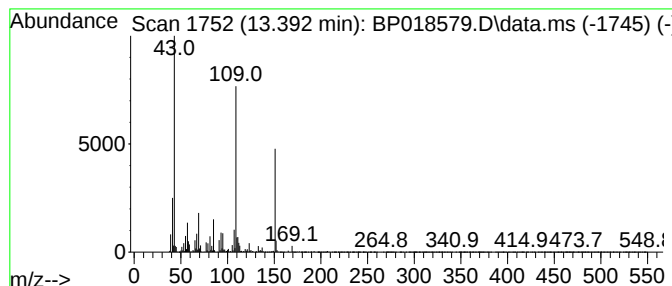

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018579.D
Acq On : 04 Dec 2023 23:58
Operator : MA/JU
Sample : 05439-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2,4,7,9-Tetrame...	13.392	3.9	ng/u1	945530	3	14.481	4844090	20.0