

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018580.D
 Acq On : 05 Dec 2023 00:32
 Operator : MA/JU
 Sample : 05439-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AFO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018580.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	37	rVB	87620	106166	0.99%	0.105%
2	3.687	99	102	114	rBV	448990	688755	6.43%	0.681%
3	3.928	141	143	148	rVB3	21317	23089	0.22%	0.023%
4	4.016	155	158	165	rVB2	25312	42119	0.39%	0.042%
5	7.022	663	669	680	rVB	370279	592096	5.52%	0.585%
6	7.193	691	698	709	rVB	1452948	2323517	21.68%	2.298%
7	7.381	724	730	740	rBV	1330445	2073335	19.34%	2.050%
8	7.463	740	744	756	rVB2	44611	89838	0.84%	0.089%
9	7.851	804	810	818	rBV	1486117	2375457	22.16%	2.349%
10	8.392	898	902	905	rVB2	10958	18053	0.17%	0.018%
11	8.451	905	912	913	rBV	13091	19353	0.18%	0.019%
12	8.563	925	931	938	rBV	1120840	1734768	16.18%	1.715%
13	9.016	1000	1008	1018	rBV	1735339	2783766	25.97%	2.753%
14	9.439	1076	1080	1086	rVB3	11929	23908	0.22%	0.024%
15	9.734	1123	1130	1139	rBV	1245504	2014614	18.79%	1.992%
16	10.269	1214	1221	1232	rBV	2094787	3372810	31.47%	3.335%
17	10.651	1278	1286	1294	rBV	2214985	3632308	33.89%	3.592%
18	10.792	1302	1310	1320	rBV	1809769	3043162	28.39%	3.009%
19	11.922	1499	1502	1510	rVB3	11567	23739	0.22%	0.023%
20	12.239	1550	1556	1562	rVB2	41186	67566	0.63%	0.067%
21	13.110	1700	1704	1709	rVB2	18856	30591	0.29%	0.030%
22	13.386	1745	1751	1759	rBV	170829	277346	2.59%	0.274%
23	13.457	1759	1763	1767	rVB3	8083	14601	0.14%	0.014%
24	13.898	1831	1838	1847	rBV	4396356	6222887	58.05%	6.153%
25	14.175	1878	1885	1893	rBV	4823461	7070882	65.96%	6.992%
26	14.480	1930	1937	1945	rBV	3562946	5206089	48.57%	5.148%
27	14.680	1965	1971	1981	rBV2	322201	521827	4.87%	0.516%
28	14.898	2004	2008	2014	rVB3	18132	32687	0.30%	0.032%
29	15.474	2099	2106	2114	rBV	6918943	9595955	89.52%	9.489%
30	15.592	2120	2126	2136	rBV	1802537	2488431	23.21%	2.461%
31	15.710	2143	2146	2154	rVB2	32253	53238	0.50%	0.053%
32	16.257	2236	2239	2243	rVB4	11673	14126	0.13%	0.014%
33	17.227	2398	2404	2414	rBV	4226432	6047831	56.42%	5.980%
34	17.327	2415	2421	2433	rBV	7553785	10719166	100.00%	10.600%
35	18.121	2551	2556	2560	rBV2	134874	176492	1.65%	0.175%
36	19.039	2709	2712	2716	rVB3	48431	53591	0.50%	0.053%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018580.D
Acq On : 05 Dec 2023 00:32
Operator : MA/JU
Sample : 05439-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.139	2725	2729	2736	rBV	94196	137517	1.28%	0.136%
38	19.210	2737	2741	2745	rVV	99580	129339	1.21%	0.128%
39	19.351	2762	2765	2770	rBV4	66081	81380	0.76%	0.080%
40	19.562	2796	2801	2810	rVB	7280397	9639747	89.93%	9.532%
41	21.315	3094	3099	3110	rBV	3450009	4405262	41.10%	4.356%
42	23.533	3469	3476	3493	rVB2	4385768	8645394	80.65%	8.549%
43	23.686	3496	3502	3512	rVB	2322594	4515020	42.12%	4.465%




Sum of corrected areas: 101127818

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018580.D
Acq On : 05 Dec 2023 00:32
Operator : MA/JU
Sample : 05439-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

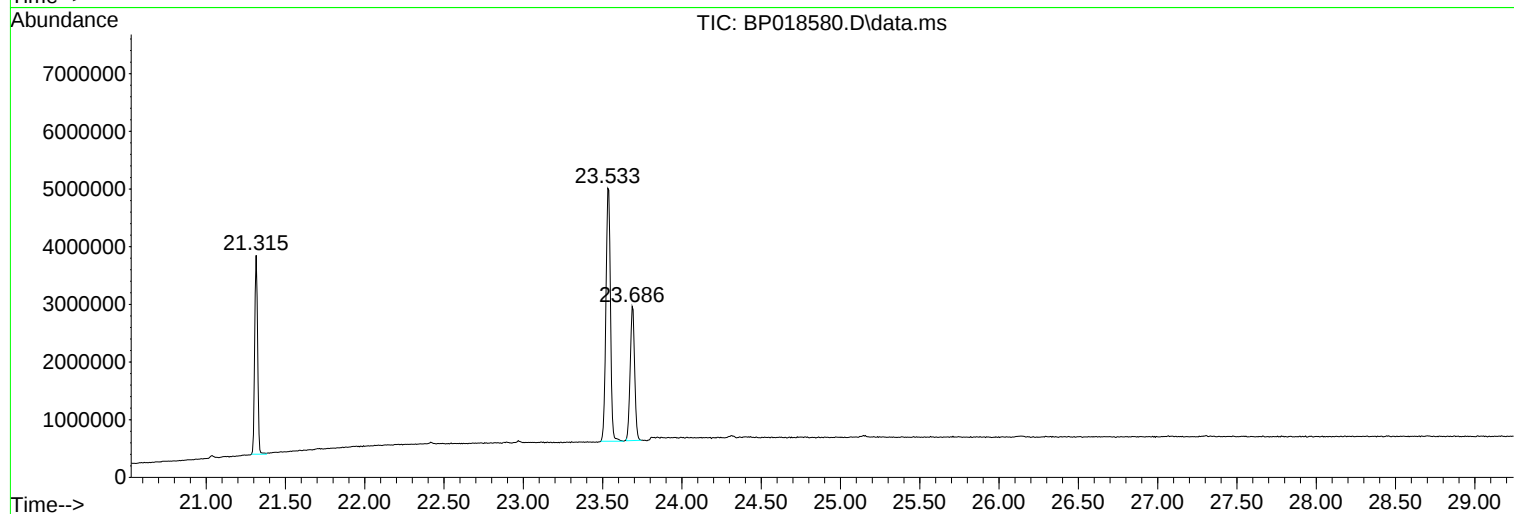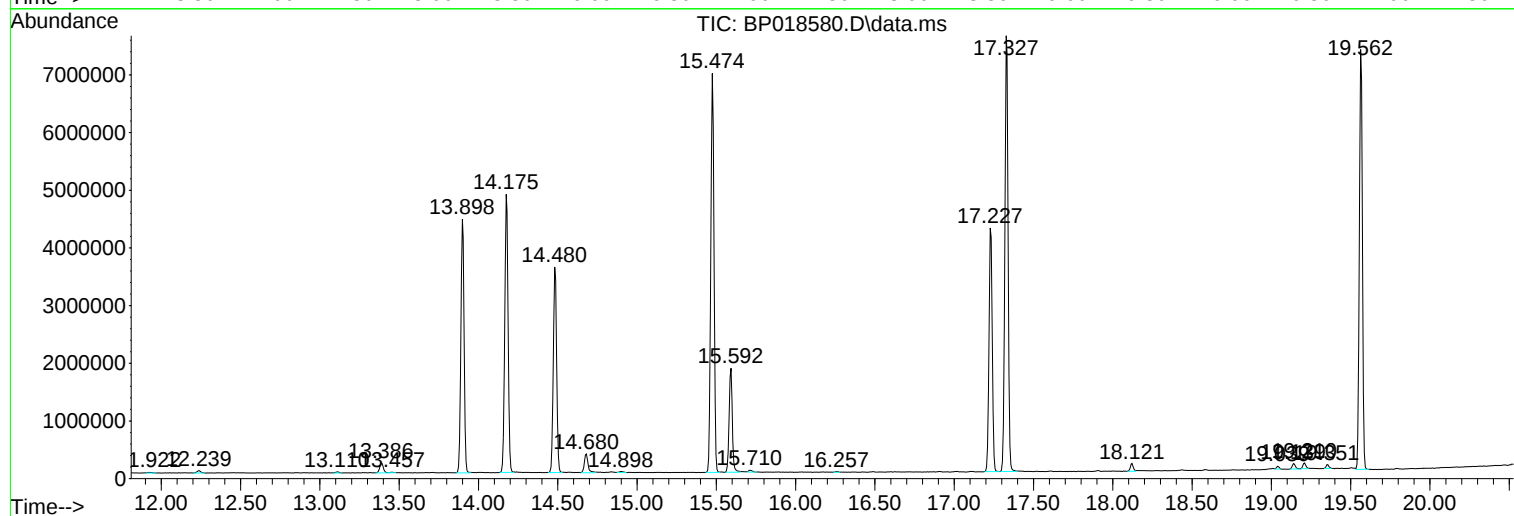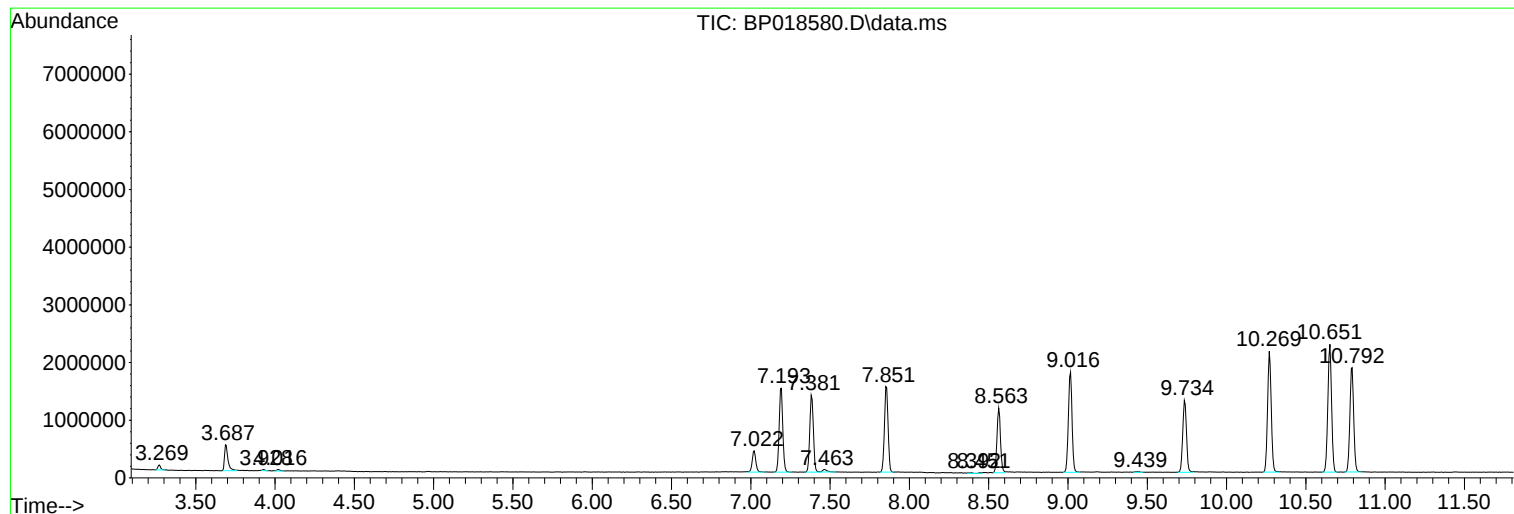

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018580.D
Acq On : 05 Dec 2023 00:32
Operator : MA/JU
Sample : 05439-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018580.D
Acq On : 05 Dec 2023 00:32
Operator : MA/JU
Sample : 05439-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc