

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018581.D
 Acq On : 05 Dec 2023 01:06
 Operator : MA/JU
 Sample : 05452-02DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AJODL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018581.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.693	98	103	116	rBV2	85573	158393	1.95%	0.282%
2	4.016	154	158	162	rBV2	21414	30068	0.37%	0.054%
3	7.022	661	669	673	rBV2	35203	58383	0.72%	0.104%
4	7.187	690	697	704	rBV	214518	344135	4.24%	0.613%
5	7.381	725	730	740	rBV2	114586	181161	2.23%	0.323%
6	7.851	801	810	818	rBV	1254922	1985660	24.49%	3.538%
7	8.563	925	931	939	rVB	125554	202177	2.49%	0.360%
8	9.010	1002	1007	1019	rVB	215665	373922	4.61%	0.666%
9	9.734	1123	1130	1138	rBV	87870	149655	1.85%	0.267%
10	10.063	1181	1186	1194	rBV6	16701	39634	0.49%	0.071%
11	10.269	1214	1221	1229	rVV	182245	307475	3.79%	0.548%
12	10.651	1278	1286	1293	rBV	1811715	3034559	37.43%	5.406%
13	10.792	1301	1310	1315	rBV	266135	463799	5.72%	0.826%
14	10.951	1332	1337	1343	rVB5	14484	24630	0.30%	0.044%
15	11.028	1346	1350	1354	rVV5	12847	26704	0.33%	0.048%
16	11.069	1354	1357	1362	rVB4	18087	24954	0.31%	0.044%
17	11.239	1381	1386	1392	rBV2	78527	129710	1.60%	0.231%
18	11.416	1411	1416	1422	rBV2	13831	26577	0.33%	0.047%
19	11.763	1469	1475	1485	rVB	73162	143783	1.77%	0.256%
20	11.981	1508	1512	1518	rVB6	14510	26763	0.33%	0.048%
21	12.063	1518	1526	1530	rVB4	19304	40103	0.49%	0.071%
22	12.198	1541	1549	1555	rVB5	41428	105113	1.30%	0.187%
23	12.486	1592	1598	1603	rBV7	64671	124532	1.54%	0.222%
24	12.633	1619	1623	1625	rVV3	15030	22775	0.28%	0.041%
25	12.669	1625	1629	1632	rVV2	45082	69350	0.86%	0.124%
26	12.704	1632	1635	1638	rVV3	22977	37826	0.47%	0.067%
27	12.733	1638	1640	1646	rVV5	28679	48669	0.60%	0.087%
28	12.833	1650	1657	1661	rBV3	23880	48531	0.60%	0.086%
29	12.904	1665	1669	1674	rVV3	32310	48283	0.60%	0.086%
30	13.004	1682	1686	1691	rVB5	33108	51748	0.64%	0.092%
31	13.275	1727	1732	1736	rBV2	37765	65109	0.80%	0.116%
32	13.316	1736	1739	1741	rBV2	23749	31420	0.39%	0.056%
33	13.386	1746	1751	1757	rVB4	52031	96408	1.19%	0.172%
34	13.539	1772	1777	1784	rVB3	177343	273417	3.37%	0.487%
35	13.628	1786	1792	1794	rBV3	34975	60423	0.75%	0.108%
36	13.675	1794	1800	1805	rVB4	58097	114577	1.41%	0.204%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018581.D
 Acq On : 05 Dec 2023 01:06
 Operator : MA/JU
 Sample : 05452-02DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COAJODL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	13.810	1819	1823	1826	rBV5	44505	72689	0.90%	0.130%
38	13.898	1832	1838	1844	rVB	696473	946908	11.68%	1.687%
39	14.039	1857	1862	1865	rBV	126566	185955	2.29%	0.331%
40	14.075	1865	1868	1874	rVB2	103751	148611	1.83%	0.265%
41	14.175	1879	1885	1889	rBV	712324	1069475	13.19%	1.905%
42	14.286	1899	1904	1915	rBV7	35928	77629	0.96%	0.138%
43	14.480	1930	1937	1943	rVV	3043369	4624273	57.04%	8.239%
44	14.545	1943	1948	1956	rVV	5615139	8107218	100.00%	14.444%
45	14.610	1956	1959	1964	rVB3	44198	65554	0.81%	0.117%
46	14.675	1966	1970	1976	rBV6	27716	54853	0.68%	0.098%
47	14.792	1985	1990	1996	rBV	124747	177508	2.19%	0.316%
48	14.886	2002	2006	2011	rVB4	31292	63389	0.78%	0.113%
49	14.957	2011	2018	2021	rBV4	18583	39061	0.48%	0.070%
50	15.104	2034	2043	2048	rBV4	64424	136206	1.68%	0.243%
51	15.192	2056	2058	2062	rVB	29154	28564	0.35%	0.051%
52	15.269	2066	2071	2074	rVV3	15128	28813	0.36%	0.051%
53	15.351	2081	2085	2088	rVB6	16063	23029	0.28%	0.041%
54	15.475	2100	2106	2110	rBV	1043365	1435295	17.70%	2.557%
55	15.527	2110	2115	2121	rVB	1128903	1643724	20.27%	2.928%
56	15.586	2121	2125	2128	rBV	93228	130644	1.61%	0.233%
57	15.651	2133	2136	2140	rBV	142727	187132	2.31%	0.333%
58	15.739	2146	2151	2156	rVB5	66489	108026	1.33%	0.192%
59	15.822	2162	2165	2175	rVB5	36851	70507	0.87%	0.126%
60	15.969	2178	2190	2199	rVV2	230244	535406	6.60%	0.954%
61	16.057	2199	2205	2211	rVV3	36939	65013	0.80%	0.116%
62	16.204	2225	2230	2236	rVB	161894	236325	2.91%	0.421%
63	16.322	2245	2250	2257	rBV	132341	204281	2.52%	0.364%
64	16.392	2257	2262	2267	rBV3	87334	140117	1.73%	0.250%
65	16.492	2274	2279	2280	rBV3	42646	58476	0.72%	0.104%
66	16.533	2283	2286	2290	rVV2	80921	114673	1.41%	0.204%
67	16.580	2291	2294	2298	rVB3	27834	36806	0.45%	0.066%
68	16.686	2308	2312	2316	rBV2	44405	57140	0.70%	0.102%
69	16.963	2353	2359	2362	rBV6	30997	64185	0.79%	0.114%
70	17.010	2364	2367	2370	rVV2	57866	65255	0.80%	0.116%
71	17.045	2370	2373	2377	rVB2	67193	89892	1.11%	0.160%
72	17.104	2380	2383	2385	rBV3	20824	25991	0.32%	0.046%
73	17.145	2386	2390	2395	rVB2	53579	88504	1.09%	0.158%
74	17.233	2398	2405	2410	rBV	3970837	5746729	70.88%	10.238%
75	17.269	2410	2411	2415	rVB2	92837	85213	1.05%	0.152%
76	17.327	2415	2421	2426	rBV	1138547	1636689	20.19%	2.916%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018581.D
 Acq On : 05 Dec 2023 01:06
 Operator : MA/JU
 Sample : 05452-02DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AJODL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

77	17.421	2431	2437	2448	rVB3	86592	193161	2.38%	0.344%
78	17.604	2463	2468	2473	rBV3	110308	191896	2.37%	0.342%
79	17.974	2528	2531	2536	rVB4	50691	77853	0.96%	0.139%
80	18.063	2542	2546	2550	rBV	125579	156190	1.93%	0.278%
81	18.121	2551	2556	2557	rVV4	141728	196098	2.42%	0.349%
82	18.139	2557	2559	2564	rVB	186632	231666	2.86%	0.413%
83	18.216	2567	2572	2578	rVB2	205045	294911	3.64%	0.525%
84	18.286	2578	2584	2589	rBV	316729	475484	5.86%	0.847%
85	18.368	2595	2598	2601	rBV2	35279	52184	0.64%	0.093%
86	18.468	2612	2615	2619	rVB4	41858	50096	0.62%	0.089%
87	18.521	2620	2624	2630	rVV2	112009	163634	2.02%	0.292%
88	18.580	2630	2634	2638	rBV3	73284	99494	1.23%	0.177%
89	18.621	2638	2641	2648	rVV4	35195	57500	0.71%	0.102%
90	18.845	2677	2679	2684	rVB5	30931	32236	0.40%	0.057%
91	18.963	2696	2699	2709	rVB4	56306	100543	1.24%	0.179%
92	19.239	2742	2746	2753	rVB	736195	907571	11.19%	1.617%
93	19.357	2763	2766	2771	rVB3	72233	86763	1.07%	0.155%
94	19.563	2796	2801	2805	rBV	1528198	2120324	26.15%	3.778%
95	19.592	2805	2806	2814	rVB	394720	351600	4.34%	0.626%
96	19.963	2866	2869	2875	rVB	140827	183602	2.26%	0.327%
97	20.645	2982	2985	2991	rBV	109831	135475	1.67%	0.241%
98	21.315	3094	3099	3105	rBV	4635497	5908513	72.88%	10.527%
99	23.533	3471	3476	3483	rVB	669145	1208235	14.90%	2.153%
100	23.686	3496	3502	3513	rVB	2707745	5207720	64.24%	9.278%




Sum of corrected areas: 56128933

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018581.D
Acq On : 05 Dec 2023 01:06
Operator : MA/JU
Sample : 05452-02DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COAJ0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

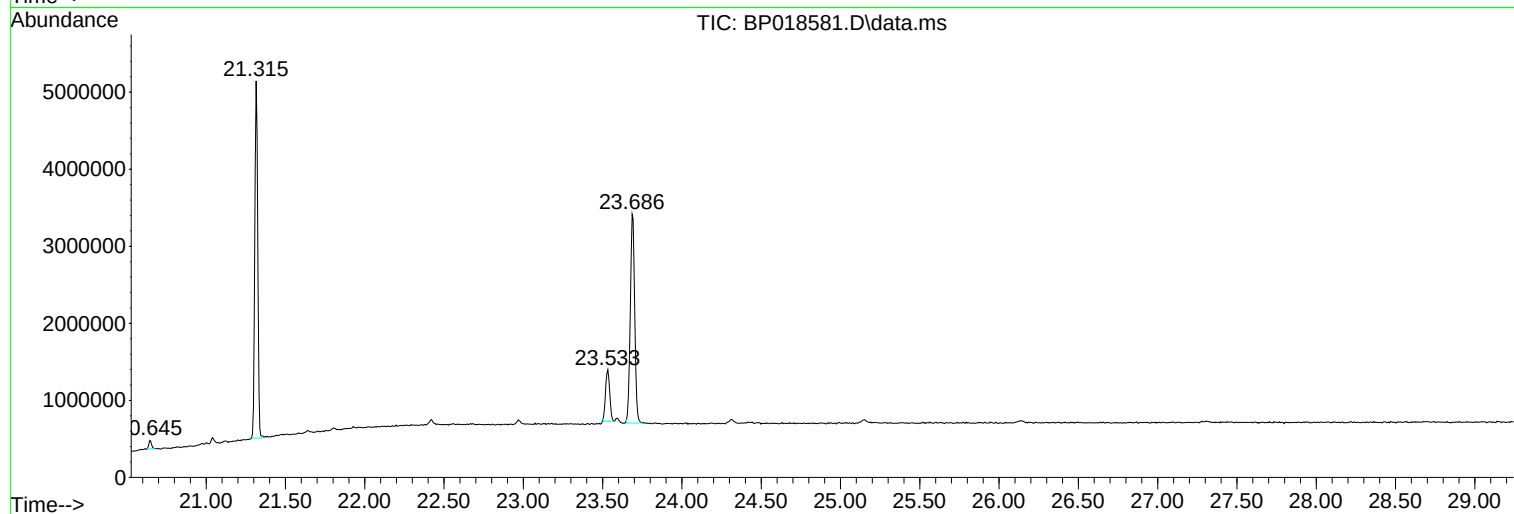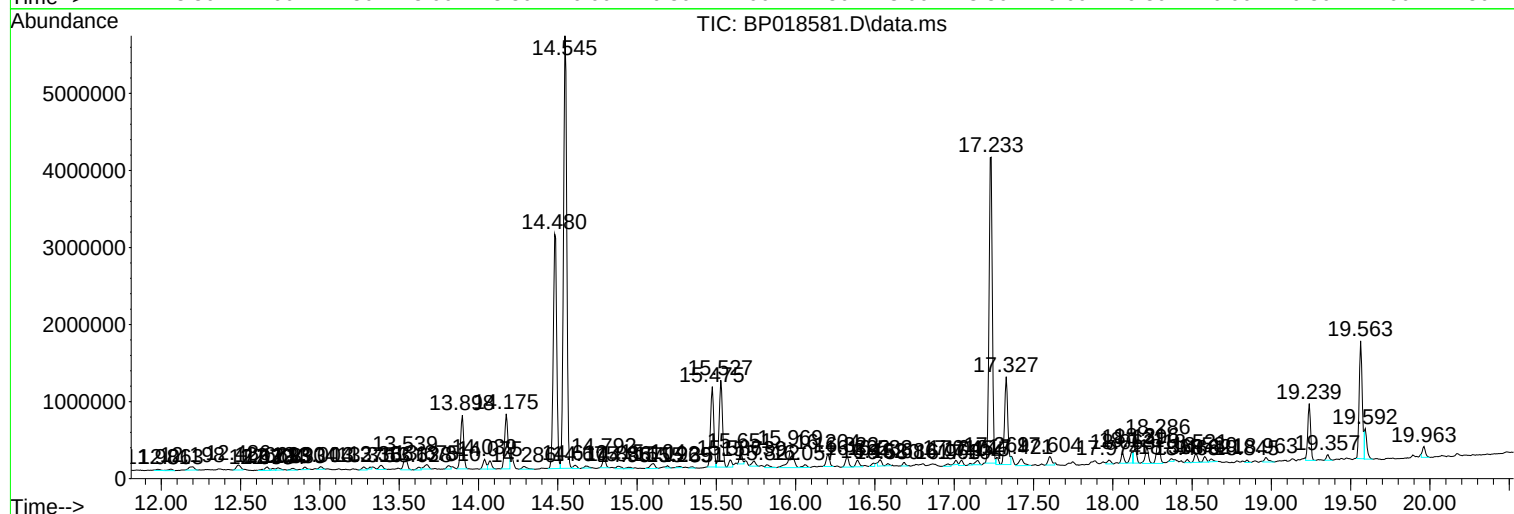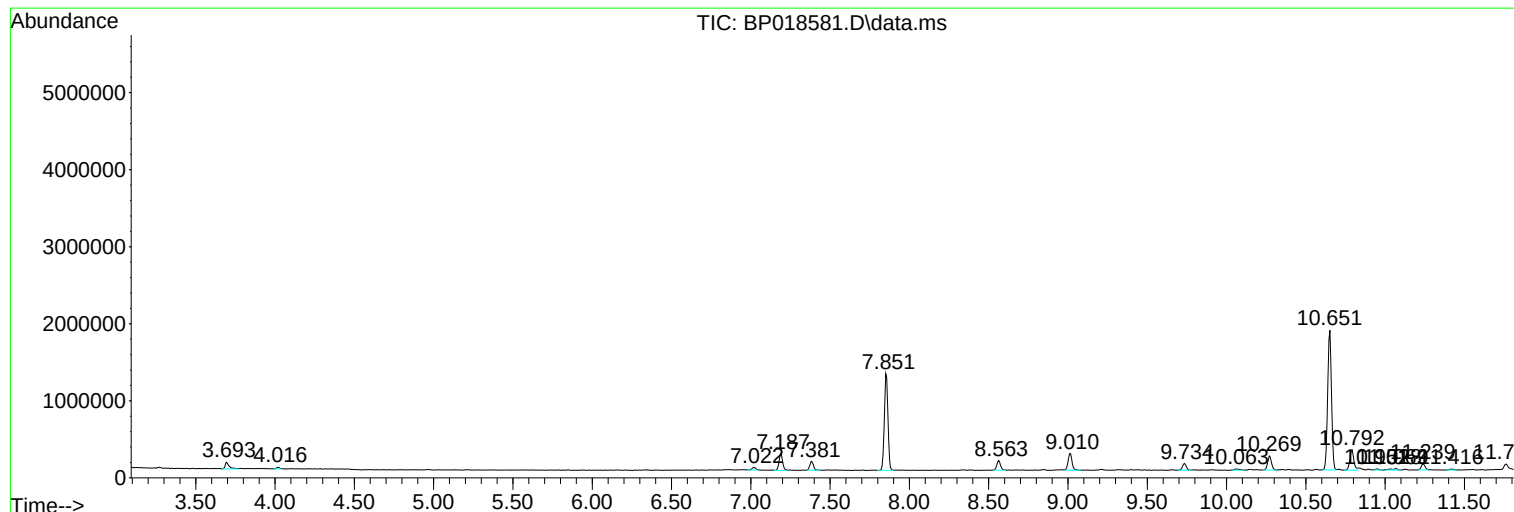

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018581.D
Acq On : 05 Dec 2023 01:06
Operator : MA/JU
Sample : 05452-02DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018581.D
Acq On : 05 Dec 2023 01:06
Operator : MA/JU
Sample : 05452-02DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------