

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018584.D
 Acq On : 05 Dec 2023 02:47
 Operator : MA/JU
 Sample : 05411-13RX
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QJ2RX

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018584.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	40	rVB	68130	91424	0.99%	0.108%
2	3.693	99	103	111	rBV	279311	406674	4.40%	0.479%
3	3.928	139	143	149	rVB	22553	32565	0.35%	0.038%
4	4.022	154	159	164	rVB	29959	41378	0.45%	0.049%
5	4.951	314	317	321	rVB3	5872	9301	0.10%	0.011%
6	5.357	379	386	392	rBV	50668	78677	0.85%	0.093%
7	5.493	402	409	410	rBV6	6885	10141	0.11%	0.012%
8	5.863	468	472	476	rVB	11622	16249	0.18%	0.019%
9	7.022	661	669	676	rBV	262717	419104	4.53%	0.494%
10	7.193	690	698	710	rVB	1084903	1721627	18.62%	2.029%
11	7.381	724	730	738	rBV	970276	1544232	16.70%	1.820%
12	7.469	740	745	746	rBV3	10991	12002	0.13%	0.014%
13	7.851	803	810	819	rVB	1068047	1653869	17.89%	1.949%
14	8.228	867	874	880	rBV2	60048	105924	1.15%	0.125%
15	8.563	924	931	939	rVV	853709	1302798	14.09%	1.536%
16	9.016	1001	1008	1018	rVB	1292859	2103138	22.75%	2.479%
17	9.439	1076	1080	1084	rVB6	7923	10990	0.12%	0.013%
18	9.734	1121	1130	1138	rBV	998389	1583508	17.13%	1.867%
19	9.898	1154	1158	1165	rVB4	10838	22119	0.24%	0.026%
20	10.075	1184	1188	1193	rVB7	7162	15147	0.16%	0.018%
21	10.269	1213	1221	1230	rBV	1575554	2559989	27.69%	3.018%
22	10.651	1276	1286	1291	rBV	1504359	2553326	27.62%	3.010%
23	10.698	1291	1294	1301	rVB	413272	641119	6.94%	0.756%
24	10.786	1301	1309	1320	rBV	1453615	2503586	27.08%	2.951%
25	11.933	1497	1504	1510	rBV5	8289	13631	0.15%	0.016%
26	12.233	1551	1555	1562	rVB2	33716	56114	0.61%	0.066%
27	12.310	1562	1568	1574	rBV	122057	188365	2.04%	0.222%
28	12.528	1600	1605	1612	rBV	49130	77747	0.84%	0.092%
29	13.098	1699	1702	1707	rVB6	7271	11529	0.12%	0.014%
30	13.322	1736	1740	1745	rVB2	13334	20061	0.22%	0.024%
31	13.386	1745	1751	1758	rVV2	40792	66803	0.72%	0.079%
32	13.457	1758	1763	1764	rVV4	8983	12839	0.14%	0.015%
33	13.516	1767	1773	1781	rVB4	15366	31486	0.34%	0.037%
34	13.645	1789	1795	1796	rBV5	10245	14807	0.16%	0.017%
35	13.710	1803	1806	1812	rVB4	5485	10008	0.11%	0.012%
36	13.810	1818	1823	1827	rVB5	11516	17603	0.19%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018584.D
 Acq On : 05 Dec 2023 02:47
 Operator : MA/JU
 Sample : 05411-13RX
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QJ2RX

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	13.857	1827	1831	1832	rBV3	10191	10340	0.11%	0.012%
38	13.898	1832	1838	1849	rVB	3553485	4877054	52.76%	5.749%
39	14.175	1875	1885	1895	rBV	3905802	5698734	61.64%	6.717%
40	14.480	1930	1937	1945	rBV	2503835	3782090	40.91%	4.458%
41	14.545	1945	1948	1952	rVB2	17105	23264	0.25%	0.027%
42	14.680	1962	1971	1980	rBV	233456	385722	4.17%	0.455%
43	14.892	2004	2007	2014	rVB6	15040	24702	0.27%	0.029%
44	15.298	2071	2076	2078	rBV5	7344	13500	0.15%	0.016%
45	15.474	2099	2106	2113	rBV	5393483	7472908	80.84%	8.809%
46	15.533	2113	2116	2119	rVV4	11799	15143	0.16%	0.018%
47	15.592	2119	2126	2140	rVV	1340275	1914682	20.71%	2.257%
48	15.716	2143	2147	2156	rVB4	26895	49987	0.54%	0.059%
49	16.045	2198	2203	2207	rVB3	8844	11250	0.12%	0.013%
50	16.257	2236	2239	2243	rVB5	8946	11875	0.13%	0.014%
51	16.633	2300	2303	2309	rVB8	7630	10747	0.12%	0.013%
52	17.227	2398	2404	2410	rBV	3130456	4436324	47.99%	5.229%
53	17.327	2415	2421	2432	rVV	5926739	8403440	90.90%	9.905%
54	17.904	2516	2519	2525	rVB4	20689	27612	0.30%	0.033%
55	17.998	2532	2535	2538	rBV4	9435	11926	0.13%	0.014%
56	18.121	2551	2556	2563	rBV	130646	183950	1.99%	0.217%
57	19.139	2725	2729	2734	rBV3	76235	101902	1.10%	0.120%
58	19.210	2736	2741	2744	rBV	76777	111296	1.20%	0.131%
59	19.351	2762	2765	2774	rBV5	58711	86224	0.93%	0.102%
60	19.562	2795	2801	2808	rBV	7106922	9244529	100.00%	10.897%
61	21.033	3048	3051	3057	rBV4	63620	106613	1.15%	0.126%
62	21.315	3094	3099	3108	rBV	3251891	4218106	45.63%	4.972%
63	23.533	3469	3476	3483	rBV2	4793269	9089988	98.33%	10.715%
64	23.686	3495	3502	3511	rVB	2296716	4553316	49.25%	5.367%



Sum of corrected areas: 84837104

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018584.D
Acq On : 05 Dec 2023 02:47
Operator : MA/JU
Sample : 05411-13RX
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ2RX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

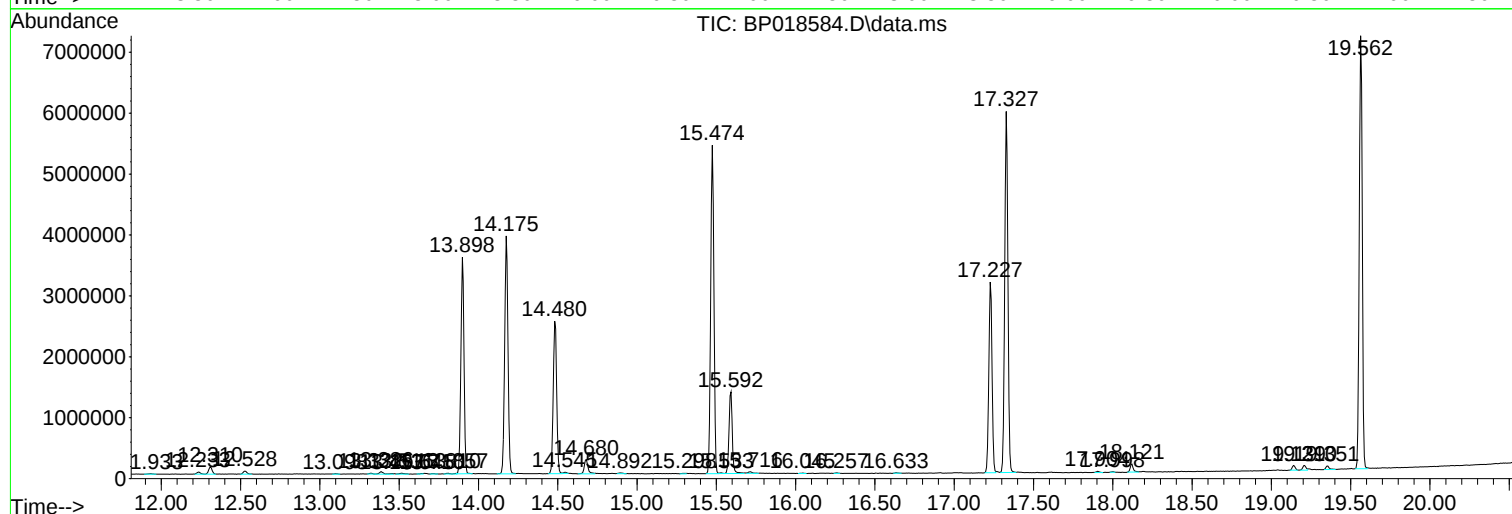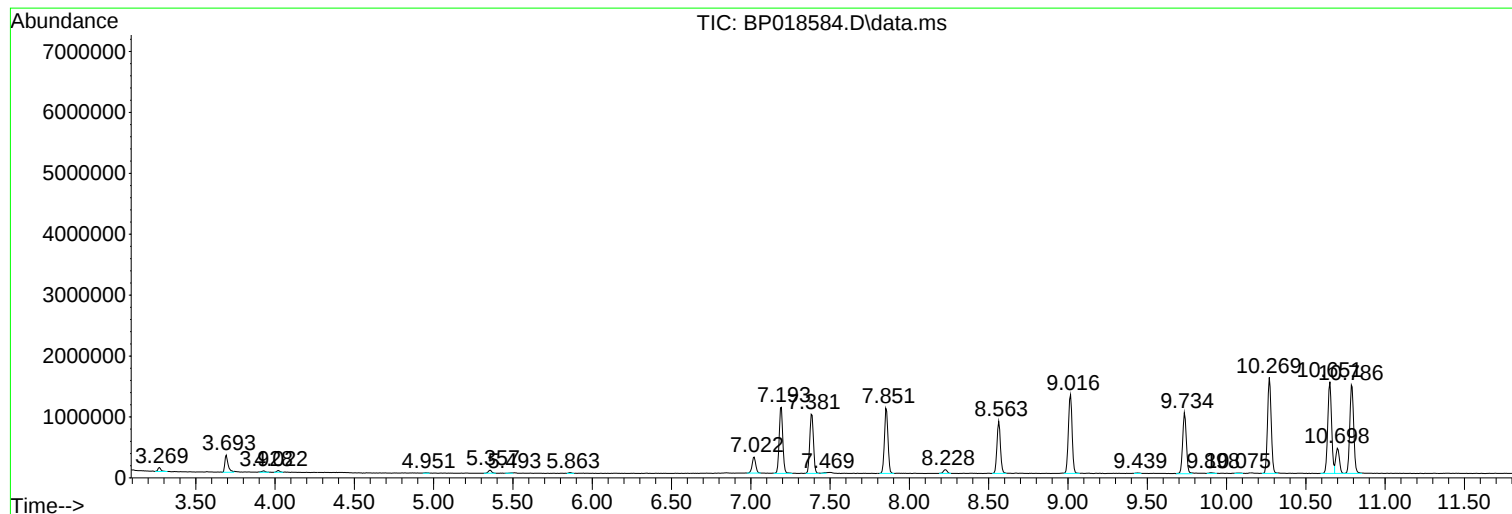

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018584.D
Acq On : 05 Dec 2023 02:47
Operator : MA/JU
Sample : 05411-13RX
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ2RX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018584.D
Acq On : 05 Dec 2023 02:47
Operator : MA/JU
Sample : 05411-13RX
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ2RX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------