

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018586.D
 Acq On : 05 Dec 2023 03:55
 Operator : MA/JU
 Sample : 05441-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018586.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	36	rVB	62812	78453	0.69%	0.083%
2	3.687	98	102	119	rVB	398471	597867	5.24%	0.635%
3	3.928	140	143	147	rVB3	17028	22935	0.20%	0.024%
4	4.017	155	158	164	rBV2	22998	33771	0.30%	0.036%
5	7.022	663	669	679	rVB	301262	481376	4.22%	0.511%
6	7.187	691	697	706	rVB	1354242	2117194	18.57%	2.248%
7	7.381	724	730	740	rVV	1181434	1839961	16.14%	1.954%
8	7.475	744	746	753	rVB4	10741	15493	0.14%	0.016%
9	7.852	803	810	818	rVB	1187167	1856328	16.28%	1.971%
10	8.563	924	931	940	rBV	986751	1534962	13.46%	1.630%
11	9.016	1001	1008	1015	rBV	1557940	2521323	22.11%	2.677%
12	9.440	1077	1080	1088	rVB4	12575	22725	0.20%	0.024%
13	9.734	1123	1130	1142	rBV	1174389	1852403	16.25%	1.967%
14	10.269	1214	1221	1232	rBV	1894416	3025821	26.54%	3.213%
15	10.652	1278	1286	1295	rVB	1736287	2882982	25.28%	3.061%
16	10.787	1302	1309	1323	rVB	1733280	2879086	25.25%	3.057%
17	11.181	1374	1376	1379	rVB	10899	12788	0.11%	0.014%
18	11.469	1416	1425	1429	rBV6	10854	23476	0.21%	0.025%
19	11.899	1492	1498	1499	rBV2	9142	12438	0.11%	0.013%
20	12.234	1551	1555	1562	rVB3	37747	61891	0.54%	0.066%
21	13.387	1747	1751	1757	rVB2	43976	67235	0.59%	0.071%
22	13.898	1831	1838	1846	rBV	4203499	5682838	49.84%	6.034%
23	14.175	1876	1885	1895	rBV2	4512225	6632903	58.17%	7.043%
24	14.481	1931	1937	1946	rVB	2983390	4244099	37.22%	4.506%
25	14.675	1965	1970	1981	rBV2	249236	402535	3.53%	0.427%
26	14.898	2006	2008	2013	rVB5	14667	19646	0.17%	0.021%
27	15.475	2099	2106	2112	rBV	6259111	8811294	77.27%	9.355%
28	15.592	2119	2126	2136	rBV	1601652	2227978	19.54%	2.366%
29	15.710	2143	2146	2152	rVB2	29140	46943	0.41%	0.050%
30	16.263	2237	2240	2244	rVB3	11827	18258	0.16%	0.019%
31	16.904	2346	2349	2353	rBV5	10839	15486	0.14%	0.016%
32	17.228	2398	2404	2411	rBV	3563265	5116966	44.87%	5.433%
33	17.328	2415	2421	2432	rBV2	7208921	10219839	89.63%	10.851%
34	18.116	2551	2555	2562	rBV2	65881	102268	0.90%	0.109%
35	19.139	2725	2729	2736	rBV2	89908	123811	1.09%	0.131%
36	19.204	2737	2740	2745	rVV	79730	107977	0.95%	0.115%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018586.D
Acq On : 05 Dec 2023 03:55
Operator : MA/JU
Sample : 05441-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.351	2762	2765	2769	rBV4	41715	52891	0.46%	0.056%
38	19.563	2795	2801	2815	rBV	8976844	11402743	100.00%	12.107%
39	21.316	3094	3099	3105	rBV	3537602	4400587	38.59%	4.672%
40	23.533	3469	3476	3491	rVB	4449569	8583666	75.28%	9.114%
41	23.680	3495	3501	3516	rVB	1985623	4030394	35.35%	4.279%




Sum of corrected areas: 94183630

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018586.D
Acq On : 05 Dec 2023 03:55
Operator : MA/JU
Sample : 05441-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

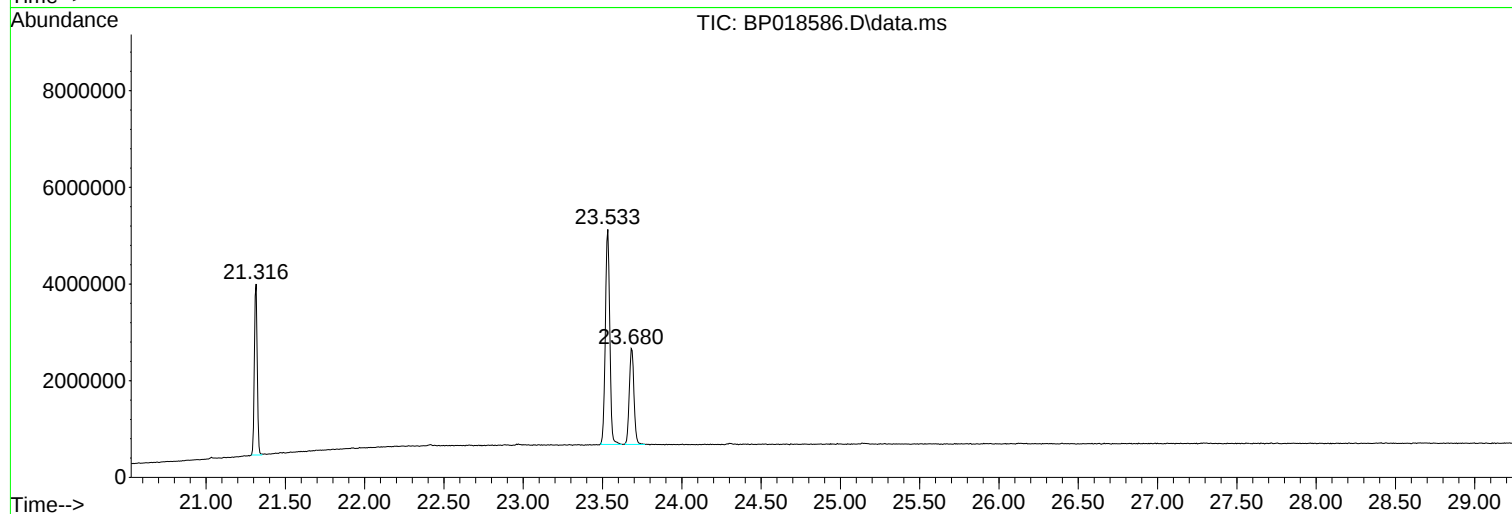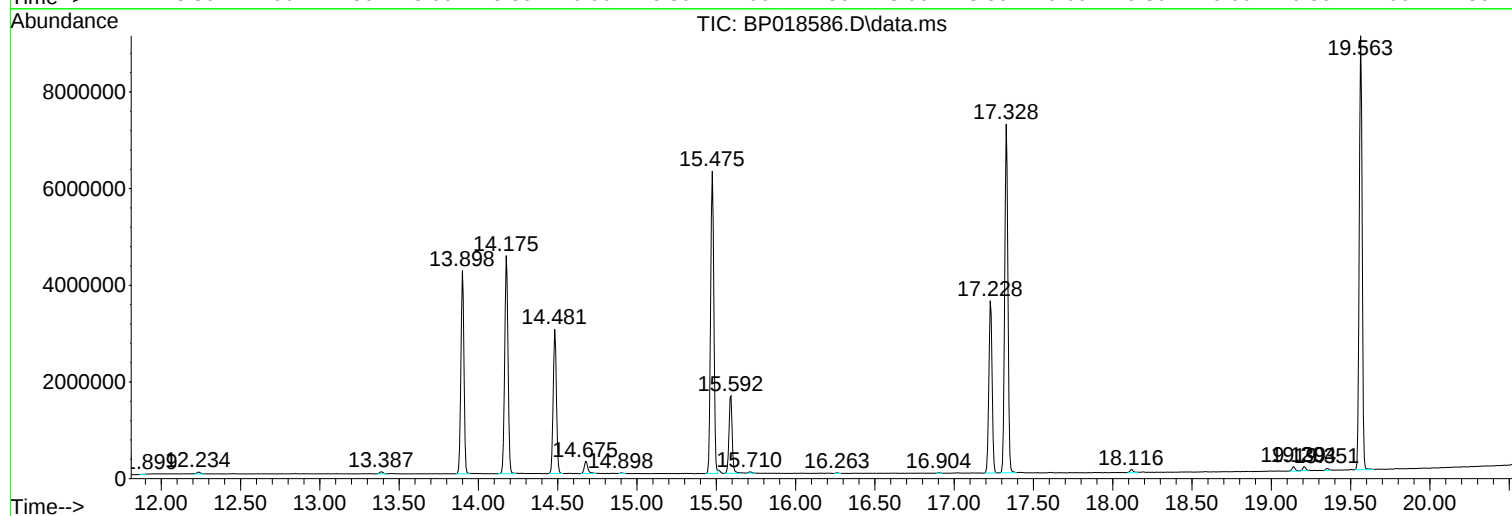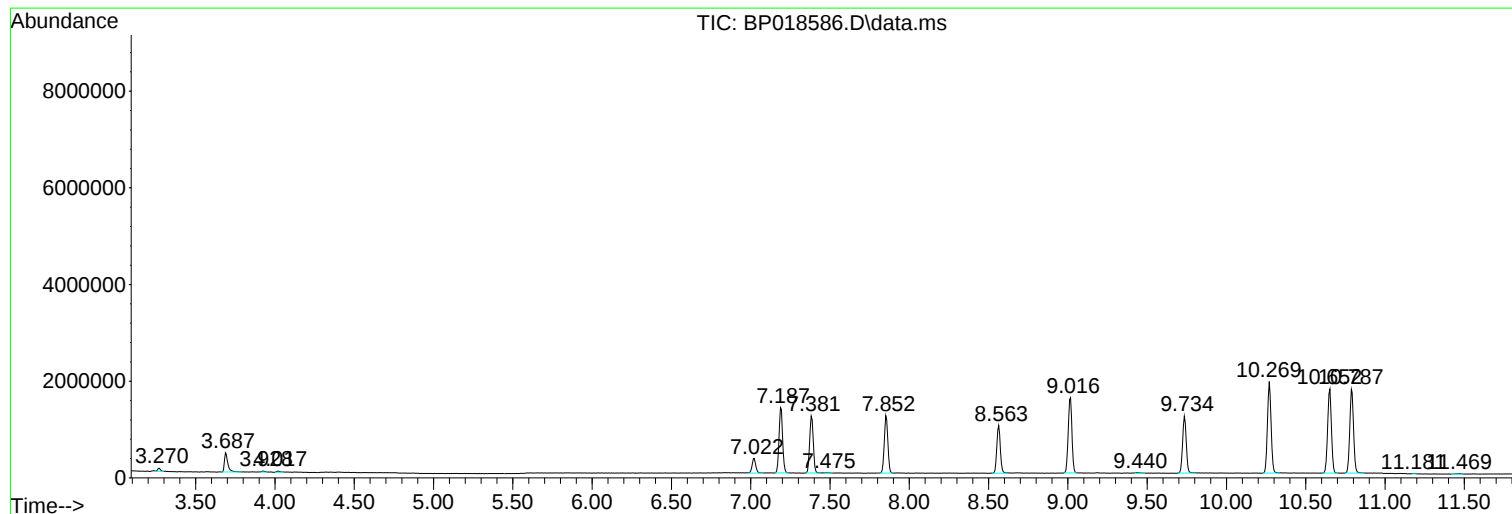

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018586.D
Acq On : 05 Dec 2023 03:55
Operator : MA/JU
Sample : 05441-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018586.D
Acq On : 05 Dec 2023 03:55
Operator : MA/JU
Sample : 05441-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc