

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018589.D
 Acq On : 05 Dec 2023 06:11
 Operator : MA/JU
 Sample : PB157333BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK333

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018589.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	41	rVB	107832	159545	1.46%	0.150%
2	3.687	97	102	117	rBV	1329632	2010511	18.39%	1.890%
3	4.017	154	158	166	rVB2	19792	33036	0.30%	0.031%
4	7.022	662	669	679	rVB	1646929	2587512	23.66%	2.432%
5	7.187	690	697	706	rVB	1321509	2058285	18.82%	1.935%
6	7.381	722	730	740	rBV	1553473	2423983	22.17%	2.279%
7	7.564	753	761	764	rBV4	6372	16404	0.15%	0.015%
8	7.852	803	810	819	rVB	1378354	2154478	19.70%	2.025%
9	8.564	923	931	941	rBV	2155468	3391205	31.01%	3.188%
10	9.016	1000	1008	1019	rBV	1589376	2594016	23.72%	2.438%
11	9.734	1122	1130	1145	rBV	1260881	2037870	18.64%	1.916%
12	10.269	1214	1221	1232	rBV	2180086	3467491	31.71%	3.260%
13	10.652	1278	1286	1293	rBV	1969701	3302724	30.21%	3.105%
14	10.787	1302	1309	1321	rBV	1741101	2913717	26.65%	2.739%
15	12.234	1549	1555	1562	rBV3	42301	75518	0.69%	0.071%
16	13.387	1746	1751	1759	rBV4	27247	46930	0.43%	0.044%
17	13.899	1831	1838	1847	rBV	4396379	5822431	53.25%	5.473%
18	14.175	1878	1885	1894	rBV	4789511	6848028	62.63%	6.437%
19	14.481	1931	1937	1945	rBV	3399700	4931688	45.10%	4.636%
20	14.681	1964	1971	1982	rBV	1878437	2687869	24.58%	2.527%
21	15.475	2099	2106	2113	rBV	5985193	8218001	75.16%	7.725%
22	15.534	2113	2116	2119	rVV	8332	11657	0.11%	0.011%
23	15.593	2119	2126	2141	rVV	1482642	2161118	19.76%	2.032%
24	15.710	2143	2146	2154	rVB	33922	55509	0.51%	0.052%
25	16.263	2235	2240	2244	rVB7	8607	15014	0.14%	0.014%
26	17.010	2365	2367	2374	rVB3	10351	19768	0.18%	0.019%
27	17.228	2397	2404	2414	rBV	4325559	6110226	55.88%	5.744%
28	17.328	2415	2421	2440	rVB	6829954	9626637	88.04%	9.049%
29	18.122	2553	2556	2560	rBV4	13833	20395	0.19%	0.019%
30	19.139	2725	2729	2734	rBV	90107	122268	1.12%	0.115%
31	19.210	2737	2741	2746	rVV	81746	109195	1.00%	0.103%
32	19.563	2795	2801	2811	rBV	8333897	10934185	100.00%	10.278%
33	21.316	3094	3099	3105	rBV	4604030	5658395	51.75%	5.319%
34	23.533	3469	3476	3484	rBV2	4481056	8521962	77.94%	8.011%
35	23.686	3495	3502	3516	rVB	2685890	5231971	47.85%	4.918%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018589.D
Acq On : 05 Dec 2023 06:11
Operator : MA/JU
Sample : PB157333BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK333

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 106379542

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018589.D
Acq On : 05 Dec 2023 06:11
Operator : MA/JU
Sample : PB157333BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK333

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

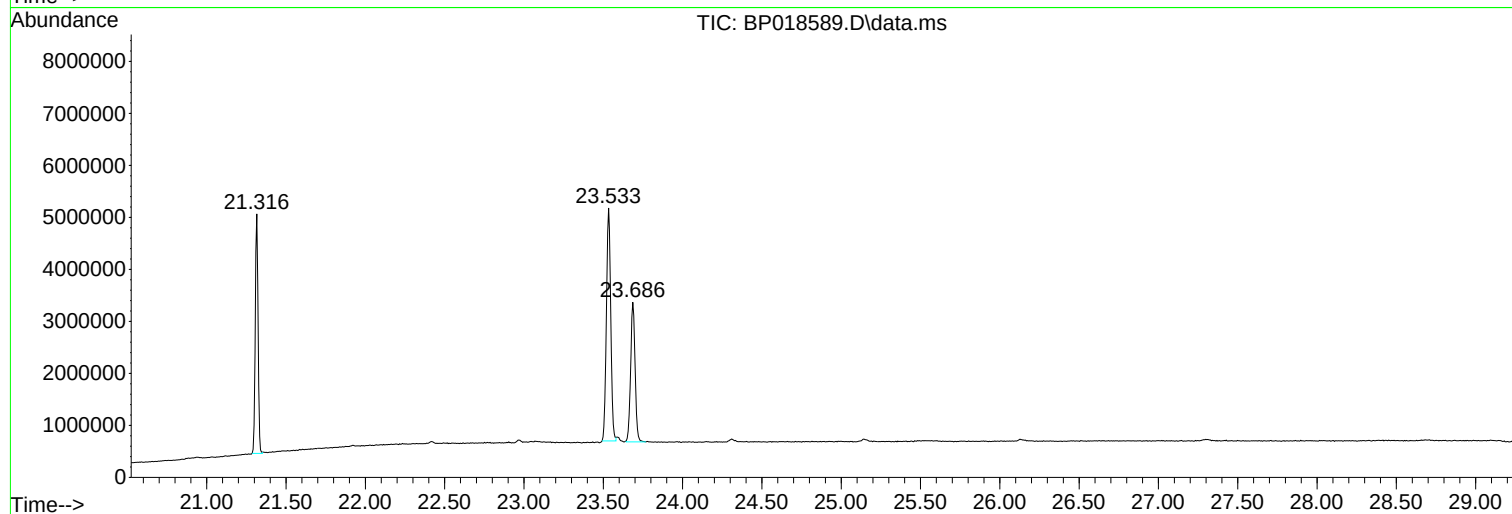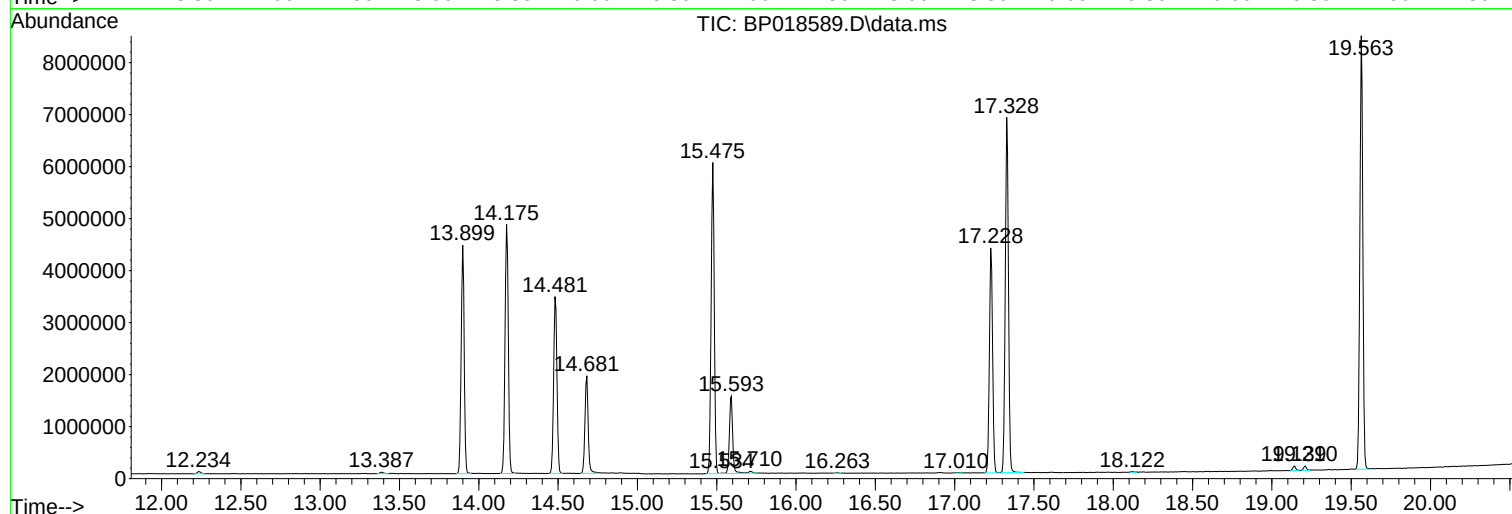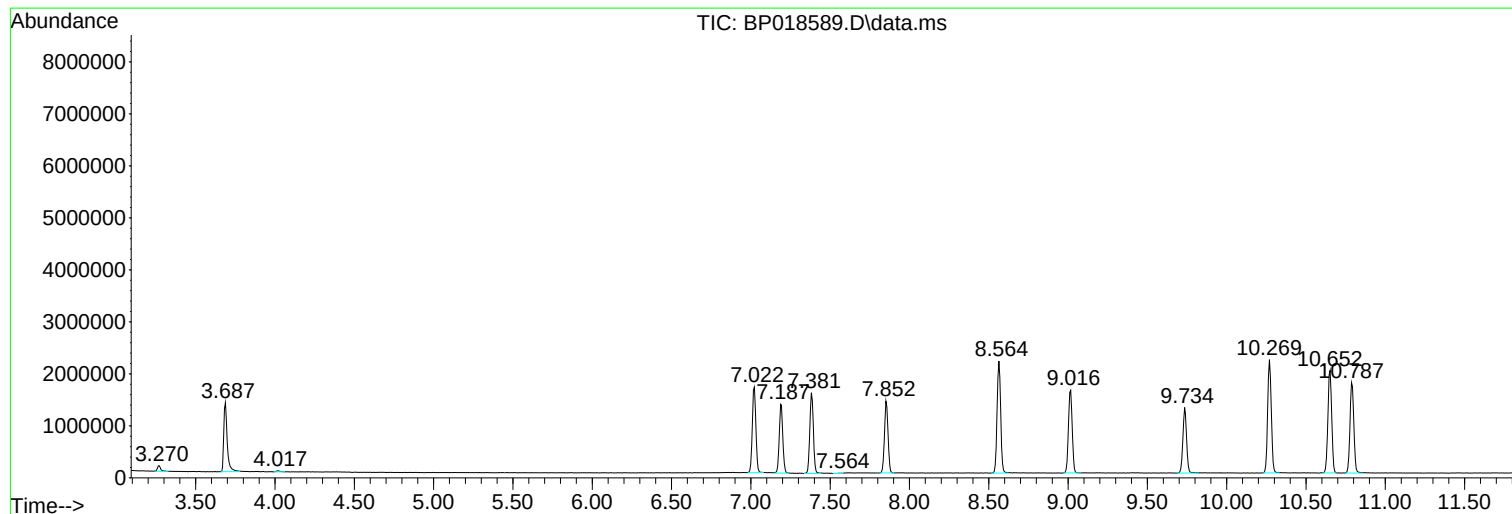

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018589.D
Acq On : 05 Dec 2023 06:11
Operator : MA/JU
Sample : PB157333BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK333

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018589.D
Acq On : 05 Dec 2023 06:11
Operator : MA/JU
Sample : PB157333BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK333

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------