

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018592.D
 Acq On : 05 Dec 2023 08:55
 Operator : MA/JU
 Sample : PB157362BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK362

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018592.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	41	rVB	137697	201738	1.64%	0.168%
2	3.681	97	101	114	rBV	1522677	2339351	19.02%	1.944%
3	4.011	154	157	165	rVB3	26307	42975	0.35%	0.036%
4	5.811	453	463	468	rBV5	24511	90145	0.73%	0.075%
5	7.010	660	667	675	rBV	1896934	2898214	23.56%	2.408%
6	7.181	689	696	704	rVB	1619394	2464639	20.03%	2.048%
7	7.375	720	729	738	rBV	1839769	2910776	23.66%	2.419%
8	7.846	801	809	817	rBV	1528630	2401692	19.52%	1.996%
9	8.422	900	907	908	rBV5	8402	15194	0.12%	0.013%
10	8.557	923	930	942	rBV	2350422	3777706	30.71%	3.139%
11	9.004	998	1006	1015	rBV	1803645	2924964	23.78%	2.430%
12	9.181	1027	1036	1048	rVB6	27896	108413	0.88%	0.090%
13	9.728	1121	1129	1144	rBV	1350587	2165769	17.61%	1.800%
14	9.993	1169	1174	1175	rBV2	10155	13147	0.11%	0.011%
15	10.263	1211	1220	1231	rBV	2389705	3874823	31.50%	3.220%
16	10.646	1277	1285	1293	rVV	2219843	3682233	29.93%	3.060%
17	10.781	1298	1308	1323	rVB	1912081	3258377	26.49%	2.707%
18	11.875	1489	1494	1497	rBV3	15297	25625	0.21%	0.021%
19	12.234	1549	1555	1561	rVB	46049	79574	0.65%	0.066%
20	12.440	1585	1590	1598	rBV4	9018	22655	0.18%	0.019%
21	12.834	1652	1657	1663	rVB6	7679	15309	0.12%	0.013%
22	13.387	1745	1751	1756	rVB4	17182	30312	0.25%	0.025%
23	13.457	1756	1763	1765	rBV5	8851	19984	0.16%	0.017%
24	13.898	1831	1838	1849	rBV	4751253	6599912	53.65%	5.484%
25	14.175	1876	1885	1900	rBV	5255566	7646713	62.16%	6.354%
26	14.481	1930	1937	1948	rBV	3737859	5527244	44.93%	4.593%
27	14.681	1964	1971	1982	rBV	2215813	3127920	25.43%	2.599%
28	15.475	2099	2106	2118	rBV	6964038	10014360	81.41%	8.321%
29	15.592	2120	2126	2141	rVV	1870501	2503202	20.35%	2.080%
30	15.716	2143	2147	2151	rVB3	32505	48597	0.40%	0.040%
31	16.039	2200	2202	2208	rVB3	8451	13131	0.11%	0.011%
32	16.722	2315	2318	2323	rVB6	11943	17261	0.14%	0.014%
33	17.016	2365	2368	2376	rVB3	11777	24230	0.20%	0.020%
34	17.233	2398	2405	2415	rBV	4885346	6871596	55.86%	5.710%
35	17.333	2415	2422	2439	rBV	7792185	10805965	87.84%	8.979%
36	17.904	2515	2519	2524	rVB3	10232	14755	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018592.D
Acq On : 05 Dec 2023 08:55
Operator : MA/JU
Sample : PB157362BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK362

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	18.122	2553	2556	2559	rBV3	25716	32164	0.26%	0.027%
38	19.145	2726	2730	2735	rBV	94871	131751	1.07%	0.109%
39	19.216	2738	2742	2746	rBV	91064	123944	1.01%	0.103%
40	19.569	2796	2802	2809	rBV	9298627	12301839	100.00%	10.222%
41	21.321	3095	3100	3106	rBV	4665314	5627863	45.75%	4.676%
42	23.545	3471	3478	3485	rBV2	5013253	9603768	78.07%	7.980%
43	23.698	3497	3504	3515	rVB	3033334	5949035	48.36%	4.943%




Sum of corrected areas: 120348865

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018592.D
Acq On : 05 Dec 2023 08:55
Operator : MA/JU
Sample : PB157362BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK362

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

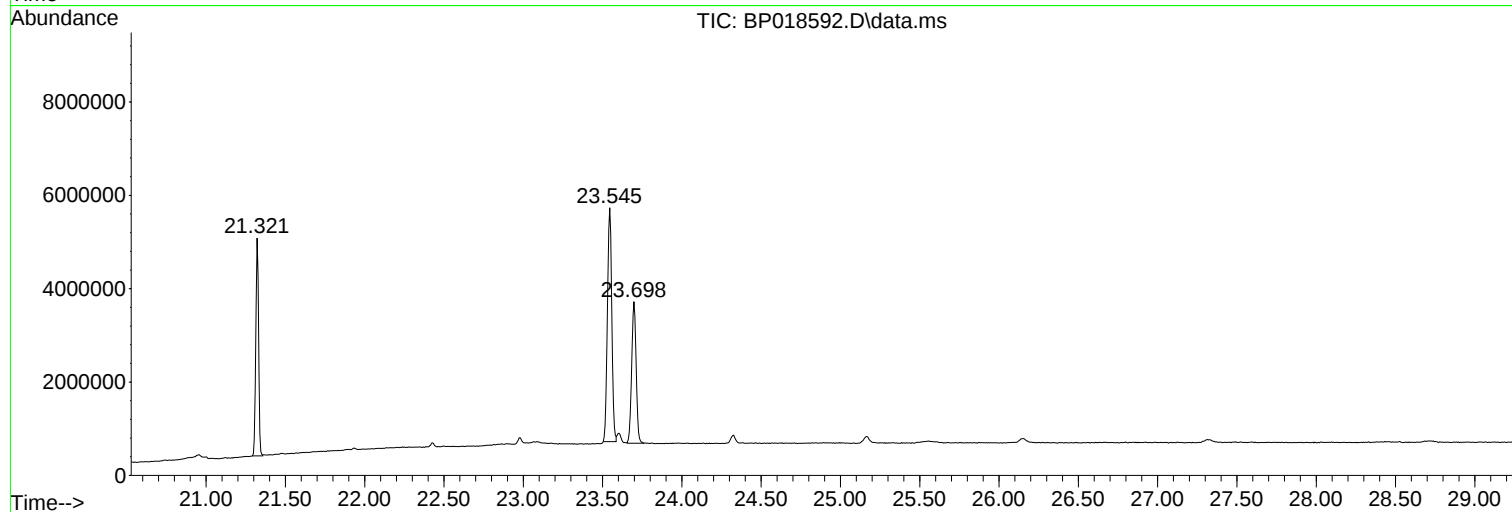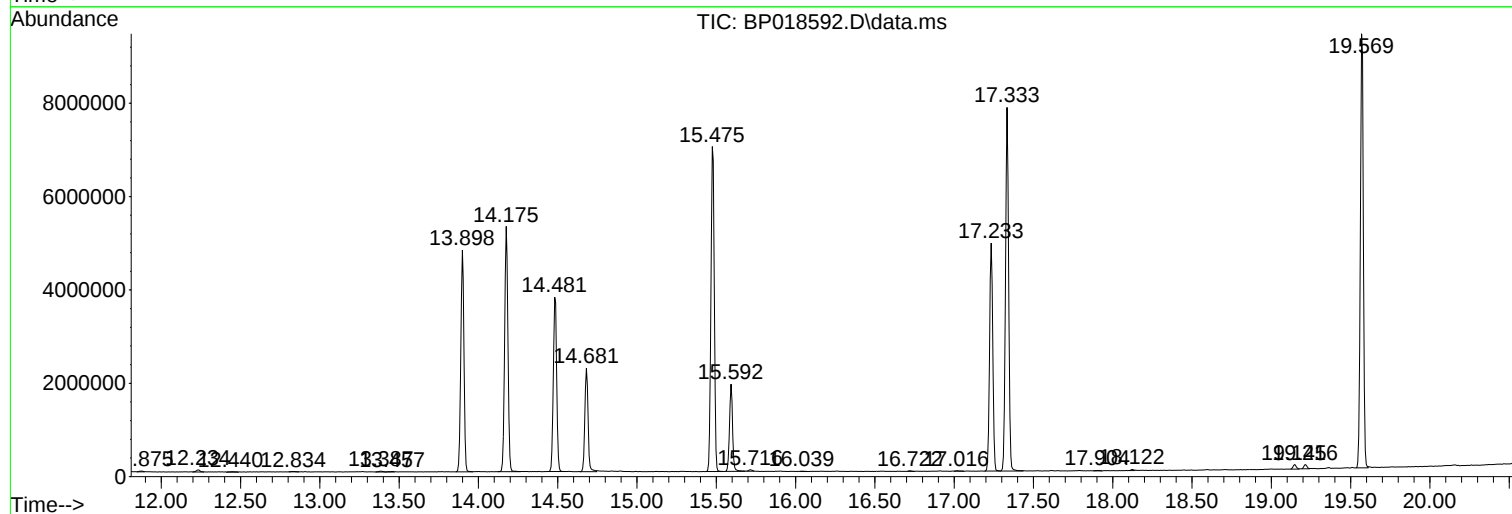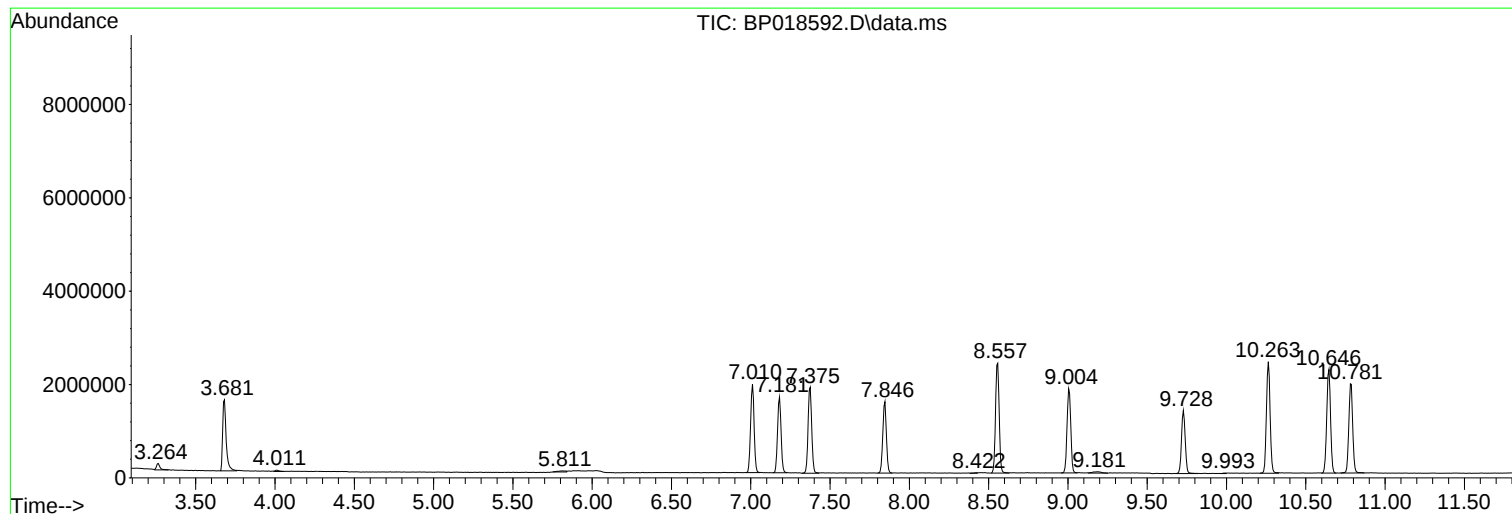

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018592.D
Acq On : 05 Dec 2023 08:55
Operator : MA/JU
Sample : PB157362BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK362

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018592.D
Acq On : 05 Dec 2023 08:55
Operator : MA/JU
Sample : PB157362BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK362

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------