

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018594.D
 Acq On : 05 Dec 2023 10:03
 Operator : MA/JU
 Sample : 05441-13
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	35	rVB2	69289	91181	0.80%	0.092%
2	3.687	98	102	116	rBV	336216	523212	4.59%	0.530%
3	3.922	139	142	147	rVB2	20295	28922	0.25%	0.029%
4	4.017	154	158	168	rVB3	26987	47784	0.42%	0.048%
5	7.016	661	668	677	rVB	332287	514552	4.52%	0.521%
6	7.187	691	697	706	rBV	1472023	2251142	19.77%	2.279%
7	7.381	724	730	742	rBV	1284868	1969816	17.30%	1.995%
8	7.852	803	810	820	rBV	1376673	2146209	18.85%	2.173%
9	8.563	924	931	939	rBV	1046809	1616279	14.19%	1.637%
10	9.010	1000	1007	1017	rBV	1649661	2686765	23.59%	2.720%
11	9.175	1032	1035	1040	rBV3	9433	16019	0.14%	0.016%
12	9.440	1075	1080	1086	rVB4	20628	33298	0.29%	0.034%
13	9.734	1122	1130	1144	rBV	1199230	1957453	17.19%	1.982%
14	10.269	1213	1221	1230	rBV	1952886	3188436	28.00%	3.228%
15	10.646	1278	1285	1294	rVB	1957984	3308121	29.05%	3.350%
16	10.787	1302	1309	1321	rBV	1797466	3029204	26.60%	3.067%
17	11.434	1415	1419	1421	rBV2	8496	11973	0.11%	0.012%
18	11.834	1485	1487	1491	rVB	8801	12634	0.11%	0.013%
19	11.928	1498	1503	1507	rVB5	11024	20402	0.18%	0.021%
20	11.993	1511	1514	1517	rBV	10341	15883	0.14%	0.016%
21	12.234	1546	1555	1560	rBV3	39171	68122	0.60%	0.069%
22	13.387	1746	1751	1756	rBV2	40502	65757	0.58%	0.067%
23	13.898	1832	1838	1846	rBV	4180000	5670046	49.79%	5.741%
24	14.175	1877	1885	1896	rBV	4675279	6749844	59.27%	6.834%
25	14.481	1929	1937	1946	rBV	3320807	4846144	42.55%	4.907%
26	14.681	1965	1971	1981	rBV	243983	389532	3.42%	0.394%
27	14.898	2004	2008	2012	rBV7	12417	21621	0.19%	0.022%
28	15.475	2099	2106	2113	rBV	6204864	8775092	77.05%	8.885%
29	15.587	2119	2125	2139	rBV	1518451	2123727	18.65%	2.150%
30	15.710	2142	2146	2151	rVB3	30729	49426	0.43%	0.050%
31	16.392	2257	2262	2266	rBV7	10364	16018	0.14%	0.016%
32	16.904	2345	2349	2353	rVB2	9345	16731	0.15%	0.017%
33	17.010	2365	2367	2373	rVB4	9189	13355	0.12%	0.014%
34	17.228	2397	2404	2414	rBV	4212879	5967000	52.39%	6.042%
35	17.328	2414	2421	2436	rVV	7107505	10042422	88.18%	10.168%
36	17.898	2516	2518	2524	rBV5	7453	11430	0.10%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018594.D
Acq On : 05 Dec 2023 10:03
Operator : MA/JU
Sample : 05441-13
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	18.116	2551	2555	2561	rBV2	65727	89230	0.78%	0.090%
38	19.139	2725	2729	2734	rBV2	91819	123925	1.09%	0.125%
39	19.210	2736	2741	2746	rBV	82321	126145	1.11%	0.128%
40	19.351	2762	2765	2768	rBV4	36452	43544	0.38%	0.044%
41	19.563	2795	2801	2812	rBV	8730885	11388612	100.00%	11.531%
42	21.316	3094	3099	3107	rBV	4372764	5421385	47.60%	5.489%
43	23.533	3469	3476	3484	rBV2	4521155	8524934	74.85%	8.632%
44	23.686	3495	3502	3513	rVB	2393389	4748928	41.70%	4.808%




Sum of corrected areas: 98762255

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018594.D
Acq On : 05 Dec 2023 10:03
Operator : MA/JU
Sample : 05441-13
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

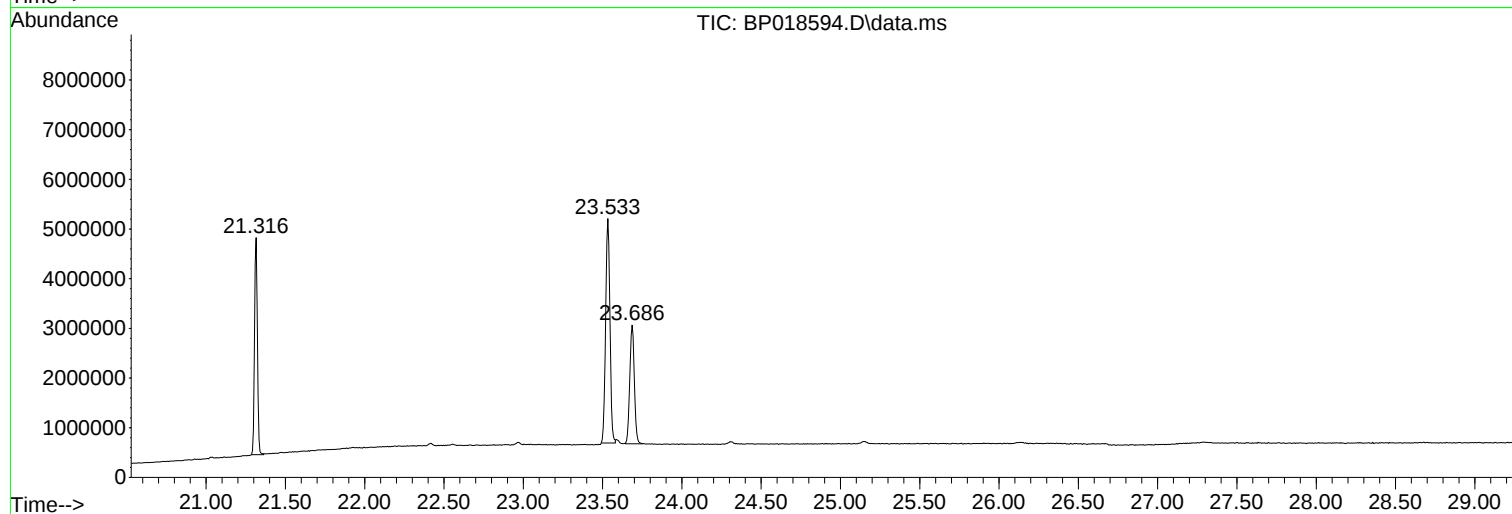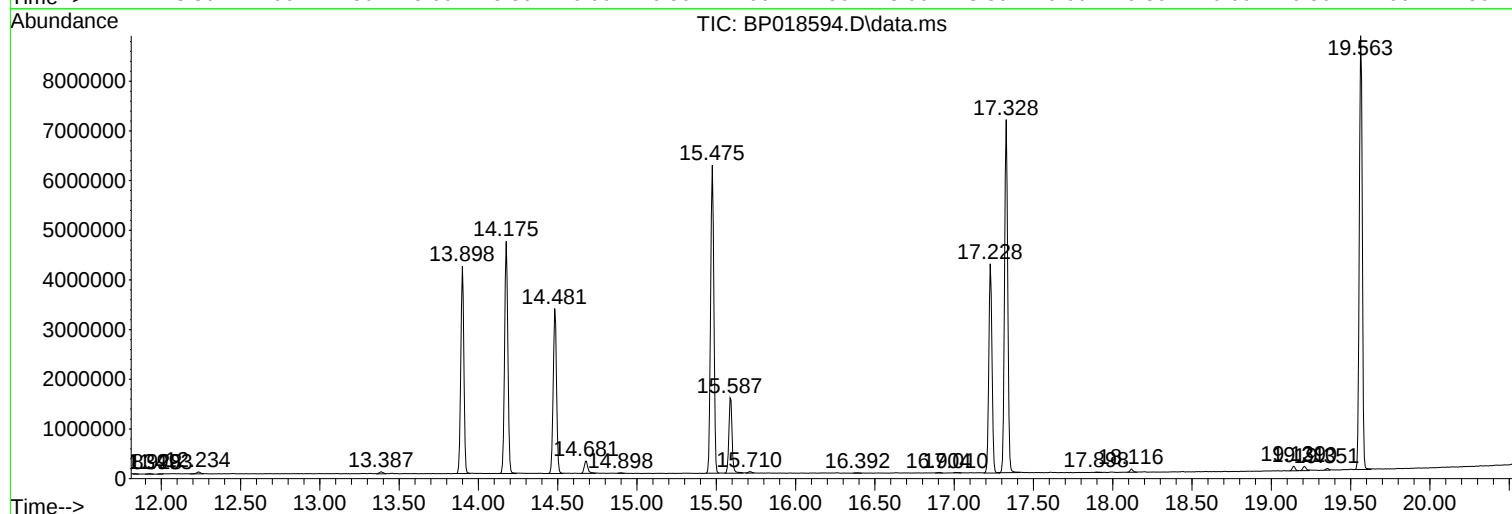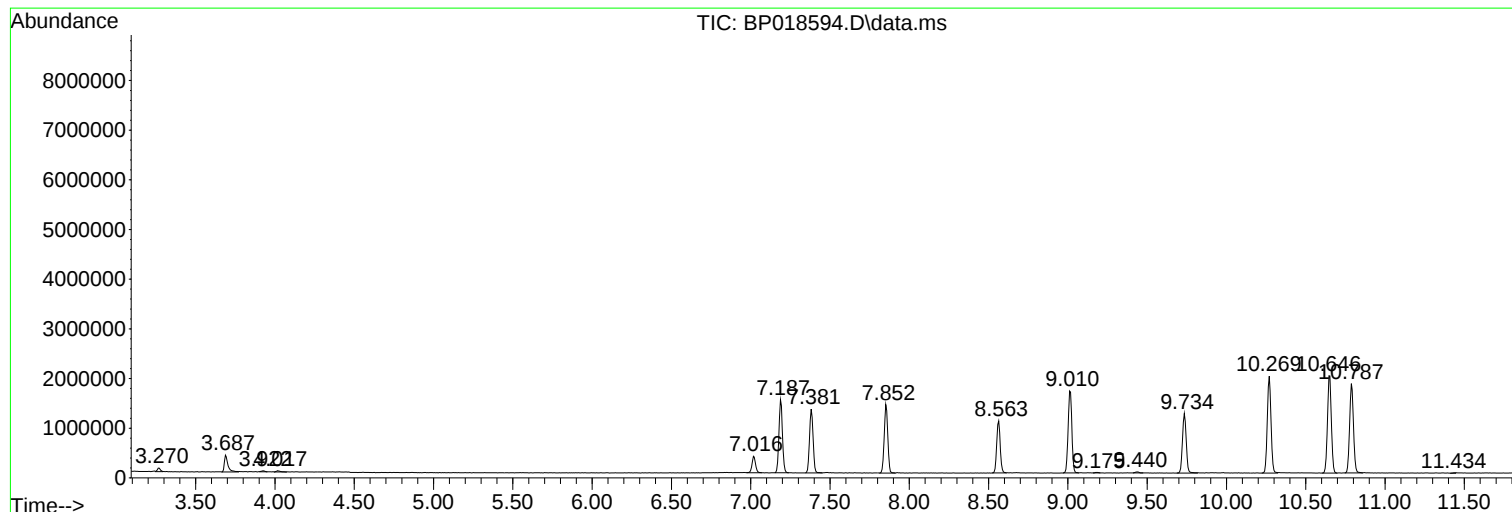

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018594.D
Acq On : 05 Dec 2023 10:03
Operator : MA/JU
Sample : 05441-13
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018594.D
Acq On : 05 Dec 2023 10:03
Operator : MA/JU
Sample : 05441-13
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc