

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018596.D
 Acq On : 05 Dec 2023 11:11
 Operator : MA/JU
 Sample : 05441-15
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018596.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	28	rBV	57593	76839	0.64%	0.079%
2	3.269	28	31	38	rVB	72879	97549	0.81%	0.100%
3	3.687	99	102	113	rBV	335332	504440	4.21%	0.517%
4	3.928	140	143	147	rVB2	22207	28508	0.24%	0.029%
5	4.016	155	158	163	rVB	19645	26389	0.22%	0.027%
6	7.016	662	668	679	rVB	349657	581253	4.85%	0.596%
7	7.187	691	697	706	rVB	1071599	1667375	13.92%	1.709%
8	7.381	722	730	738	rBV	972901	1508253	12.59%	1.546%
9	7.475	742	746	752	rBV3	9384	14175	0.12%	0.015%
10	7.852	802	810	818	rBV	1034752	1582123	13.21%	1.622%
11	8.563	924	931	939	rBV	855353	1339819	11.19%	1.374%
12	9.010	1000	1007	1016	rBV	1258846	2064603	17.24%	2.117%
13	9.181	1034	1036	1040	rVB3	10313	12132	0.10%	0.012%
14	9.434	1075	1079	1085	rVB2	16167	29663	0.25%	0.030%
15	9.640	1110	1114	1115	rBV2	13276	18256	0.15%	0.019%
16	9.734	1122	1130	1144	rBV	1171331	1871581	15.63%	1.919%
17	10.269	1213	1221	1233	rBV	1901770	3102948	25.91%	3.181%
18	10.651	1278	1286	1293	rBV	1842739	3064598	25.59%	3.142%
19	10.787	1301	1309	1319	rBV	1860647	3099113	25.88%	3.177%
20	12.234	1551	1555	1561	rVB2	37030	60567	0.51%	0.062%
21	13.387	1746	1751	1756	rBV3	34262	55511	0.46%	0.057%
22	13.451	1759	1762	1769	rVB4	9279	16495	0.14%	0.017%
23	13.898	1831	1838	1845	rBV	4395591	6028424	50.33%	6.181%
24	14.175	1878	1885	1895	rBV	4808949	6732938	56.21%	6.903%
25	14.481	1930	1937	1947	rVB	3241412	4651406	38.84%	4.769%
26	14.675	1965	1970	1983	rBV	314196	481771	4.02%	0.494%
27	14.904	2005	2009	2013	rVB4	19857	28470	0.24%	0.029%
28	15.475	2098	2106	2118	rBV	6673084	9339154	77.97%	9.575%
29	15.586	2120	2125	2141	rVV	1727636	2424740	20.24%	2.486%
30	15.716	2143	2147	2154	rVB5	32143	52139	0.44%	0.053%
31	17.228	2398	2404	2413	rVB	3941965	5608620	46.83%	5.750%
32	17.328	2414	2421	2430	rBV2	7598787	10694133	89.29%	10.964%
33	18.116	2551	2555	2562	rBV	160808	212100	1.77%	0.217%
34	19.139	2725	2729	2736	rBV2	92434	120951	1.01%	0.124%
35	19.210	2736	2741	2745	rBV	92330	133993	1.12%	0.137%
36	19.351	2762	2765	2772	rBV2	92466	115796	0.97%	0.119%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018596.D
Acq On : 05 Dec 2023 11:11
Operator : MA/JU
Sample : 05441-15
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.563	2795	2801	2808	rBV	9064823	11977224	100.00%	12.280%
38	21.316	3094	3099	3105	rBV	3965897	4844494	40.45%	4.967%
39	23.533	3469	3476	3491	rVB2	4554221	8901010	74.32%	9.126%
40	23.686	3495	3502	3514	rVB	2264334	4367576	36.47%	4.478%




Sum of corrected areas: 97537129

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018596.D
Acq On : 05 Dec 2023 11:11
Operator : MA/JU
Sample : 05441-15
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

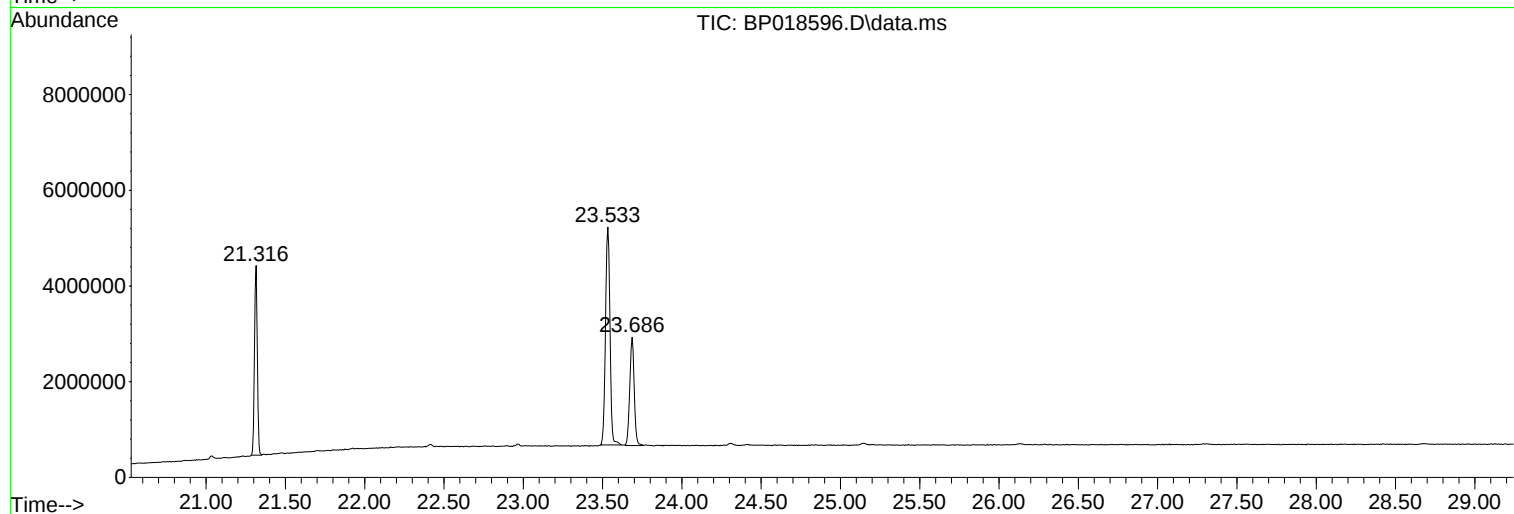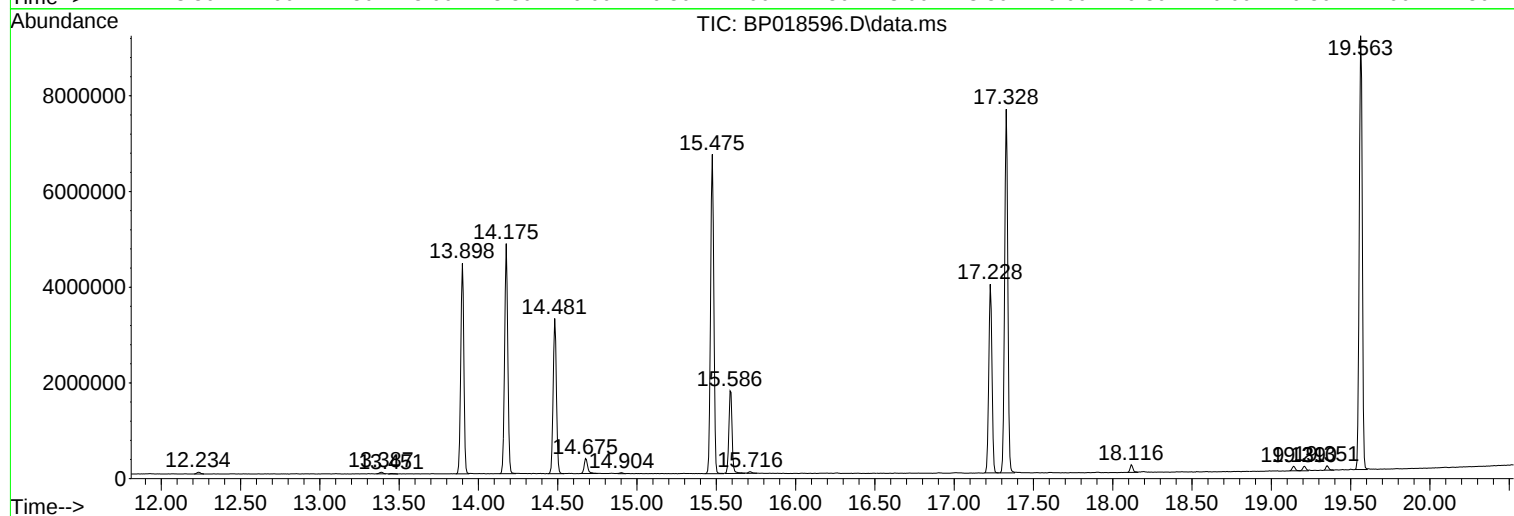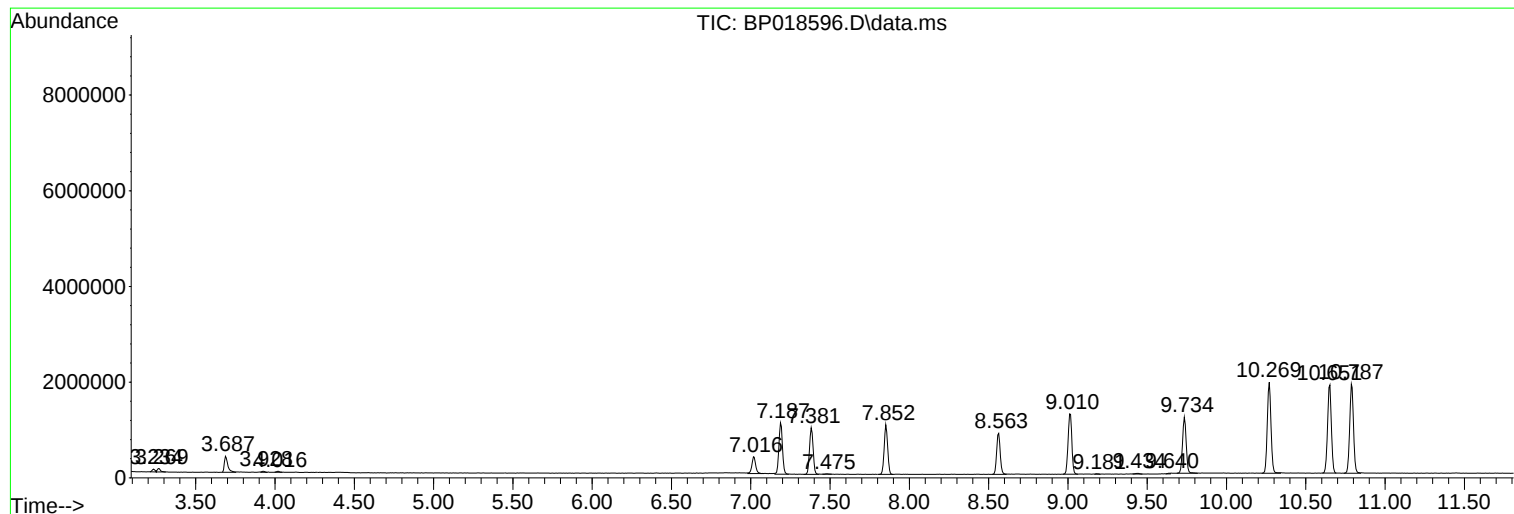

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018596.D
Acq On : 05 Dec 2023 11:11
Operator : MA/JU
Sample : 05441-15
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018596.D
Acq On : 05 Dec 2023 11:11
Operator : MA/JU
Sample : 05441-15
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc