

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018597.D
 Acq On : 05 Dec 2023 11:44
 Operator : MA/JU
 Sample : 05441-16
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018597.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	22	24	28	rBV5	16331	24546	0.20%	0.025%
2	3.270	28	31	35	rVB	71186	85311	0.68%	0.086%
3	3.546	75	78	88	rBV	99455	144283	1.15%	0.146%
4	3.687	99	102	115	rBV	295957	461616	3.67%	0.468%
5	3.923	139	142	148	rVB2	18407	27819	0.22%	0.028%
6	4.023	155	159	166	rBV2	19371	30208	0.24%	0.031%
7	6.699	608	614	615	rBV	9088	13761	0.11%	0.014%
8	7.016	662	668	678	rVB	329323	507594	4.04%	0.514%
9	7.187	691	697	706	rVB	1456408	2239830	17.83%	2.270%
10	7.381	723	730	741	rBV	1276660	1953045	15.54%	1.979%
11	7.481	743	747	751	rVB5	8580	16544	0.13%	0.017%
12	7.852	803	810	818	rBV	1073392	1677491	13.35%	1.700%
13	8.563	923	931	942	rBV	1047307	1643956	13.08%	1.666%
14	9.010	1000	1007	1016	rBV	1677950	2686149	21.38%	2.722%
15	9.187	1032	1037	1041	rVB4	14064	23139	0.18%	0.023%
16	9.434	1076	1079	1085	rVB3	12178	21562	0.17%	0.022%
17	9.734	1122	1130	1145	rBV	1248452	1998924	15.91%	2.026%
18	10.269	1211	1221	1229	rBV	1826887	2986275	23.77%	3.026%
19	10.652	1276	1286	1293	rBV	1493436	2597694	20.67%	2.632%
20	10.787	1302	1309	1320	rBV	1543588	2541513	20.23%	2.575%
21	12.234	1550	1555	1561	rVB3	39230	65234	0.52%	0.066%
22	13.387	1746	1751	1755	rVB2	28746	41603	0.33%	0.042%
23	13.898	1831	1838	1845	rBV	4530062	6258153	49.81%	6.342%
24	14.175	1878	1885	1894	rBV	5036669	7172022	57.08%	7.268%
25	14.481	1930	1937	1946	rVB	2667732	3874658	30.84%	3.926%
26	14.675	1965	1970	1980	rBV2	307062	467318	3.72%	0.474%
27	14.898	2004	2008	2013	rVB5	14290	26230	0.21%	0.027%
28	15.475	2099	2106	2112	rBV	6874791	9569672	76.16%	9.697%
29	15.587	2119	2125	2137	rBV	1921722	2613508	20.80%	2.648%
30	15.710	2142	2146	2155	rVB3	32530	57116	0.45%	0.058%
31	16.257	2236	2239	2243	rVB2	12264	17103	0.14%	0.017%
32	16.904	2347	2349	2355	rVB6	12756	14658	0.12%	0.015%
33	17.228	2398	2404	2414	rBV	3241949	4635927	36.90%	4.698%
34	17.328	2414	2421	2432	rBV2	7990554	11360058	90.41%	11.511%
35	17.904	2516	2519	2524	rVB3	13650	18352	0.15%	0.019%
36	18.116	2551	2555	2559	rBV	106103	120146	0.96%	0.122%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018597.D
Acq On : 05 Dec 2023 11:44
Operator : MA/JU
Sample : 05441-16
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.139	2725	2729	2735	rVB2	98042	127919	1.02%	0.130%
38	19.204	2736	2740	2744	rBV	94513	125330	1.00%	0.127%
39	19.351	2762	2765	2770	rBV4	60166	73199	0.58%	0.074%
40	19.563	2795	2801	2808	rBV	9881662	12564808	100.00%	12.732%
41	21.316	3094	3099	3106	rBV	3137721	4030252	32.08%	4.084%
42	23.533	3469	3476	3493	rVB2	5228636	9994706	79.55%	10.128%
43	23.680	3495	3501	3514	rVB	1856114	3776148	30.05%	3.826%




Sum of corrected areas: 98685380

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018597.D
Acq On : 05 Dec 2023 11:44
Operator : MA/JU
Sample : 05441-16
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

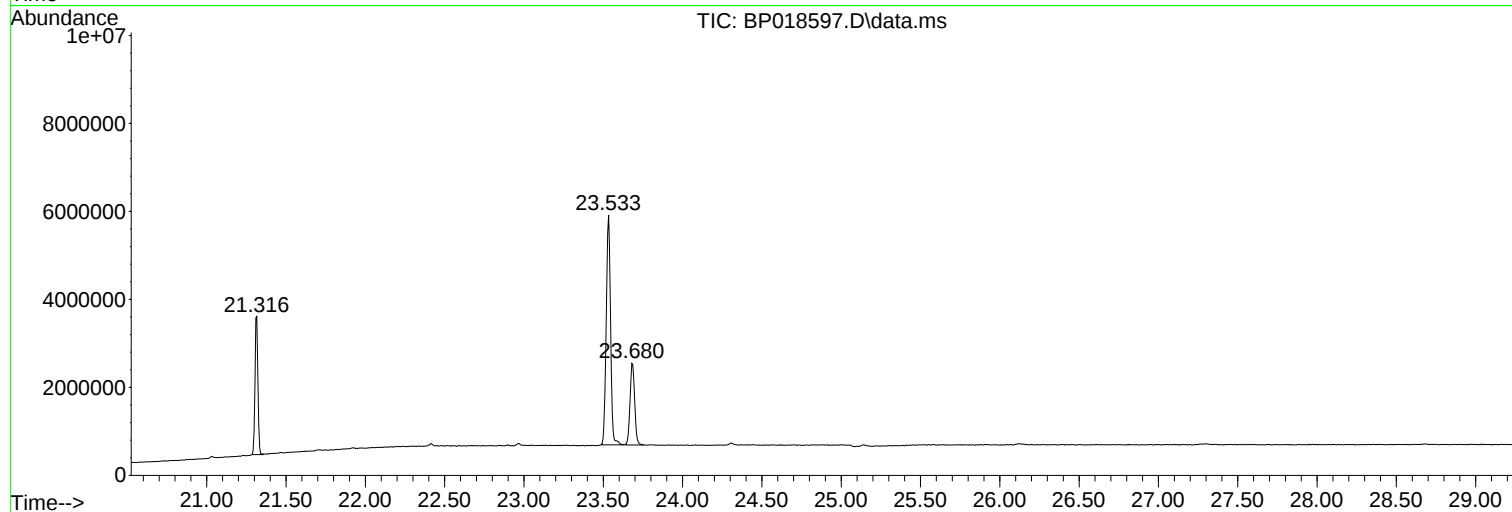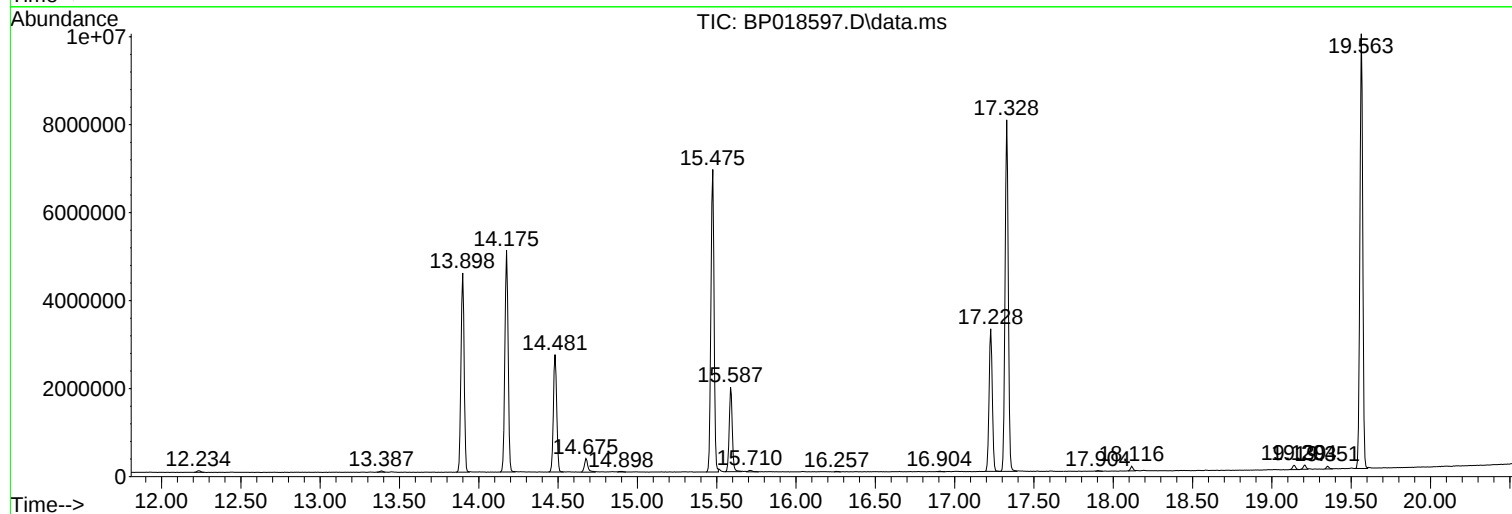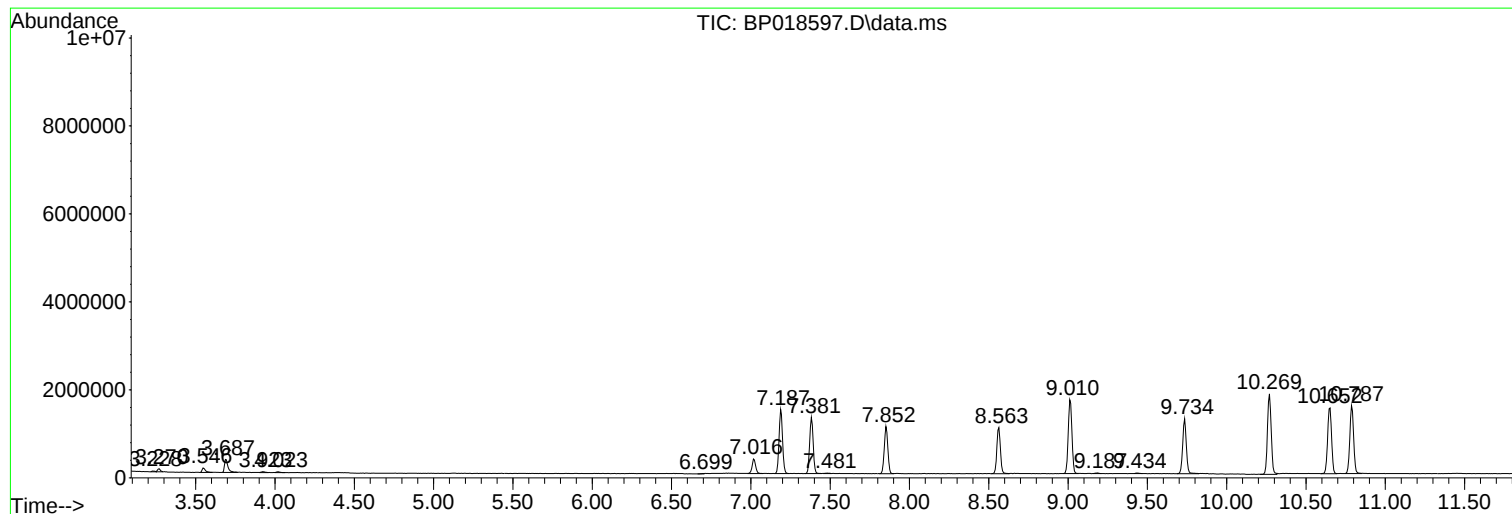

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018597.D
Acq On : 05 Dec 2023 11:44
Operator : MA/JU
Sample : 05441-16
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018597.D
Acq On : 05 Dec 2023 11:44
Operator : MA/JU
Sample : 05441-16
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc