

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018598.D
 Acq On : 05 Dec 2023 12:19
 Operator : MA/JU
 Sample : 05441-17
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QK7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018598.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	20	25	36	rBV2	533696	857248	6.75%	0.852%
2	3.558	77	80	85	rVB2	15427	21144	0.17%	0.021%
3	3.687	98	102	116	rBV	473153	718942	5.66%	0.714%
4	4.017	156	158	163	rVB2	18431	25735	0.20%	0.026%
5	7.016	662	668	676	rVB	277685	444450	3.50%	0.442%
6	7.187	691	697	706	rVB	1478874	2245857	17.69%	2.232%
7	7.381	723	730	741	rBV	1215057	1853419	14.60%	1.842%
8	7.475	743	746	751	rVB4	12492	16254	0.13%	0.016%
9	7.852	802	810	817	rBV	913116	1394857	10.98%	1.386%
10	8.563	924	931	939	rBV	776328	1211596	9.54%	1.204%
11	9.010	999	1007	1015	rBV	1359038	2188707	17.24%	2.175%
12	9.434	1075	1079	1085	rVB2	15134	25463	0.20%	0.025%
13	9.734	1122	1130	1142	rBV	1040433	1658919	13.06%	1.648%
14	10.140	1192	1199	1200	rBV	15532	24472	0.19%	0.024%
15	10.269	1214	1221	1233	rBV	1963242	3164796	24.92%	3.145%
16	10.651	1278	1286	1293	rVB	1626858	2703180	21.29%	2.686%
17	10.787	1302	1309	1323	rBV	1539552	2545595	20.05%	2.529%
18	11.463	1418	1424	1430	rBV6	9461	23583	0.19%	0.023%
19	12.234	1549	1555	1561	rBV2	38695	67574	0.53%	0.067%
20	13.316	1735	1739	1742	rBV2	15075	19317	0.15%	0.019%
21	13.387	1746	1751	1758	rVV	46435	73529	0.58%	0.073%
22	13.898	1832	1838	1847	rBV	4434789	6003550	47.28%	5.965%
23	14.175	1878	1885	1895	rBV	5062987	7120088	56.07%	7.075%
24	14.481	1930	1937	1949	rBV	2806329	4076890	32.11%	4.051%
25	14.675	1965	1970	1978	rBV2	227716	356775	2.81%	0.355%
26	14.898	2004	2008	2015	rVB6	16647	29138	0.23%	0.029%
27	15.475	2099	2106	2111	rBV	6598922	9477208	74.63%	9.417%
28	15.510	2111	2112	2118	rVB	111644	122282	0.96%	0.122%
29	15.592	2119	2126	2135	rBV	1668794	2337990	18.41%	2.323%
30	15.710	2143	2146	2152	rVB	32313	49398	0.39%	0.049%
31	17.228	2398	2404	2412	rBV	3573665	5080149	40.01%	5.048%
32	17.328	2414	2421	2431	rBV	7612817	10888161	85.74%	10.819%
33	18.122	2551	2556	2562	rBV	376015	507548	4.00%	0.504%
34	19.139	2725	2729	2736	rBV3	100247	140248	1.10%	0.139%
35	19.210	2737	2741	2745	rBV	102629	135211	1.06%	0.134%
36	19.351	2761	2765	2773	rBV3	117309	170056	1.34%	0.169%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018598.D
Acq On : 05 Dec 2023 12:19
Operator : MA/JU
Sample : 05441-17
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.563	2795	2801	2808	rBV	9472779	12698586	100.00%	12.618%
38	21.033	3047	3051	3062	rBV2	215639	430968	3.39%	0.428%
39	21.316	3094	3099	3106	rBV	3926942	4968850	39.13%	4.937%
40	23.533	3468	3476	3483	rBV	5347167	10306985	81.17%	10.242%
41	23.686	3495	3502	3511	rVB	2294729	4454592	35.08%	4.426%




Sum of corrected areas: 100639310

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018598.D
Acq On : 05 Dec 2023 12:19
Operator : MA/JU
Sample : 05441-17
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

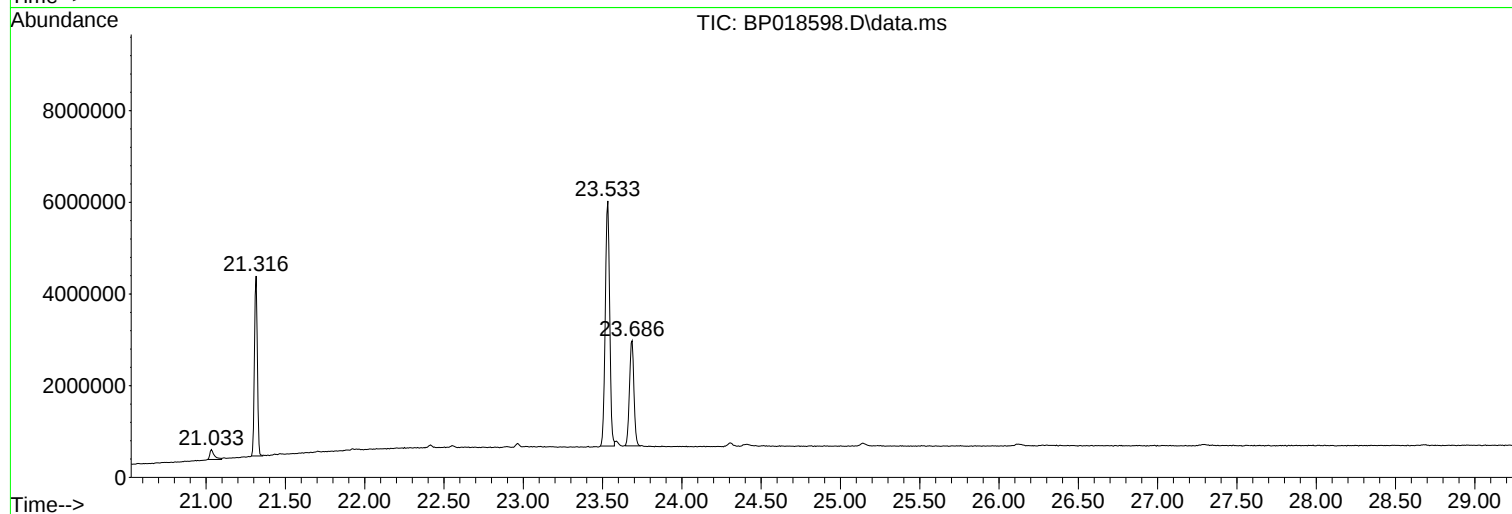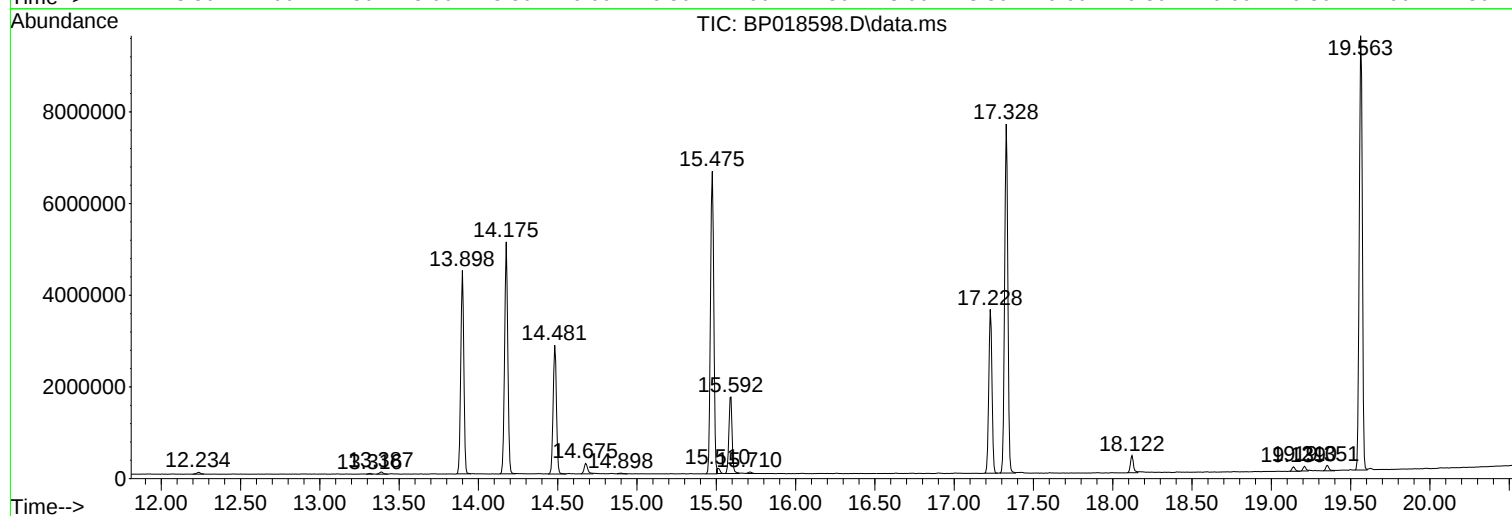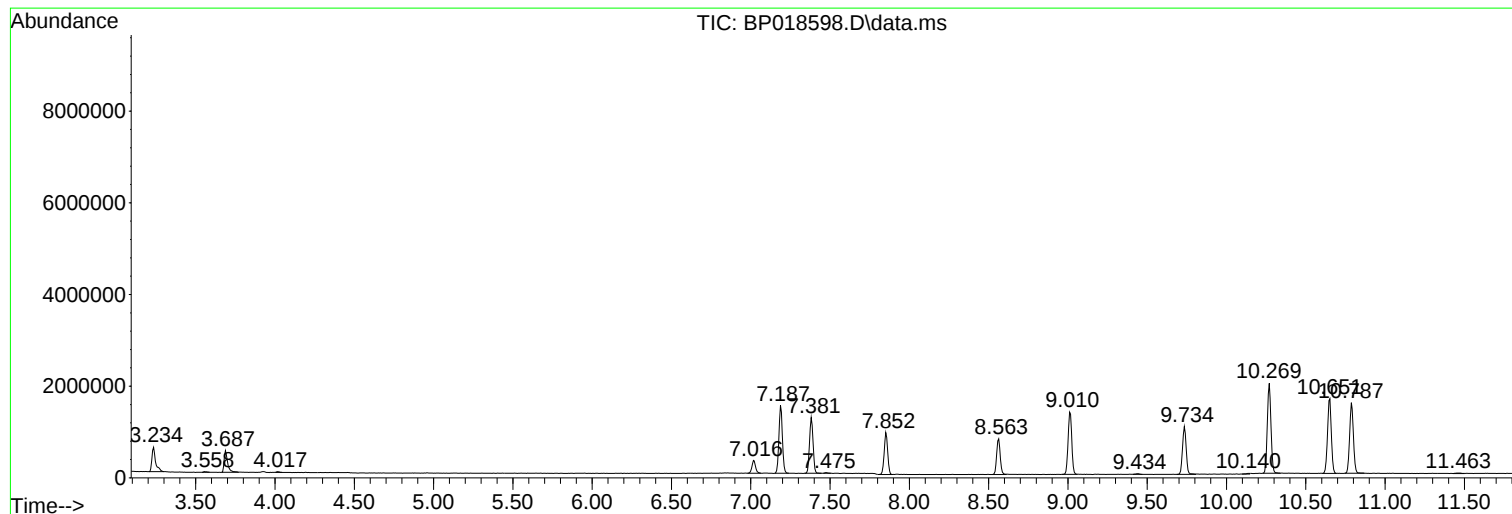

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018598.D
Acq On : 05 Dec 2023 12:19
Operator : MA/JU
Sample : 05441-17
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018598.D
Acq On : 05 Dec 2023 12:19
Operator : MA/JU
Sample : 05441-17
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
