

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018599.D
 Acq On : 05 Dec 2023 12:52
 Operator : MA/JU
 Sample : 05441-18
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018599.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	28	rBV2	63239	89648	0.77%	0.094%
2	3.264	28	30	37	rVB	69775	95845	0.82%	0.101%
3	3.687	98	102	115	rBV	373506	558568	4.80%	0.588%
4	3.922	140	142	148	rVB	18030	21614	0.19%	0.023%
5	4.017	155	158	163	rVB2	20352	28760	0.25%	0.030%
6	4.552	245	249	253	rVB3	10871	17275	0.15%	0.018%
7	7.016	659	668	678	rBV	281019	466317	4.01%	0.491%
8	7.187	691	697	705	rBV	1375213	2105390	18.11%	2.217%
9	7.381	723	730	738	rBV	1144869	1753817	15.08%	1.847%
10	7.852	803	810	819	rVB	1116419	1760317	15.14%	1.854%
11	8.563	923	931	941	rBV	910056	1420202	12.21%	1.496%
12	8.681	949	951	958	rVB	9604	14596	0.13%	0.015%
13	8.846	972	979	983	rBV2	10609	28167	0.24%	0.030%
14	9.010	1000	1007	1016	rBV	1563271	2513691	21.62%	2.647%
15	9.440	1073	1080	1084	rVB2	34500	55441	0.48%	0.058%
16	9.734	1123	1130	1142	rBV	1129662	1782929	15.33%	1.878%
17	10.269	1212	1221	1232	rBV	1792406	2933011	25.22%	3.089%
18	10.652	1278	1286	1293	rVB	1608168	2733195	23.51%	2.878%
19	10.787	1301	1309	1322	rBV	1850371	3057551	26.30%	3.220%
20	11.928	1498	1503	1509	rVB2	41483	66142	0.57%	0.070%
21	12.234	1550	1555	1560	rBV2	37947	60529	0.52%	0.064%
22	13.316	1736	1739	1744	rVB3	10492	15604	0.13%	0.016%
23	13.387	1746	1751	1758	rVB2	33244	55507	0.48%	0.058%
24	13.451	1758	1762	1766	rBV4	10359	14817	0.13%	0.016%
25	13.898	1832	1838	1848	rBV	4145643	5550615	47.74%	5.845%
26	14.175	1878	1885	1894	rBV	4542441	6615503	56.89%	6.967%
27	14.393	1917	1922	1926	rVV3	5471	12839	0.11%	0.014%
28	14.481	1930	1937	1950	rBV	2646830	3875738	33.33%	4.082%
29	14.675	1964	1970	1977	rBV	202440	334485	2.88%	0.352%
30	14.904	2004	2009	2013	rBV7	10045	18688	0.16%	0.020%
31	15.404	2089	2094	2097	rBV2	8358	18525	0.16%	0.020%
32	15.475	2099	2106	2115	rVV	6349639	8890644	76.46%	9.363%
33	15.587	2119	2125	2139	rVV	1544158	2141873	18.42%	2.256%
34	15.716	2142	2147	2156	rVB2	30888	59228	0.51%	0.062%
35	16.910	2346	2350	2355	rBV4	12086	16338	0.14%	0.017%
36	17.228	2398	2404	2413	rBV	3748955	5150529	44.30%	5.424%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018599.D
 Acq On : 05 Dec 2023 12:52
 Operator : MA/JU
 Sample : 05441-18
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.328	2414	2421	2432	rBV2	7174337	10153629	87.32%	10.693%
38	18.116	2551	2555	2564	rBV2	81070	108623	0.93%	0.114%
39	19.139	2725	2729	2734	rBV3	83600	111762	0.96%	0.118%
40	19.210	2736	2741	2745	rBV	82548	125667	1.08%	0.132%
41	19.351	2762	2765	2769	rBV6	37098	45409	0.39%	0.048%
42	19.563	2795	2801	2813	rBV	8957255	11627666	100.00%	12.245%
43	21.033	3048	3051	3058	rBV3	58581	100347	0.86%	0.106%
44	21.316	3094	3099	3106	rBV	3990276	4837953	41.61%	5.095%
45	23.533	3468	3476	3490	rVB	4577537	9195129	79.08%	9.684%
46	23.680	3495	3501	3510	rVB	2196774	4315644	37.12%	4.545%




Sum of corrected areas: 94955767

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018599.D
Acq On : 05 Dec 2023 12:52
Operator : MA/JU
Sample : 05441-18
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

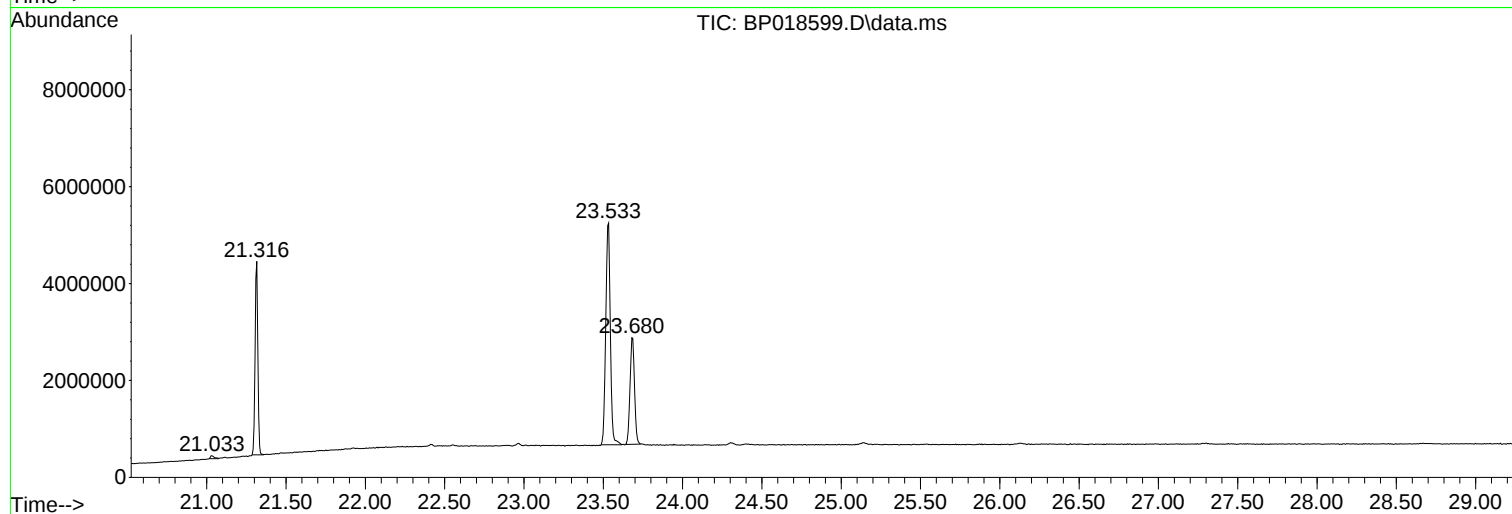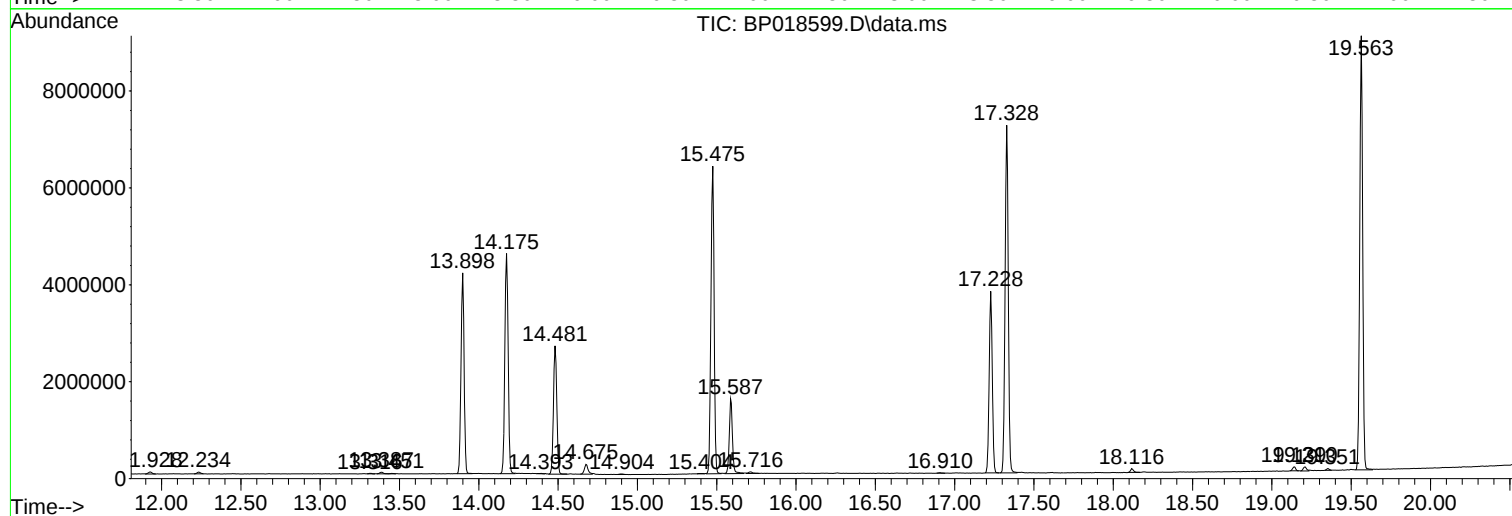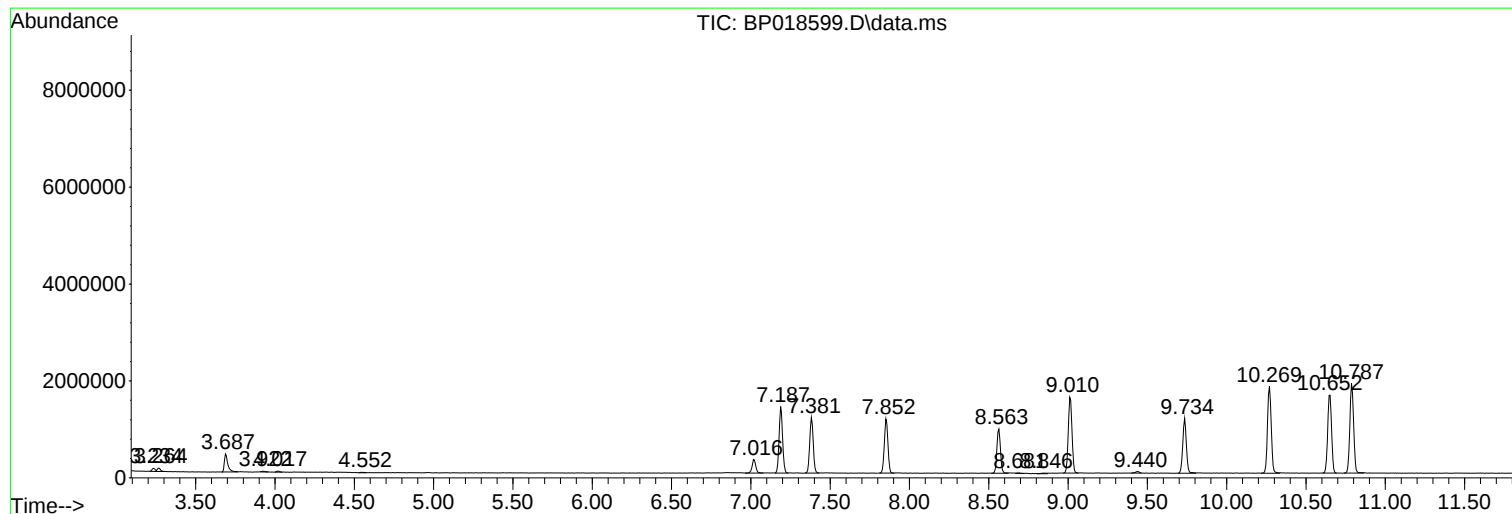

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018599.D
Acq On : 05 Dec 2023 12:52
Operator : MA/JU
Sample : 05441-18
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018599.D
Acq On : 05 Dec 2023 12:52
Operator : MA/JU
Sample : 05441-18
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc