

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018600.D
 Acq On : 05 Dec 2023 13:26
 Operator : MA/JU
 Sample : 05441-19
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QL1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018600.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	28	rBV	71701	97234	0.73%	0.092%
2	3.264	28	30	34	rVB	62836	75435	0.57%	0.071%
3	3.687	99	102	116	rBV	404949	637506	4.81%	0.601%
4	3.923	140	142	148	rVB2	20385	23469	0.18%	0.022%
5	4.017	155	158	164	rVB	18419	26108	0.20%	0.025%
6	6.717	616	617	625	rVB	13653	20385	0.15%	0.019%
7	7.017	660	668	679	rBV	313433	502611	3.79%	0.474%
8	7.187	691	697	707	rBV	1507630	2347572	17.71%	2.212%
9	7.381	722	730	740	rBV	1314063	2022452	15.26%	1.906%
10	7.852	802	810	820	rBV	1212549	1885769	14.23%	1.777%
11	8.564	924	931	941	rBV	1041483	1623862	12.25%	1.530%
12	9.011	1000	1007	1016	rBV	1748733	2818181	21.27%	2.655%
13	9.434	1074	1079	1086	rVB2	52807	87310	0.66%	0.082%
14	9.734	1122	1130	1140	rBV	1254034	2006563	15.14%	1.891%
15	10.269	1213	1221	1232	rBV	2013096	3292978	24.85%	3.103%
16	10.652	1278	1286	1295	rVB	1708427	2930285	22.11%	2.761%
17	10.787	1302	1309	1318	rBV	2021139	3368232	25.42%	3.174%
18	11.928	1498	1503	1508	rVB	85386	130740	0.99%	0.123%
19	12.234	1549	1555	1560	rBV2	43197	70424	0.53%	0.066%
20	13.387	1746	1751	1756	rBV2	36468	55422	0.42%	0.052%
21	13.899	1831	1838	1846	rBV	4729813	6263413	47.26%	5.901%
22	14.175	1878	1885	1895	rBV	5024088	7347606	55.44%	6.923%
23	14.481	1930	1937	1948	rVB	3064317	4384766	33.09%	4.131%
24	14.675	1965	1970	1981	rBV	285712	442605	3.34%	0.417%
25	14.898	2004	2008	2013	rVB6	11858	22831	0.17%	0.022%
26	15.475	2099	2106	2113	rBV	6763902	9829563	74.17%	9.262%
27	15.587	2119	2125	2138	rBV	1804801	2470452	18.64%	2.328%
28	15.710	2143	2146	2151	rVB2	33501	46980	0.35%	0.044%
29	17.228	2397	2404	2412	rBV	4037581	5537542	41.78%	5.218%
30	17.328	2414	2421	2435	rBV	8002018	11286799	85.17%	10.635%
31	18.116	2551	2555	2561	rBV2	74713	92499	0.70%	0.087%
32	19.139	2725	2729	2734	rBV2	100121	126270	0.95%	0.119%
33	19.204	2736	2740	2744	rBV	93700	129558	0.98%	0.122%
34	19.351	2762	2765	2769	rBV3	41617	50211	0.38%	0.047%
35	19.563	2795	2801	2811	rBV	10274755	13252541	100.00%	12.487%
36	21.316	3093	3099	3105	rBV	4269926	5394463	40.71%	5.083%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018600.D
Acq On : 05 Dec 2023 13:26
Operator : MA/JU
Sample : 05441-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QL1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	23.533	3468	3476	3485	rBV2	5479845	10669896	80.51%	10.053%
38	23.686	3495	3502	3511	rVB	2442049	4762769	35.94%	4.488%




Sum of corrected areas: 106133302

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018600.D
Acq On : 05 Dec 2023 13:26
Operator : MA/JU
Sample : 05441-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QL1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

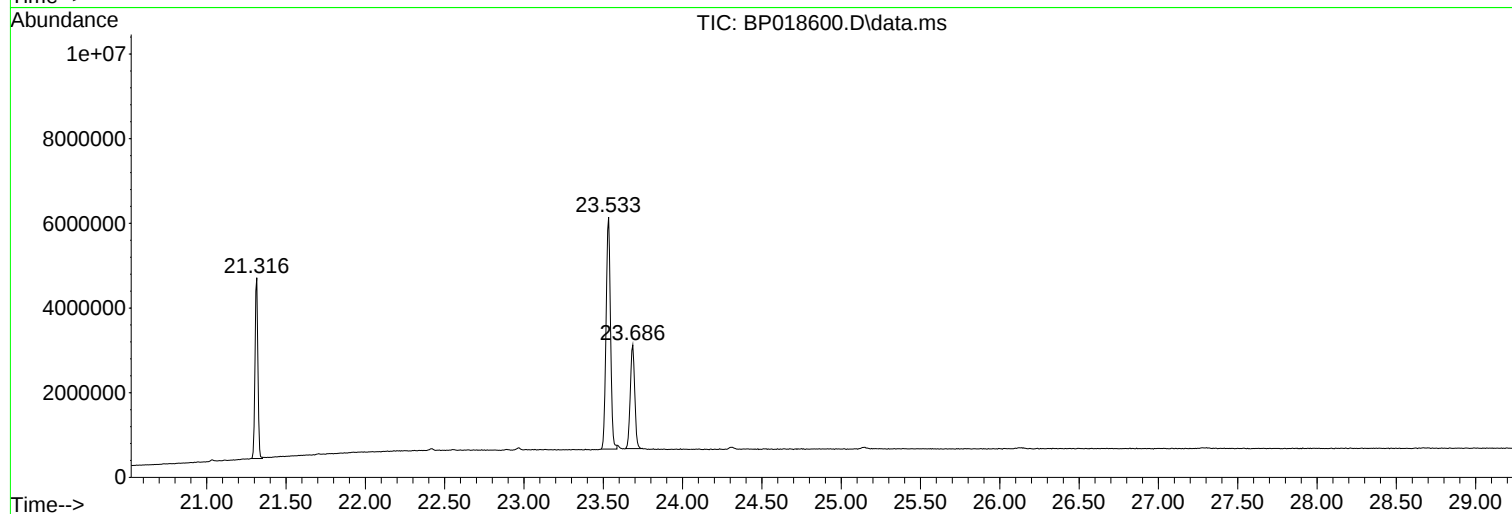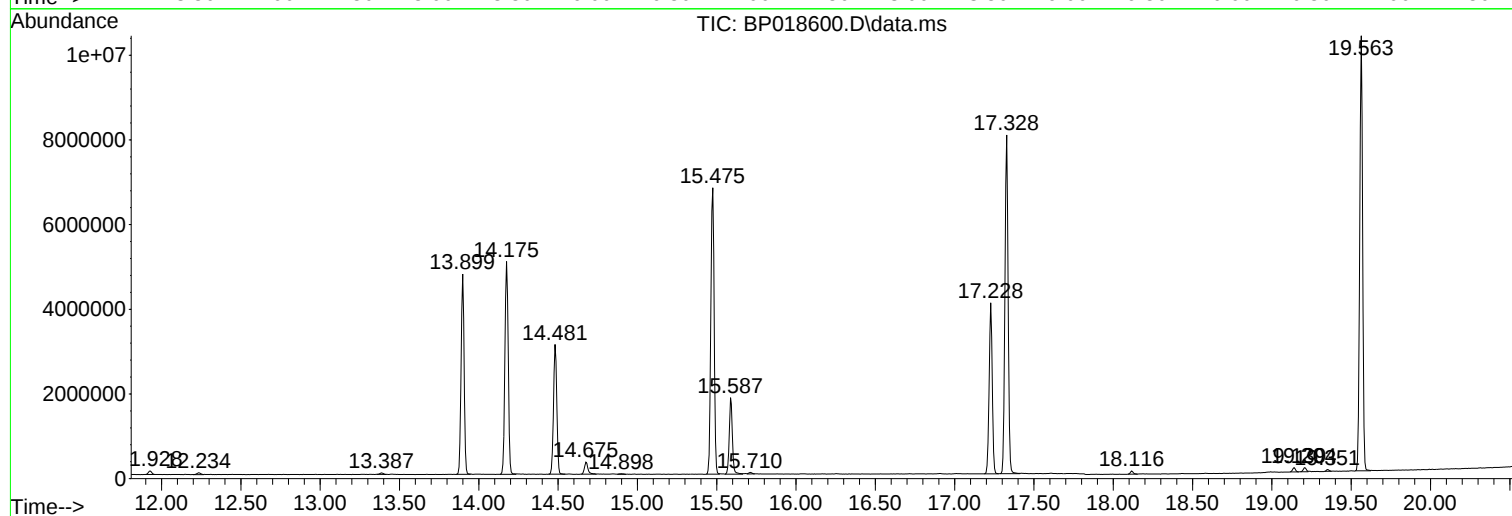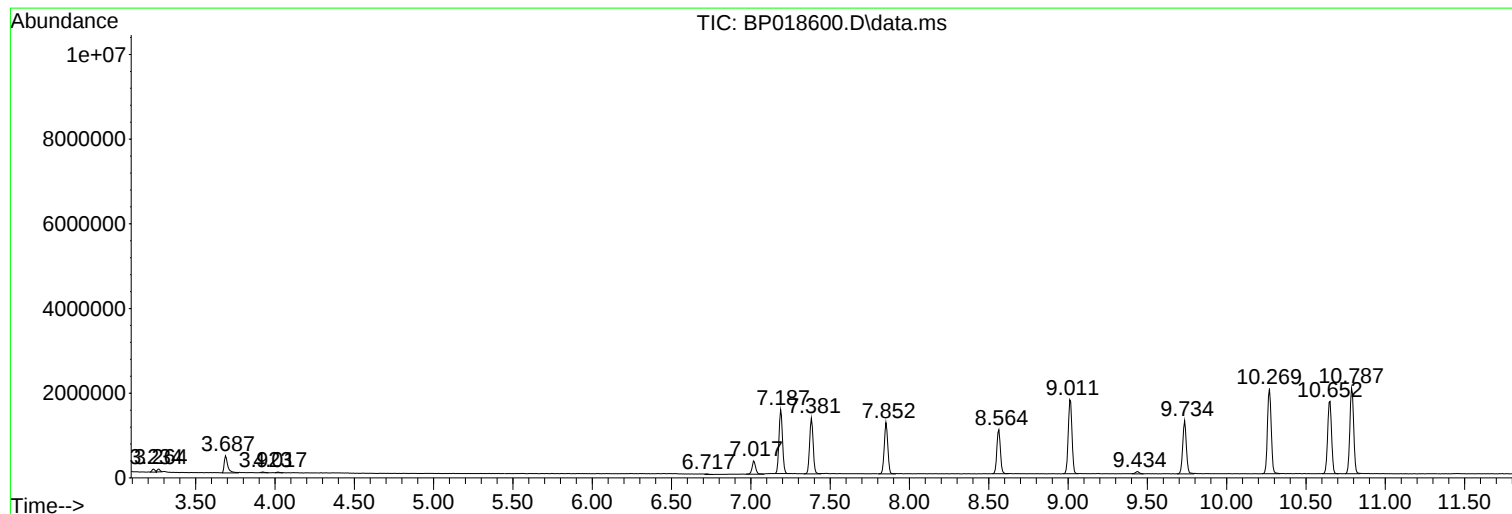

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018600.D
Acq On : 05 Dec 2023 13:26
Operator : MA/JU
Sample : 05441-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QL1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018600.D
Acq On : 05 Dec 2023 13:26
Operator : MA/JU
Sample : 05441-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QL1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
