

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018608.D
 Acq On : 05 Dec 2023 17:58
 Operator : MA/JU
 Sample : PB157366BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK366

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018608.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	37	rVB	122561	156492	1.18%	0.126%
2	3.687	98	102	118	rBV	1556795	2327412	17.49%	1.869%
3	4.016	155	158	164	rVB	24429	35870	0.27%	0.029%
4	7.016	662	668	678	rVB	1861232	2952092	22.18%	2.371%
5	7.187	691	697	709	rVB	1622175	2523673	18.96%	2.027%
6	7.381	723	730	739	rBV	1870589	2933791	22.04%	2.356%
7	7.851	803	810	820	rBV	1414682	2174446	16.34%	1.746%
8	8.563	924	931	941	rBV	2477072	3909152	29.37%	3.139%
9	9.016	1000	1008	1019	rBV	1822340	3038700	22.83%	2.440%
10	9.734	1123	1130	1141	rBV	1499407	2380159	17.88%	1.911%
11	10.269	1213	1221	1235	rBV	2489587	4087829	30.71%	3.283%
12	10.645	1274	1285	1293	rBV	1821015	3104710	23.32%	2.493%
13	10.787	1301	1309	1321	rBV	1580595	2689679	20.21%	2.160%
14	12.234	1550	1555	1564	rBV	41482	66343	0.50%	0.053%
15	12.557	1604	1610	1612	rBV	7930	14663	0.11%	0.012%
16	12.598	1612	1617	1618	rBV	10383	14261	0.11%	0.011%
17	13.386	1747	1751	1755	rBV3	33934	50774	0.38%	0.041%
18	13.898	1831	1838	1849	rBV	5054189	7033003	52.84%	5.648%
19	14.175	1878	1885	1896	rBV2	5402255	8181255	61.46%	6.570%
20	14.481	1930	1937	1945	rBV	3483952	5212917	39.16%	4.186%
21	14.681	1964	1971	1984	rBV	2355605	3335649	25.06%	2.679%
22	15.475	2099	2106	2113	rBV	7611321	10555129	79.30%	8.476%
23	15.586	2119	2125	2138	rBV	2019026	2772529	20.83%	2.226%
24	15.716	2143	2147	2152	rVB3	33264	51109	0.38%	0.041%
25	17.227	2397	2404	2414	rBV	4780106	6516704	48.96%	5.233%
26	17.327	2414	2421	2434	rBV	8366471	11580163	87.00%	9.299%
27	18.116	2553	2555	2559	rVB4	16177	16950	0.13%	0.014%
28	19.139	2725	2729	2735	rBV	109721	132540	1.00%	0.106%
29	19.204	2736	2740	2748	rBV	99516	146245	1.10%	0.117%
30	19.563	2795	2801	2808	rBV	10137652	13310695	100.00%	10.689%
31	21.315	3093	3099	3108	rBV	4900922	6314781	47.44%	5.071%
32	23.533	3468	3476	3483	rBV	5695474	11022585	82.81%	8.852%
33	23.686	3495	3502	3514	rVB	2991537	5885402	44.22%	4.726%




Sum of corrected areas: 124527702

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018608.D
Acq On : 05 Dec 2023 17:58
Operator : MA/JU
Sample : PB157366BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK366

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

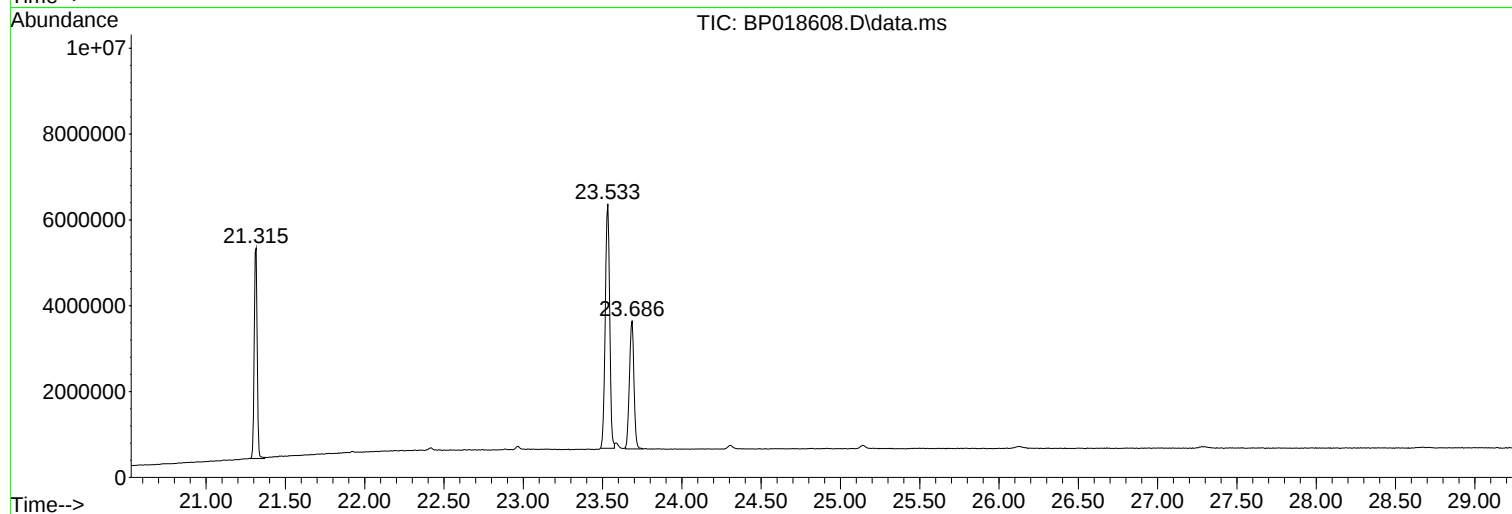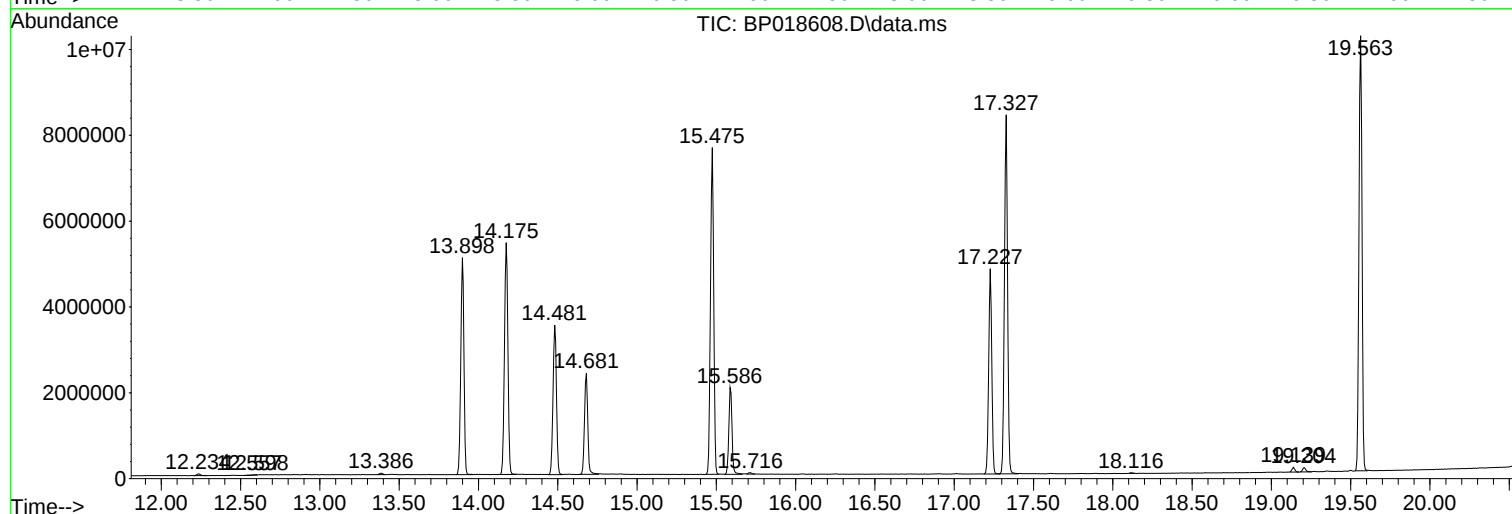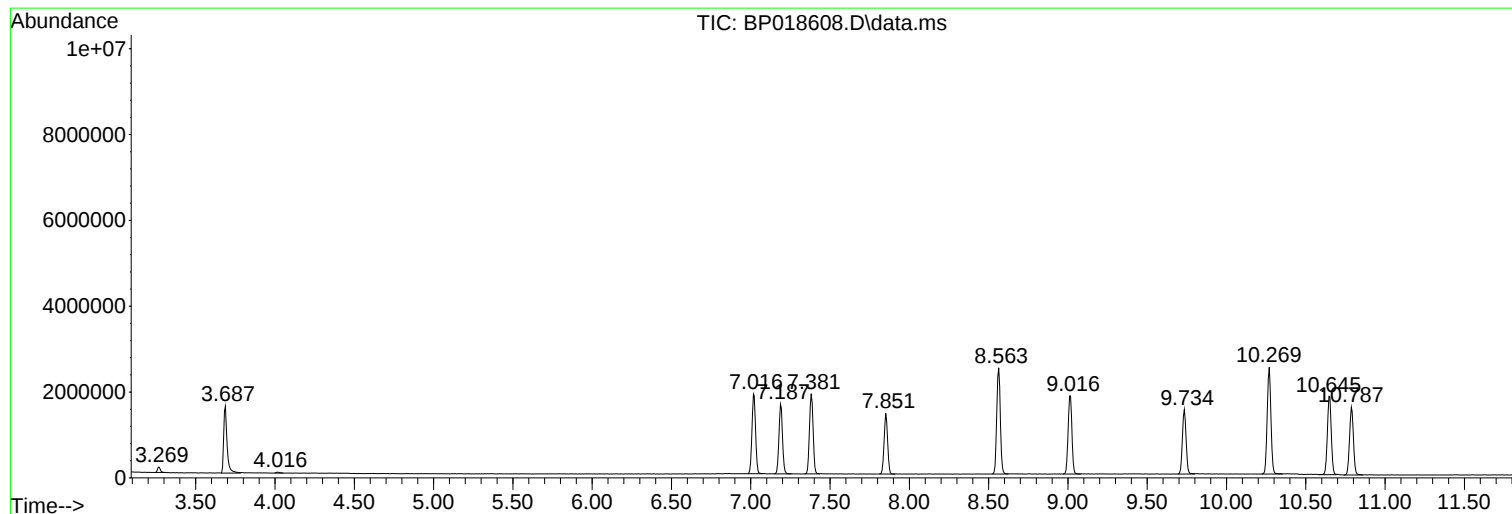

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018608.D
Acq On : 05 Dec 2023 17:58
Operator : MA/JU
Sample : PB157366BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK366

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018608.D
Acq On : 05 Dec 2023 17:58
Operator : MA/JU
Sample : PB157366BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK366

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc