

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018609.D
 Acq On : 05 Dec 2023 18:32
 Operator : MA/JU
 Sample : PB157355BL
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK355

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018609.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	41	rVB	106679	160349	1.42%	0.149%
2	3.681	97	101	119	rBV	1264077	2013067	17.86%	1.866%
3	4.017	155	158	162	rVB	16935	20367	0.18%	0.019%
4	7.016	661	668	679	rVB	1621667	2517957	22.34%	2.334%
5	7.187	690	697	706	rBV	1385032	2136870	18.96%	1.980%
6	7.381	723	730	739	rBV	1602334	2456774	21.79%	2.277%
7	7.852	804	810	817	rBV	1311287	2012791	17.86%	1.865%
8	8.563	924	931	942	rBV	2078258	3291023	29.19%	3.050%
9	9.011	1000	1007	1015	rBV	1599545	2546317	22.59%	2.360%
10	9.734	1121	1130	1139	rBV	1153241	1841623	16.34%	1.707%
11	10.269	1212	1221	1231	rBV	2078092	3422224	30.36%	3.172%
12	10.646	1277	1285	1294	rVB	1880244	3179147	28.20%	2.946%
13	10.787	1301	1309	1323	rBV	1740694	2888027	25.62%	2.677%
14	12.234	1549	1555	1561	rBV2	40292	69607	0.62%	0.065%
15	13.128	1702	1707	1711	rBV	6144	14207	0.13%	0.013%
16	13.381	1746	1750	1757	rVB2	33446	56562	0.50%	0.052%
17	13.451	1757	1762	1767	rBV6	6992	13414	0.12%	0.012%
18	13.898	1829	1838	1849	rBV	4111664	5792936	51.39%	5.369%
19	14.175	1878	1885	1895	rBV	4782300	6797759	60.30%	6.300%
20	14.481	1930	1937	1945	rVB	3350586	4850231	43.03%	4.495%
21	14.675	1964	1970	1982	rBV	1876048	2763899	24.52%	2.562%
22	14.840	1996	1998	2004	rVB6	9795	11496	0.10%	0.011%
23	15.475	2099	2106	2116	rVB	6188425	8869494	78.68%	8.220%
24	15.587	2116	2125	2138	rBV	1592639	2140902	18.99%	1.984%
25	15.710	2142	2146	2154	rVB2	30258	54045	0.48%	0.050%
26	16.257	2234	2239	2244	rVB6	11678	20046	0.18%	0.019%
27	17.228	2397	2404	2411	rBV	4319155	6118435	54.28%	5.671%
28	17.328	2414	2421	2434	rVV	6767149	9729167	86.31%	9.017%
29	17.604	2465	2468	2478	rVB6	11608	21005	0.19%	0.019%
30	17.898	2516	2518	2524	rVB6	12879	13414	0.12%	0.012%
31	18.116	2553	2555	2559	rVB4	10673	11802	0.10%	0.011%
32	19.139	2725	2729	2736	rBV3	87470	112756	1.00%	0.105%
33	19.204	2736	2740	2744	rBV	85907	109430	0.97%	0.101%
34	19.563	2795	2801	2811	rBV	8408960	11272696	100.00%	10.447%
35	21.310	3093	3098	3105	rBV	4600915	6069190	53.84%	5.625%
36	23.527	3468	3475	3483	rBV2	4653487	8999670	79.84%	8.341%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018609.D
Acq On : 05 Dec 2023 18:32
Operator : MA/JU
Sample : PB157355BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK355

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	23.680	3495	3501	3514	rVB	2740882	5499957	48.79%	5.097%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 107898656

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018609.D
Acq On : 05 Dec 2023 18:32
Operator : MA/JU
Sample : PB157355BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK355

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

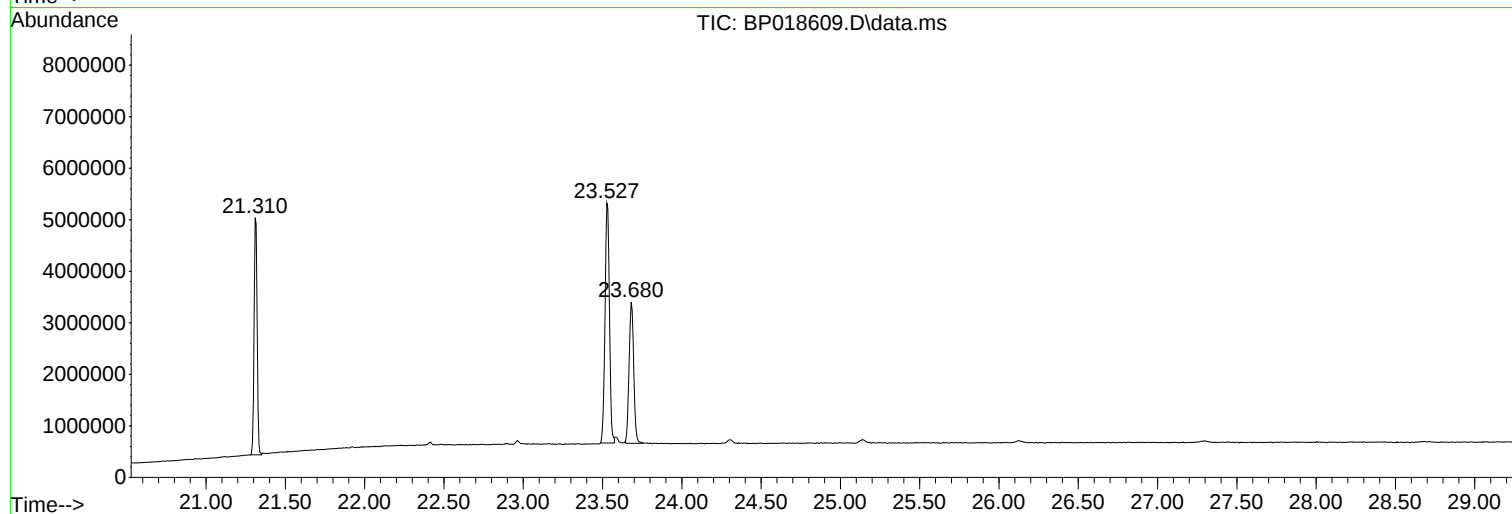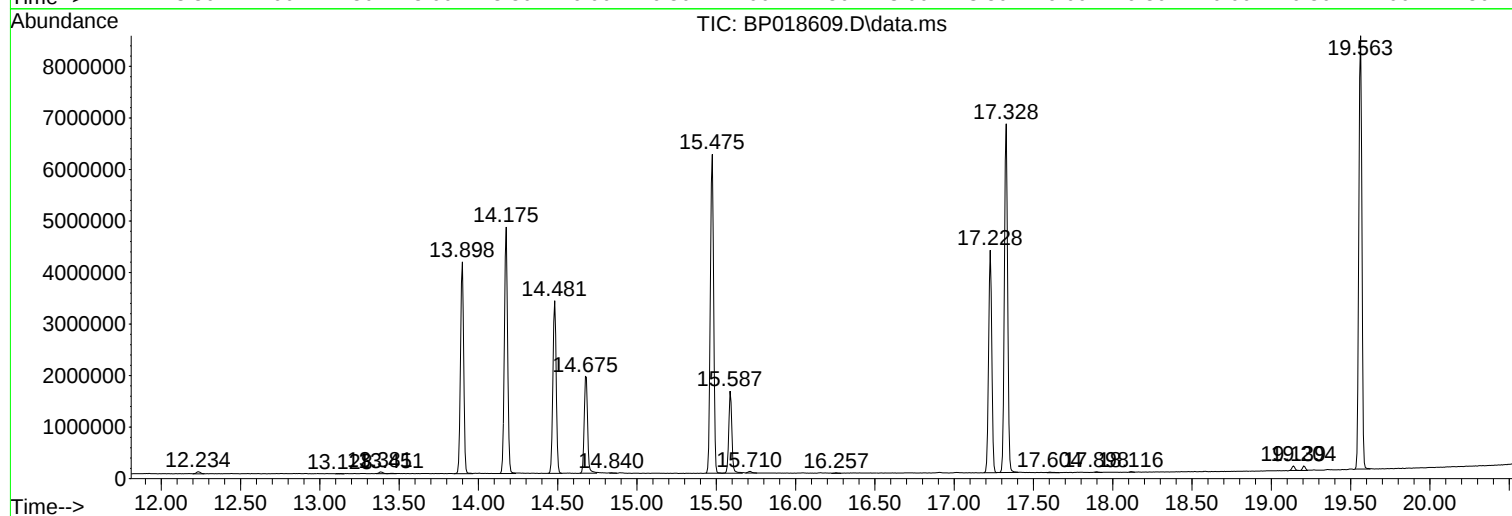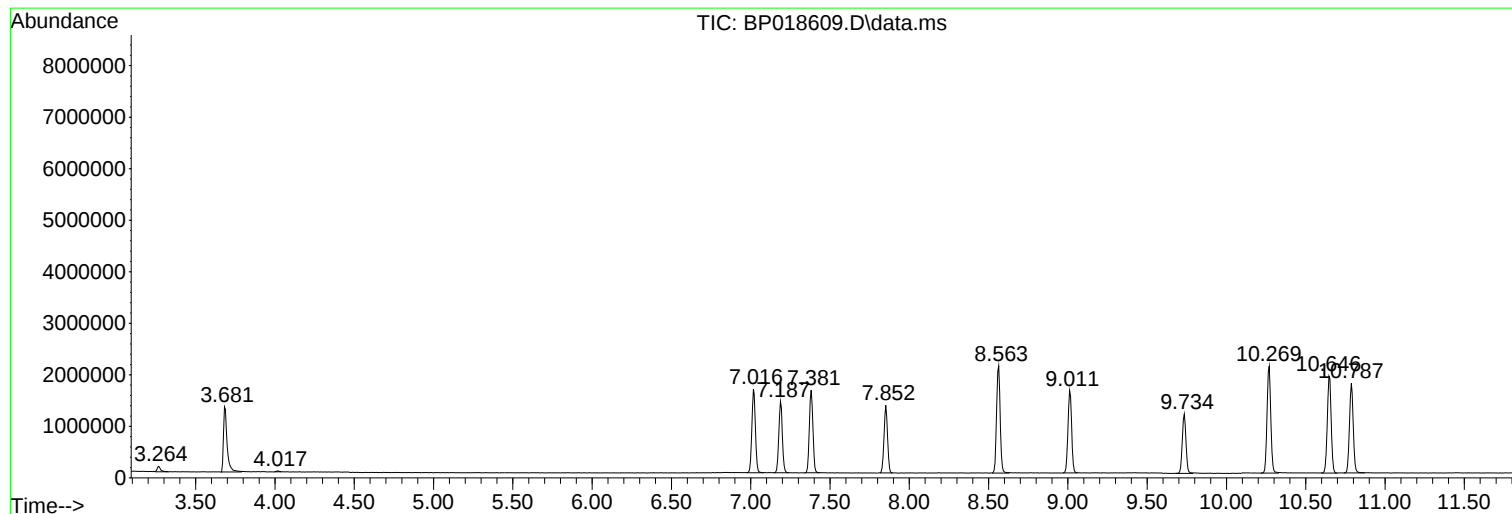

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018609.D
Acq On : 05 Dec 2023 18:32
Operator : MA/JU
Sample : PB157355BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK355

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018609.D
Acq On : 05 Dec 2023 18:32
Operator : MA/JU
Sample : PB157355BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK355

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------