

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018610.D
 Acq On : 05 Dec 2023 19:06
 Operator : MA/JU
 Sample : 05455-03
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E05L1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018610.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	44	rVB	68860	113765	0.84%	0.104%
2	3.687	98	102	112	rBV	507741	752049	5.58%	0.687%
3	3.922	138	142	149	rVB4	20830	35315	0.26%	0.032%
4	4.017	155	158	163	rVB	22851	31355	0.23%	0.029%
5	7.016	662	668	678	rVB	359107	561469	4.16%	0.513%
6	7.187	690	697	707	rBV	1628184	2479062	18.39%	2.266%
7	7.381	723	730	743	rVB	1397916	2113815	15.68%	1.932%
8	7.852	803	810	818	rVB	1227898	1914595	14.20%	1.750%
9	8.563	924	931	938	rBV	997680	1599820	11.87%	1.462%
10	9.010	1000	1007	1016	rBV	1863543	3003966	22.28%	2.745%
11	9.734	1122	1130	1137	rBV	1350294	2161930	16.04%	1.976%
12	10.269	1213	1221	1234	rBV	2180799	3538105	26.24%	3.234%
13	10.646	1278	1285	1293	rBV	1767883	2968156	22.02%	2.713%
14	10.787	1300	1309	1323	rBV	2226194	3701793	27.46%	3.383%
15	11.440	1416	1420	1425	rBV3	11312	18457	0.14%	0.017%
16	12.234	1550	1555	1562	rVB3	44594	77659	0.58%	0.071%
17	13.104	1698	1703	1706	rBV2	10761	18616	0.14%	0.017%
18	13.387	1744	1751	1754	rBV4	24805	44444	0.33%	0.041%
19	13.451	1758	1762	1766	rBV5	13560	19617	0.15%	0.018%
20	13.898	1831	1838	1845	rBV	4900199	6679525	49.55%	6.105%
21	14.016	1854	1858	1861	rVB4	8869	13895	0.10%	0.013%
22	14.175	1877	1885	1898	rBV	5414574	7895342	58.56%	7.216%
23	14.481	1930	1937	1947	rVB	3177681	4519987	33.53%	4.131%
24	14.675	1964	1970	1983	rBV	307952	502781	3.73%	0.459%
25	14.898	2003	2008	2013	rVB7	20447	34690	0.26%	0.032%
26	15.287	2070	2074	2076	rBV2	16036	22068	0.16%	0.020%
27	15.475	2099	2106	2117	rBV	7531484	10478865	77.73%	9.577%
28	15.587	2119	2125	2141	rVV	1856554	2593760	19.24%	2.370%
29	15.710	2142	2146	2151	rVB	37731	57338	0.43%	0.052%
30	16.251	2236	2238	2244	rBV4	11790	16035	0.12%	0.015%
31	16.898	2345	2348	2353	rVB4	10115	14639	0.11%	0.013%
32	17.228	2398	2404	2414	rVB	3899877	5486537	40.70%	5.014%
33	17.328	2414	2421	2434	rBV	8363375	12007633	89.07%	10.974%
34	17.610	2465	2469	2472	rBV3	11302	17652	0.13%	0.016%
35	17.898	2515	2518	2522	rVB6	22843	28521	0.21%	0.026%
36	18.116	2551	2555	2561	rBV2	45715	62126	0.46%	0.057%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018610.D
Acq On : 05 Dec 2023 19:06
Operator : MA/JU
Sample : 05455-03
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E05L1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.139	2725	2729	2735	rVB	103862	135973	1.01%	0.124%
38	19.204	2736	2740	2745	rBV	94496	130561	0.97%	0.119%
39	19.351	2761	2765	2770	rBV3	42737	59980	0.44%	0.055%
40	19.563	2795	2801	2812	rBV	10472761	13481711	100.00%	12.321%
41	21.310	3093	3098	3105	rBV	3980706	4981275	36.95%	4.552%
42	23.527	3468	3475	3491	rVB2	5428142	10576103	78.45%	9.666%
43	23.680	3494	3501	3513	rVB	2269241	4468533	33.15%	4.084%




Sum of corrected areas: 109419518

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018610.D
Acq On : 05 Dec 2023 19:06
Operator : MA/JU
Sample : 05455-03
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E05L1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

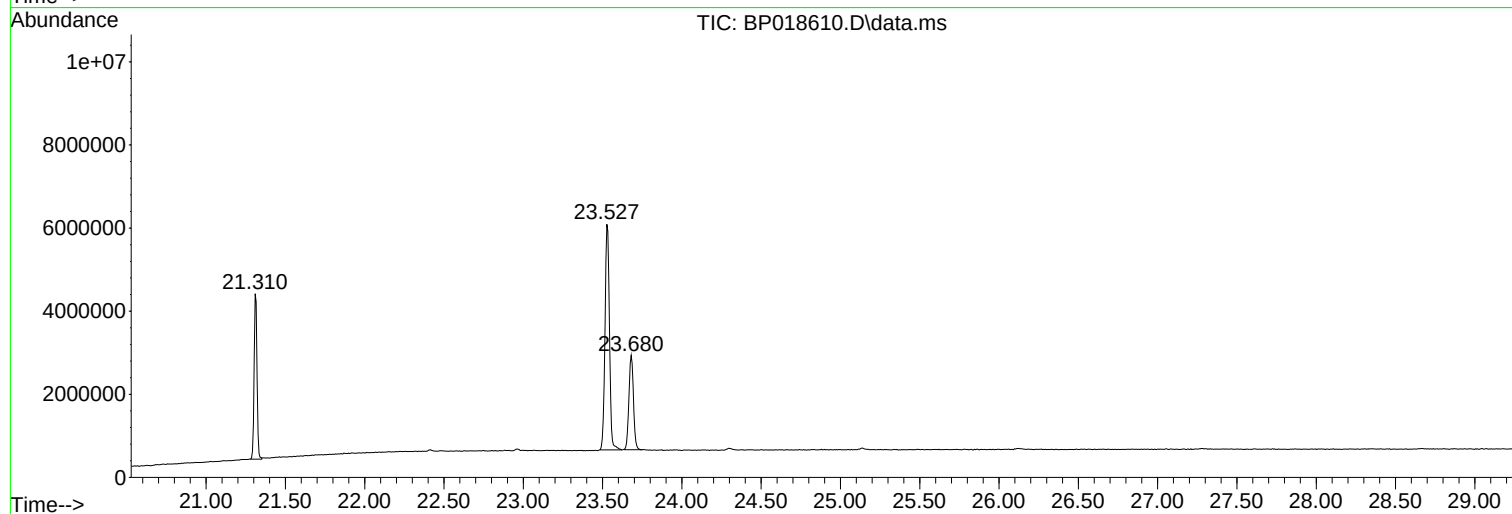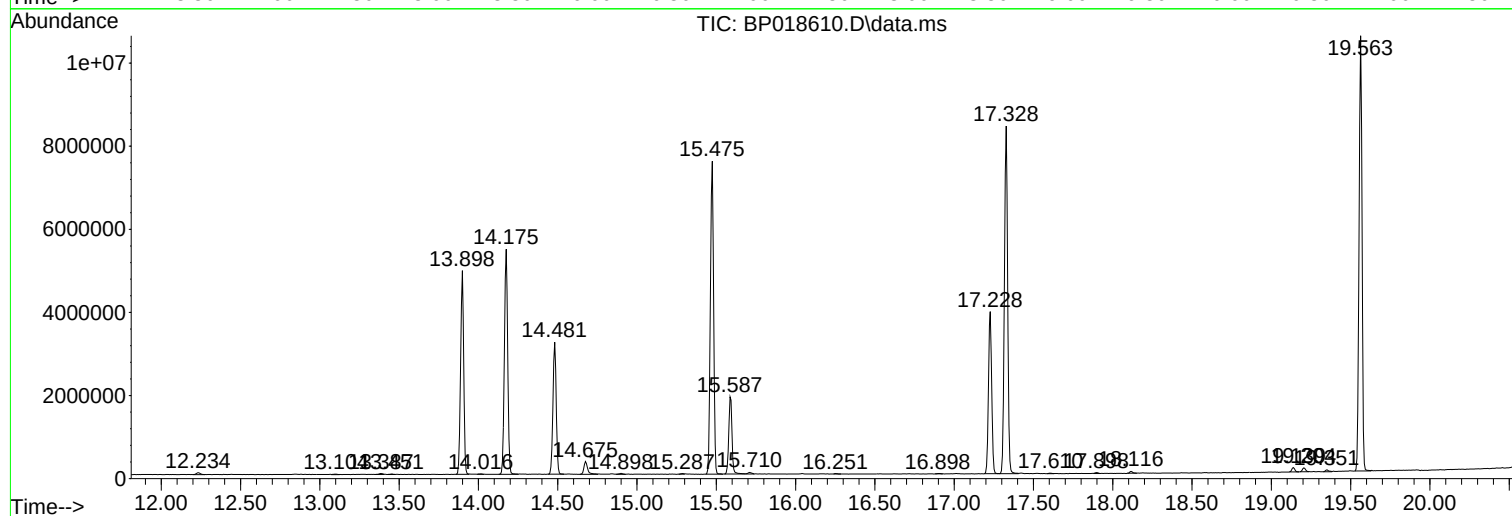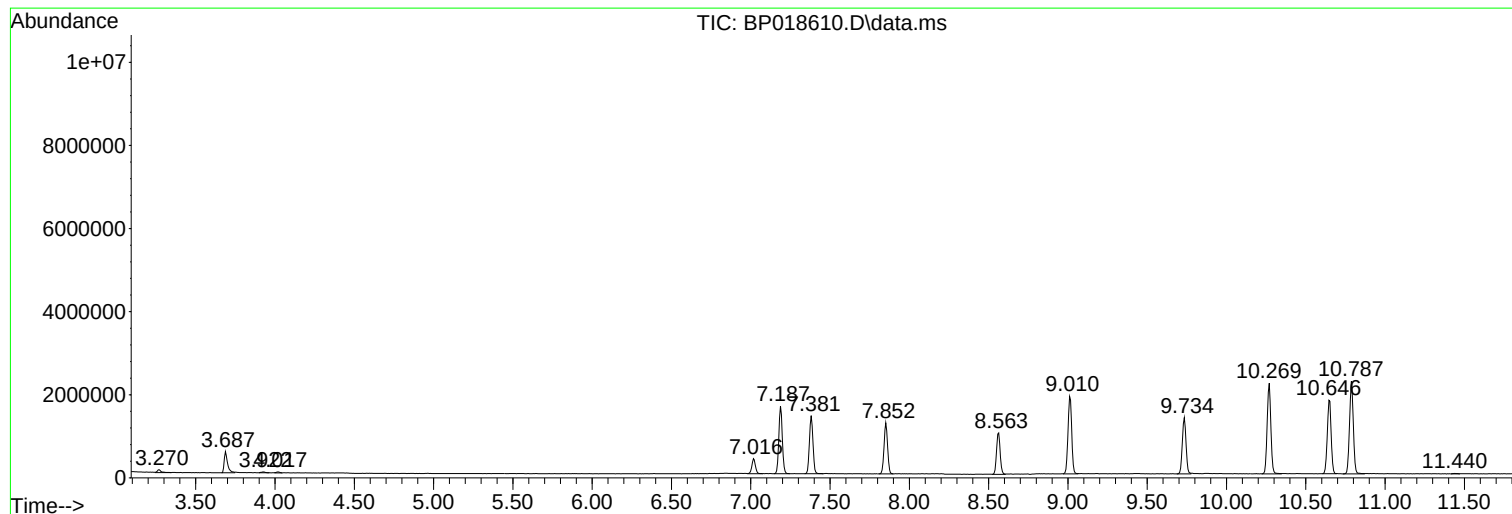

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018610.D
Acq On : 05 Dec 2023 19:06
Operator : MA/JU
Sample : 05455-03
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E05L1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018610.D
Acq On : 05 Dec 2023 19:06
Operator : MA/JU
Sample : 05455-03
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E05L1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc