

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018614.D
 Acq On : 05 Dec 2023 21:22
 Operator : MA/JU
 Sample : 05455-08
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E05N3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018614.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	37	rVB	65317	88080	0.72%	0.086%
2	3.364	44	47	53	rVB2	26173	35531	0.29%	0.035%
3	3.534	73	76	82	rVB2	16638	23403	0.19%	0.023%
4	3.687	98	102	113	rBV	380830	574167	4.70%	0.560%
5	3.923	140	142	150	rVB3	19697	30798	0.25%	0.030%
6	4.017	154	158	163	rVB	22697	29020	0.24%	0.028%
7	4.493	235	239	245	rVB	61681	86482	0.71%	0.084%
8	5.611	426	429	434	rVB4	12456	17398	0.14%	0.017%
9	5.881	470	475	482	rVB	87976	139420	1.14%	0.136%
10	6.252	534	538	543	rBV3	11442	20041	0.16%	0.020%
11	7.016	662	668	676	rVB	329908	515167	4.21%	0.503%
12	7.187	690	697	706	rVB	1498522	2276702	18.63%	2.222%
13	7.381	723	730	737	rBV	1303261	1990682	16.29%	1.943%
14	7.852	803	810	818	rVB	1311212	2052612	16.79%	2.003%
15	8.563	924	931	942	rBV	995540	1584547	12.96%	1.546%
16	9.011	1000	1007	1019	rBV	1736362	2801169	22.92%	2.734%
17	9.734	1122	1130	1137	rBV	1334971	2130651	17.43%	2.079%
18	9.793	1138	1140	1147	rVB3	18704	24320	0.20%	0.024%
19	9.963	1165	1169	1174	rBV5	7894	16414	0.13%	0.016%
20	10.269	1211	1221	1230	rBV	1930494	3176006	25.98%	3.099%
21	10.646	1278	1285	1293	rVB	1543427	2599072	21.26%	2.536%
22	10.787	1299	1309	1320	rBV	1587990	2651342	21.69%	2.587%
23	12.234	1550	1555	1565	rVB	45000	71471	0.58%	0.070%
24	13.387	1746	1751	1757	rVB2	39116	59254	0.48%	0.058%
25	13.898	1831	1838	1848	rBV	4515916	6109424	49.98%	5.962%
26	14.175	1878	1885	1900	rBV	4984582	7356106	60.18%	7.179%
27	14.481	1930	1937	1946	rBV	3270581	4732261	38.72%	4.618%
28	14.675	1965	1970	1974	rBV	277048	446786	3.66%	0.436%
29	14.746	1980	1982	1987	rVB2	25080	29528	0.24%	0.029%
30	14.898	2004	2008	2013	rVB7	14310	28037	0.23%	0.027%
31	15.281	2070	2073	2075	rBV3	11077	12890	0.11%	0.013%
32	15.475	2099	2106	2116	rBV	6591925	9546570	78.11%	9.316%
33	15.587	2119	2125	2138	rBV	1729724	2309062	18.89%	2.253%
34	15.710	2142	2146	2151	rVB2	31177	47479	0.39%	0.046%
35	16.904	2345	2349	2355	rVB3	16486	24205	0.20%	0.024%
36	17.228	2397	2404	2412	rBV	4019225	5769194	47.20%	5.630%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018614.D
Acq On : 05 Dec 2023 21:22
Operator : MA/JU
Sample : 05455-08
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E05N3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	17.328	2414	2421	2433	rVV	7637884	10833889	88.64%	10.572%
38	17.604	2465	2468	2472	rVB4	11083	15341	0.13%	0.015%
39	17.898	2515	2518	2523	rVB4	20933	26525	0.22%	0.026%
40	18.116	2551	2555	2561	rBV2	78627	111786	0.91%	0.109%
41	18.186	2564	2567	2573	rVB	50874	66846	0.55%	0.065%
42	19.139	2724	2729	2733	rBV2	100699	138969	1.14%	0.136%
43	19.204	2736	2740	2748	rVV	104669	147790	1.21%	0.144%
44	19.351	2762	2765	2772	rVB5	32470	41353	0.34%	0.040%
45	19.563	2795	2801	2807	rBV	9290238	12222664	100.00%	11.928%
46	21.310	3093	3098	3104	rBV	4275657	5295198	43.32%	5.167%
47	23.527	3467	3475	3482	rBV2	4737295	9534663	78.01%	9.304%
48	23.680	3494	3501	3510	rVB	2331907	4633543	37.91%	4.522%




Sum of corrected areas: 102473858

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018614.D
Acq On : 05 Dec 2023 21:22
Operator : MA/JU
Sample : 05455-08
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E05N3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

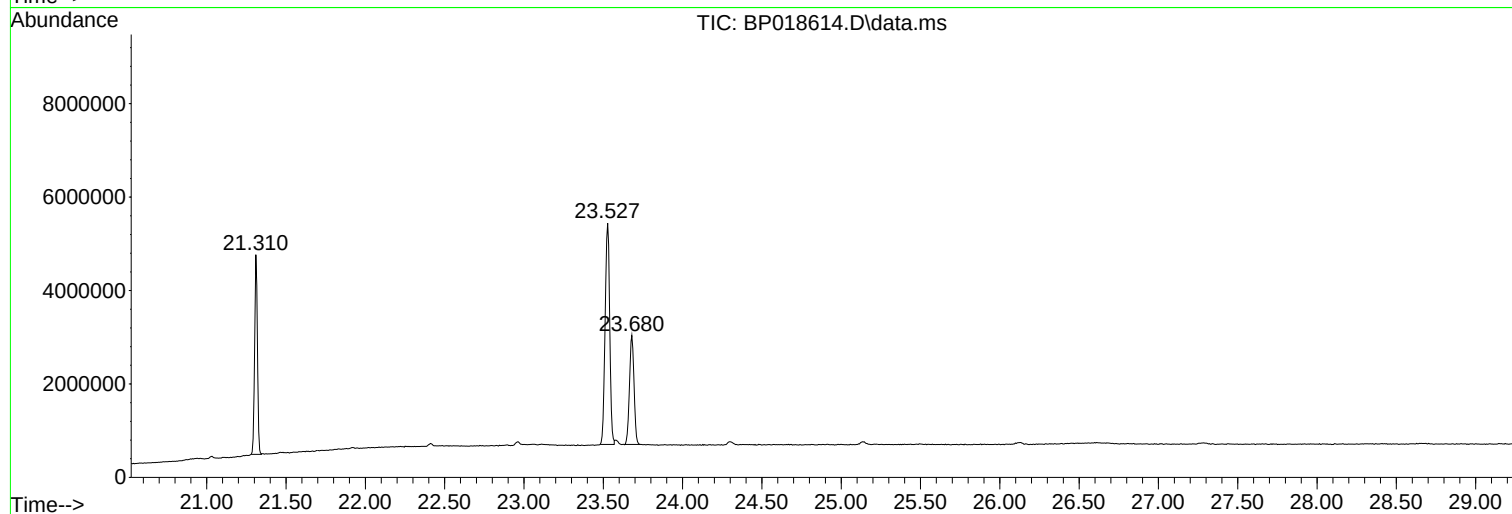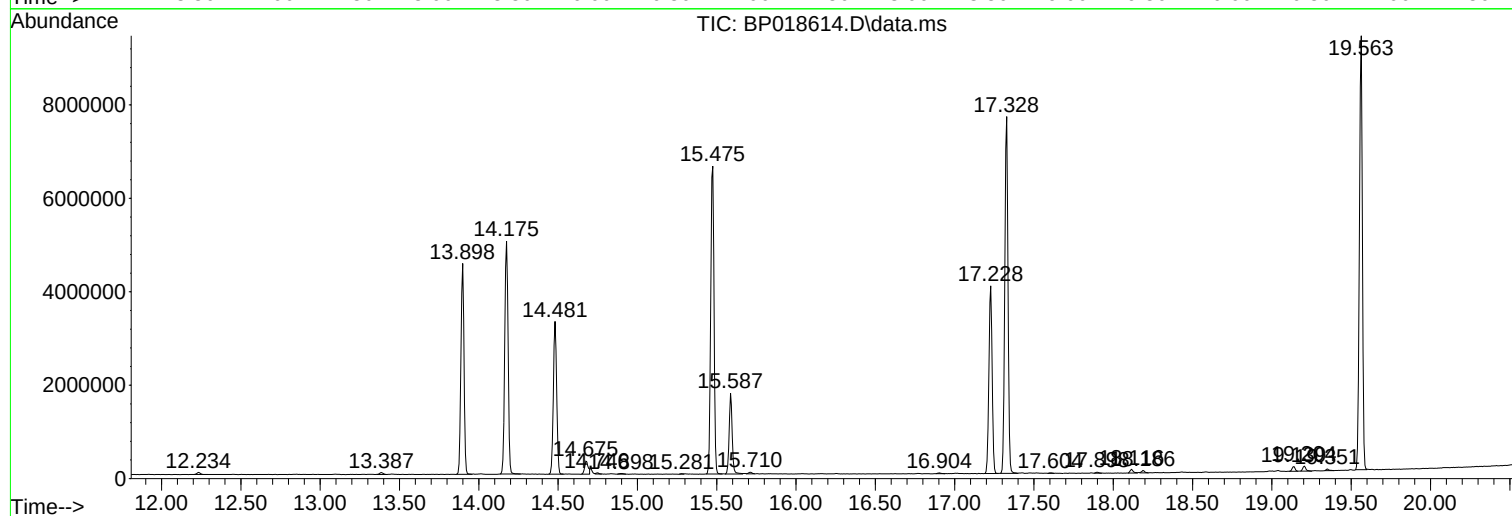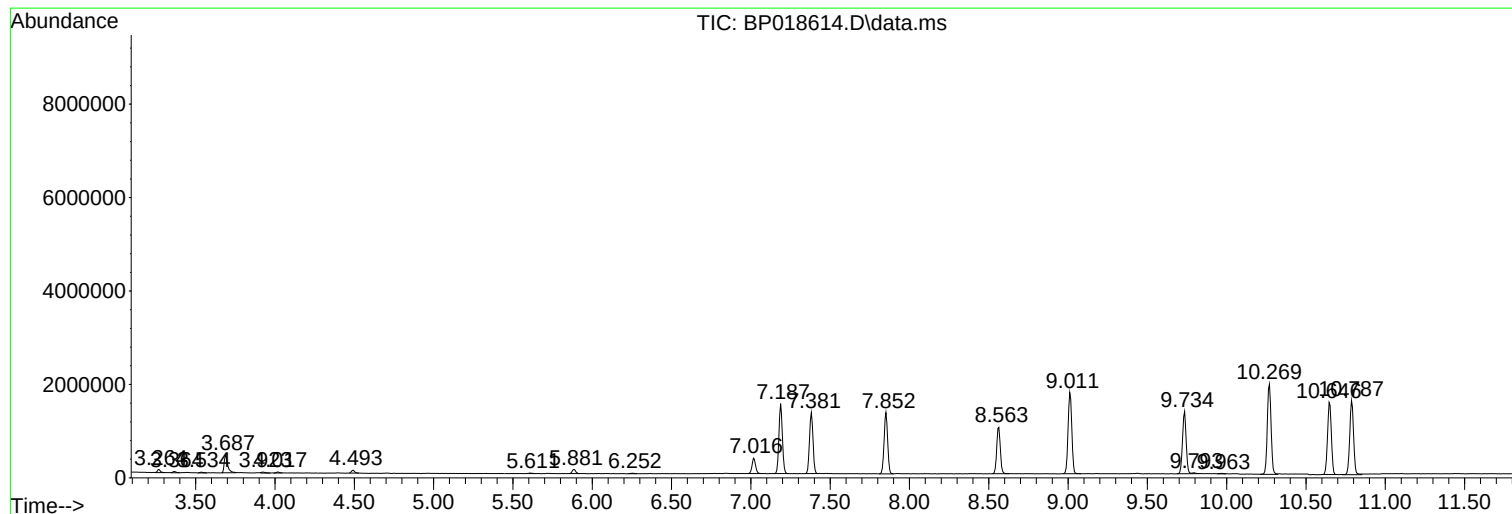

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018614.D
Acq On : 05 Dec 2023 21:22
Operator : MA/JU
Sample : 05455-08
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E05N3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018614.D
Acq On : 05 Dec 2023 21:22
Operator : MA/JU
Sample : 05455-08
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E05N3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc