

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018617.D
 Acq On : 05 Dec 2023 23:04
 Operator : MA/JU
 Sample : 05455-11
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E05N4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018617.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	36	rVB	62983	76015	0.72%	0.093%
2	3.364	45	47	54	rVB4	23924	36503	0.35%	0.045%
3	3.540	74	77	81	rVB3	13549	17447	0.17%	0.021%
4	3.693	99	103	116	rVB	228016	353816	3.37%	0.434%
5	3.922	139	142	147	rVB4	17508	26267	0.25%	0.032%
6	4.017	155	158	166	rVB2	24018	36801	0.35%	0.045%
7	4.493	235	239	243	rBV2	47304	66890	0.64%	0.082%
8	5.611	426	429	434	rVB2	17419	23908	0.23%	0.029%
9	5.716	444	447	455	rVB3	18473	40613	0.39%	0.050%
10	5.887	471	476	481	rBV	68767	104099	0.99%	0.128%
11	6.252	532	538	544	rVB2	22287	60851	0.58%	0.075%
12	7.016	661	668	677	rBV	255470	391550	3.73%	0.480%
13	7.187	689	697	706	rBV	1009829	1544152	14.73%	1.893%
14	7.381	722	730	741	rBV	945167	1468257	14.00%	1.800%
15	7.475	743	746	751	rVB4	8001	14562	0.14%	0.018%
16	7.852	801	810	818	rVB	834416	1287336	12.28%	1.578%
17	8.563	922	931	939	rBV	743646	1203151	11.47%	1.475%
18	9.010	1000	1007	1017	rBV	1221691	1986914	18.95%	2.436%
19	9.181	1031	1036	1042	rVB5	12753	19657	0.19%	0.024%
20	9.734	1122	1130	1137	rBV	978642	1587593	15.14%	1.947%
21	9.793	1137	1140	1146	rVB3	12936	21706	0.21%	0.027%
22	10.269	1213	1221	1234	rBV	1491280	2498839	23.83%	3.064%
23	10.646	1278	1285	1293	rBV	1198154	1973451	18.82%	2.420%
24	10.787	1301	1309	1317	rBV	1243529	2052965	19.58%	2.517%
25	12.234	1546	1555	1563	rVB2	34110	65527	0.62%	0.080%
26	12.846	1652	1659	1663	rBV5	9426	16215	0.15%	0.020%
27	13.387	1744	1751	1758	rBV2	34313	59573	0.57%	0.073%
28	13.451	1758	1762	1766	rVB5	5825	10873	0.10%	0.013%
29	13.898	1829	1838	1849	rBV	3419007	4776635	45.55%	5.857%
30	14.175	1877	1885	1892	rBV	3725869	5401296	51.51%	6.622%
31	14.481	1930	1937	1944	rBV	2111700	3058216	29.17%	3.750%
32	14.675	1964	1970	1980	rBV	248581	396437	3.78%	0.486%
33	14.904	2002	2009	2013	rBV8	13330	25360	0.24%	0.031%
34	15.222	2059	2063	2069	rBV	9929	14862	0.14%	0.018%
35	15.281	2069	2073	2081	rVV2	54251	81230	0.77%	0.100%
36	15.475	2097	2106	2113	rBV	4949013	7316243	69.77%	8.970%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018617.D
 Acq On : 05 Dec 2023 23:04
 Operator : MA/JU
 Sample : 05455-11
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E05N4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.587	2119	2125	2138	rBV	1402355	1955110	18.65%	2.397%
38	15.710	2142	2146	2154	rVB4	25752	44731	0.43%	0.055%
39	16.257	2235	2239	2242	rBV5	8083	12540	0.12%	0.015%
40	17.010	2362	2367	2371	rBV4	7597	15609	0.15%	0.019%
41	17.228	2397	2404	2410	rBV	2855320	3874031	36.95%	4.750%
42	17.328	2414	2421	2431	rVV	5942313	8294277	79.10%	10.169%
43	17.522	2449	2454	2461	rVB3	15720	25781	0.25%	0.032%
44	17.898	2514	2518	2523	rVB3	67625	88009	0.84%	0.108%
45	18.116	2551	2555	2559	rBV3	63744	78355	0.75%	0.096%
46	18.192	2564	2568	2571	rBV	36917	46978	0.45%	0.058%
47	19.139	2725	2729	2734	rVB3	82259	104039	0.99%	0.128%
48	19.204	2736	2740	2747	rBV	82883	118154	1.13%	0.145%
49	19.351	2761	2765	2770	rBV4	44860	58734	0.56%	0.072%
50	19.563	2795	2801	2807	rBV	7444647	9758589	93.07%	11.965%
51	21.310	3093	3098	3104	rBV	3176972	3917260	37.36%	4.803%
52	23.527	3468	3475	3483	rBV2	5362622	10485775	100.00%	12.856%
53	23.680	3494	3501	3511	rVB	2334693	4566900	43.55%	5.599%




Sum of corrected areas: 81560682

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018617.D
Acq On : 05 Dec 2023 23:04
Operator : MA/JU
Sample : 05455-11
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E05N4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

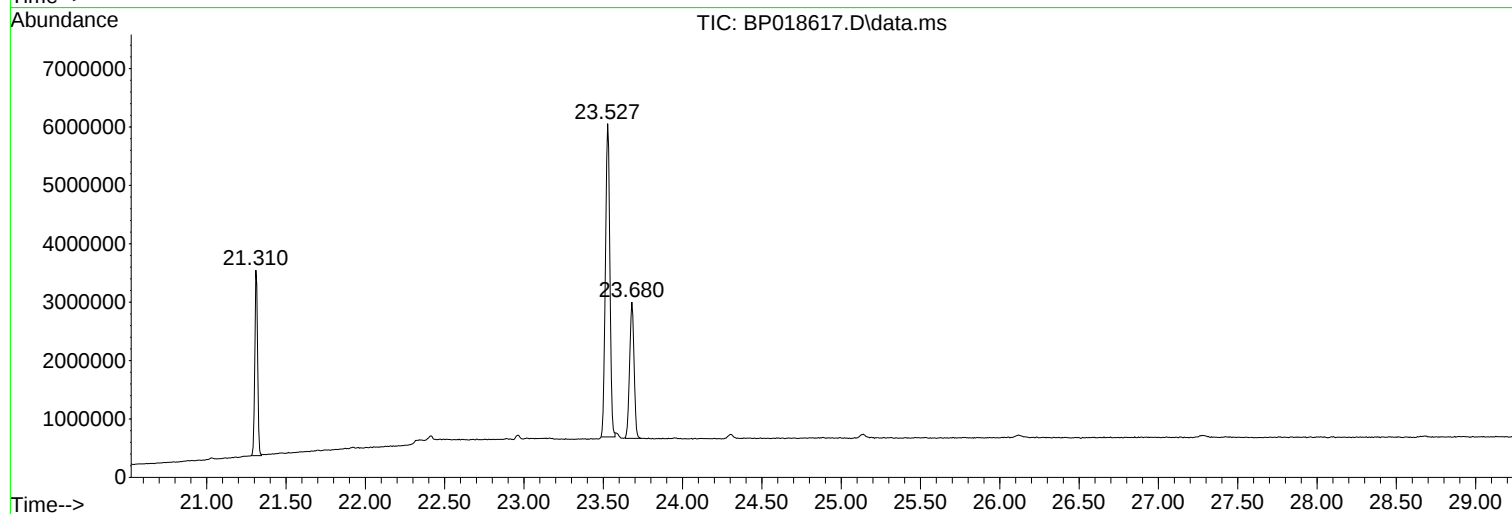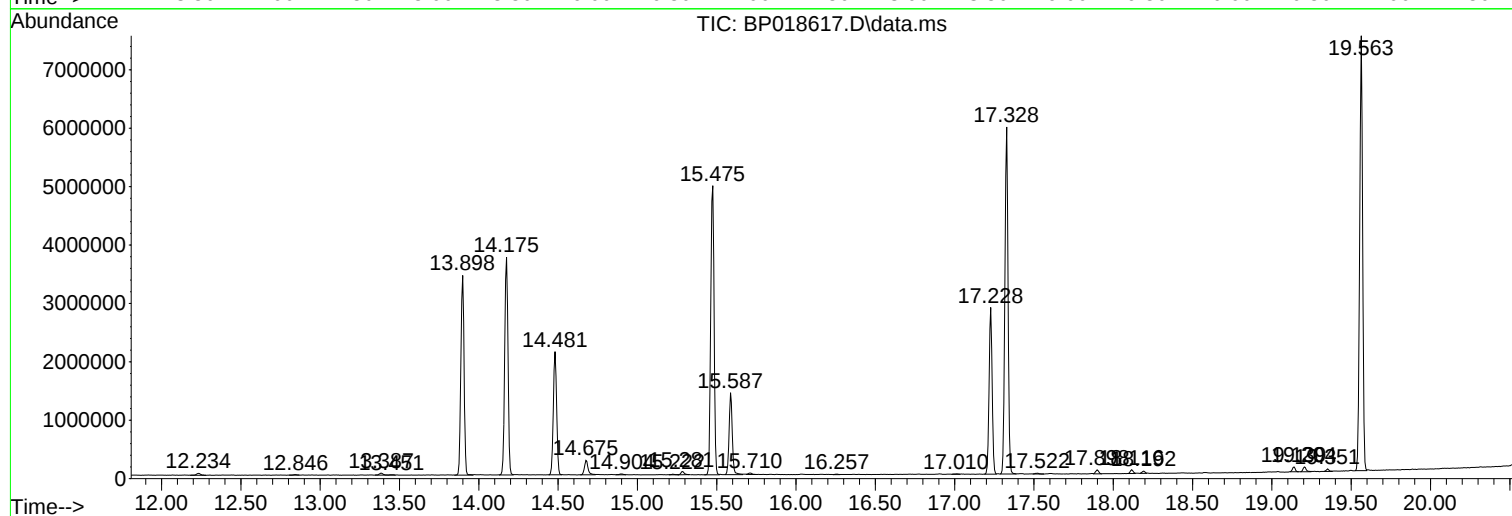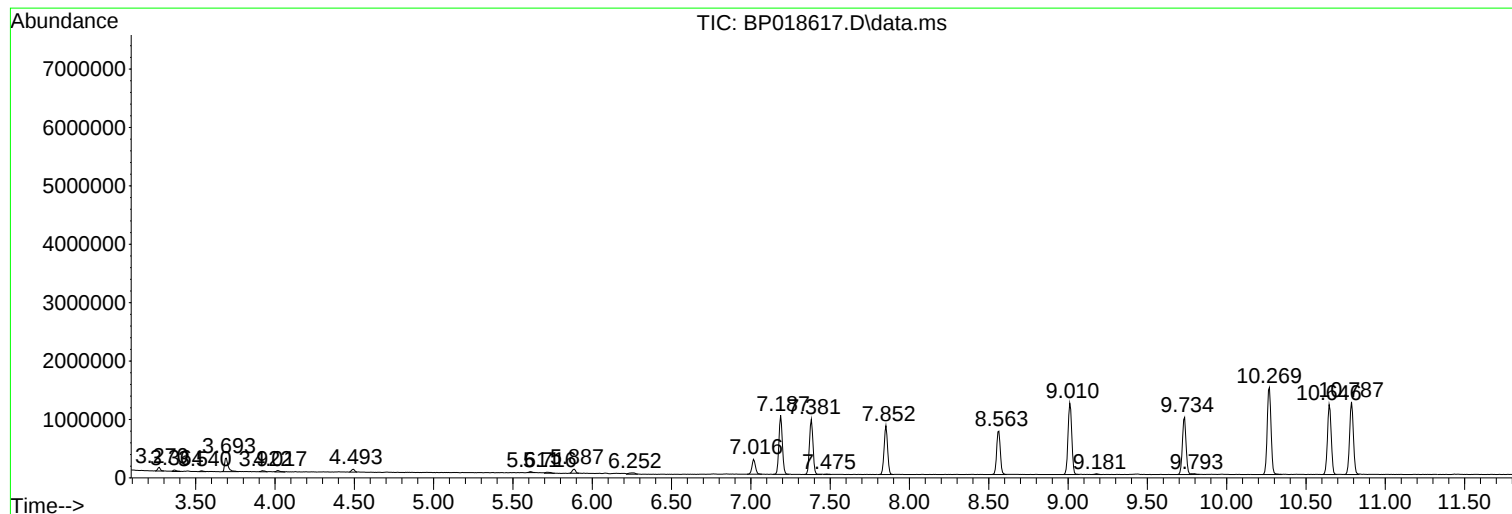

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018617.D
Acq On : 05 Dec 2023 23:04
Operator : MA/JU
Sample : 05455-11
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E05N4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018617.D
Acq On : 05 Dec 2023 23:04
Operator : MA/JU
Sample : 05455-11
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E05N4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc