

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018639.D
 Acq On : 06 Dec 2023 16:21
 Operator : MA/JU
 Sample : PB157358BL
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK358

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018639.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	38	rVB	131838	163427	1.91%	0.156%
2	3.681	97	101	116	rBV	1498841	2155059	25.18%	2.063%
3	4.016	155	158	165	rVB2	25232	38395	0.45%	0.037%
4	5.099	339	342	343	rBV	8923	9365	0.11%	0.009%
5	7.022	662	669	681	rBV	1892645	2966698	34.66%	2.840%
6	7.187	690	697	705	rBV	1603657	2417837	28.25%	2.314%
7	7.381	723	730	740	rBV	1934656	2973818	34.75%	2.847%
8	7.852	803	810	817	rBV	1501939	2322593	27.14%	2.223%
9	8.434	904	909	911	rBV	10427	16016	0.19%	0.015%
10	8.563	923	931	941	rBV	2451611	3858035	45.08%	3.693%
11	9.010	1000	1007	1015	rBV	1825629	2953023	34.50%	2.827%
12	9.734	1121	1130	1137	rBV	1498662	2431471	28.41%	2.327%
13	10.269	1213	1221	1229	rBV	2405824	3983122	46.54%	3.813%
14	10.646	1278	1285	1293	rVB	2298829	3888152	45.43%	3.722%
15	10.787	1302	1309	1321	rVB	1869686	3100979	36.23%	2.968%
16	11.440	1417	1420	1425	rBV5	5525	11755	0.14%	0.011%
17	12.234	1550	1555	1561	rVB2	49038	76905	0.90%	0.074%
18	13.387	1745	1751	1757	rVB	45686	69678	0.81%	0.067%
19	13.451	1759	1762	1767	rVB4	9192	12577	0.15%	0.012%
20	13.898	1831	1838	1844	rBV	4198972	5900233	68.94%	5.648%
21	14.039	1861	1862	1868	rVB	12789	14741	0.17%	0.014%
22	14.175	1877	1885	1898	rBV	4264741	6343157	74.12%	6.072%
23	14.481	1930	1937	1946	rBV	3398431	4954089	57.88%	4.742%
24	14.681	1963	1971	1987	rBV	1518524	2351906	27.48%	2.251%
25	14.792	1987	1990	1994	rVV	10340	20073	0.23%	0.019%
26	14.839	1996	1998	2000	rVV3	10732	10925	0.13%	0.010%
27	14.892	2004	2007	2009	rVV2	7989	9090	0.11%	0.009%
28	15.475	2099	2106	2114	rBV	6054642	8558525	100.00%	8.192%
29	15.592	2120	2126	2137	rBV	1348711	1845956	21.57%	1.767%
30	15.716	2142	2147	2151	rVB3	26808	40793	0.48%	0.039%
31	16.251	2236	2238	2243	rVB4	6506	9131	0.11%	0.009%
32	17.010	2365	2367	2374	rVB5	9891	15355	0.18%	0.015%
33	17.228	2398	2404	2411	rBV	4086954	5711483	66.73%	5.467%
34	17.328	2414	2421	2432	rVV	5829195	8252359	96.42%	7.899%
35	19.139	2725	2729	2734	rBV2	72101	102660	1.20%	0.098%
36	19.210	2737	2741	2745	rBV	73720	100551	1.17%	0.096%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018639.D
Acq On : 06 Dec 2023 16:21
Operator : MA/JU
Sample : PB157358BL
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK358

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.563	2795	2801	2808	rBV	6280310	8394105	98.08%	8.035%
38	21.316	3094	3099	3106	rBV	3964527	5039735	58.89%	4.824%
39	23.539	3469	3477	3483	rBV2	4114679	7976549	93.20%	7.635%
40	23.686	3495	3502	3514	rVB	2557590	5370084	62.75%	5.140%




Sum of corrected areas: 104470405

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018639.D
Acq On : 06 Dec 2023 16:21
Operator : MA/JU
Sample : PB157358BL
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK358

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

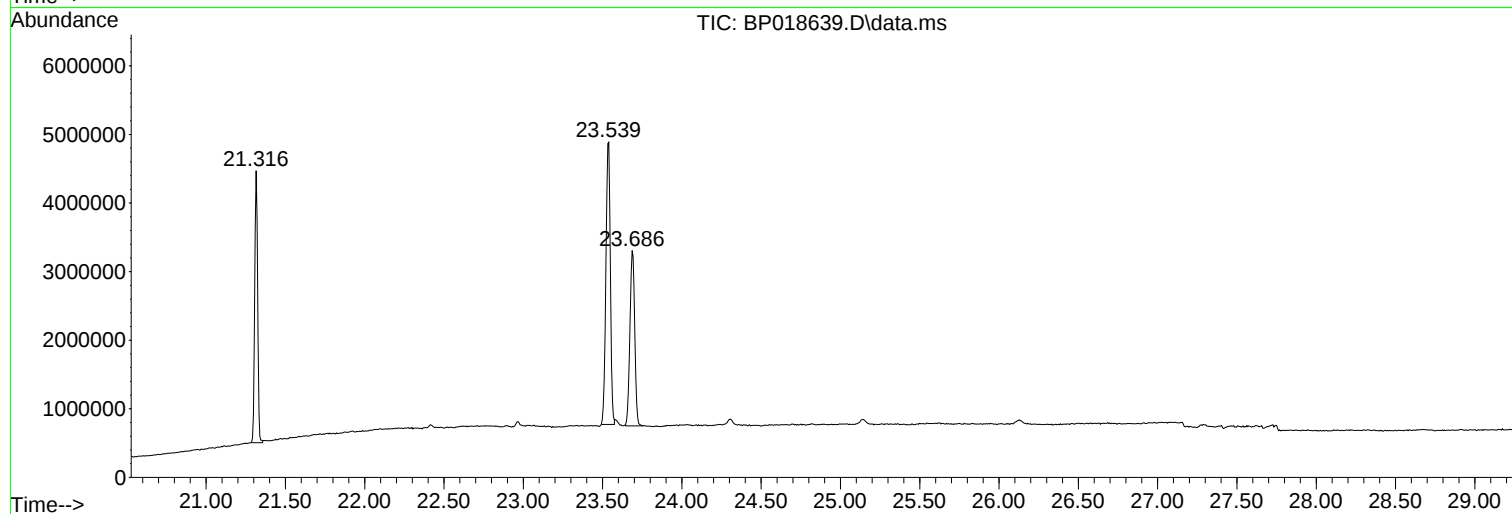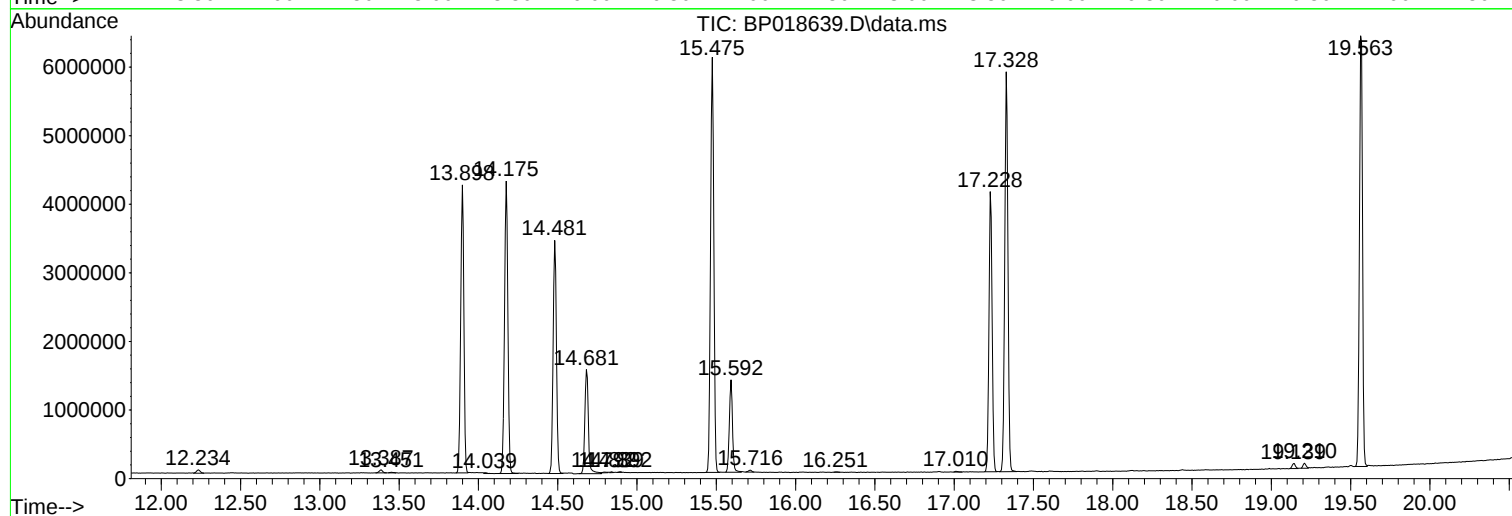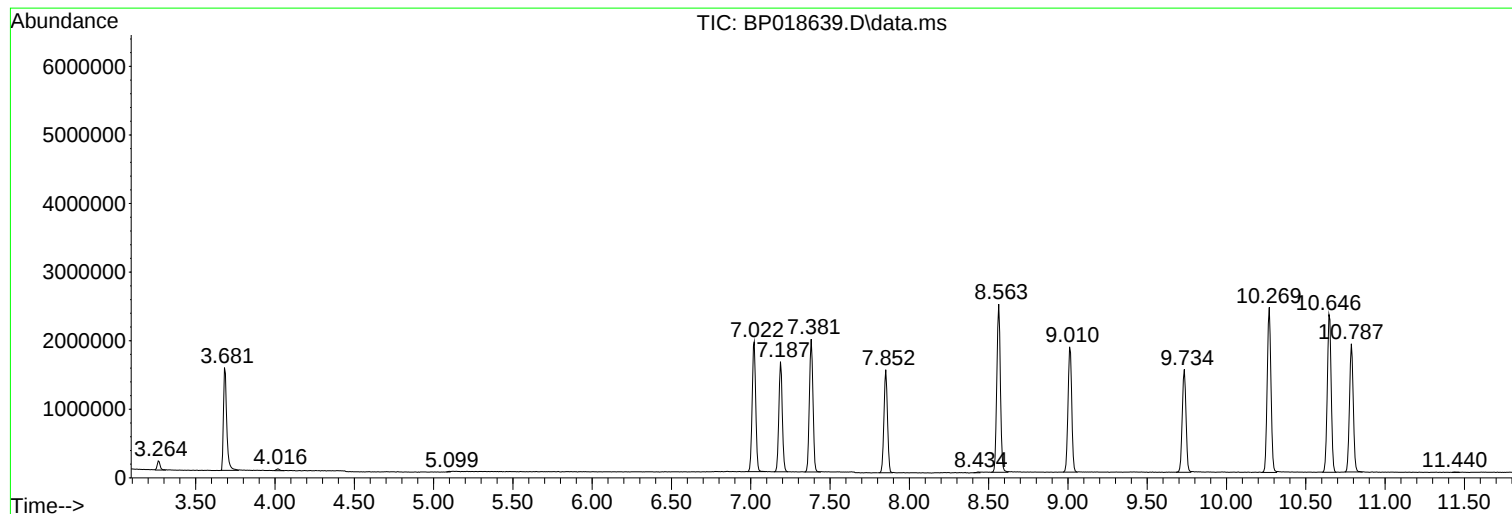

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018639.D
Acq On : 06 Dec 2023 16:21
Operator : MA/JU
Sample : PB157358BL
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK358

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018639.D
Acq On : 06 Dec 2023 16:21
Operator : MA/JU
Sample : PB157358BL
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK358

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc