

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018645.D
 Acq On : 06 Dec 2023 19:45
 Operator : MA/JU
 Sample : 05473-04
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018645.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	36	rVB	72222	91968	1.09%	0.115%
2	3.687	98	102	117	rBV	310962	452830	5.35%	0.564%
3	3.799	118	121	129	rVB	34298	44669	0.53%	0.056%
4	3.922	140	142	146	rVB2	16539	16013	0.19%	0.020%
5	4.016	155	158	164	rVB2	20335	30650	0.36%	0.038%
6	4.246	194	197	202	rVB3	16741	22451	0.27%	0.028%
7	5.046	329	333	337	rBV2	16916	24168	0.29%	0.030%
8	7.016	662	668	677	rVB	419417	647686	7.65%	0.807%
9	7.187	690	697	710	rVB	1622379	2452691	28.97%	3.055%
10	7.381	723	730	737	rBV	1497544	2331721	27.54%	2.904%
11	7.475	741	746	749	rBV3	8436	14039	0.17%	0.017%
12	7.852	803	810	818	rBV	1428544	2222031	26.25%	2.768%
13	8.099	843	852	857	rBV6	13953	32792	0.39%	0.041%
14	8.193	867	868	874	rVB	10008	8899	0.11%	0.011%
15	8.563	924	931	938	rBV	943203	1501798	17.74%	1.871%
16	9.010	995	1007	1018	rBV	1465012	2380548	28.12%	2.965%
17	9.181	1030	1036	1038	rVB5	6249	9330	0.11%	0.012%
18	9.428	1068	1078	1084	rVB5	22601	53994	0.64%	0.067%
19	9.734	1120	1130	1142	rBV	1167290	1932449	22.83%	2.407%
20	9.899	1150	1158	1161	rBV4	10322	21513	0.25%	0.027%
21	10.069	1180	1187	1193	rBV4	7093	13366	0.16%	0.017%
22	10.169	1199	1204	1207	rBV4	8401	12855	0.15%	0.016%
23	10.269	1213	1221	1229	rBV	1785555	3006414	35.51%	3.745%
24	10.334	1229	1232	1238	rVB7	15575	26803	0.32%	0.033%
25	10.428	1243	1248	1252	rBV6	8936	14307	0.17%	0.018%
26	10.522	1259	1264	1266	rBV6	5113	9569	0.11%	0.012%
27	10.646	1277	1285	1292	rBV	1524053	2501190	29.54%	3.115%
28	10.710	1292	1296	1300	rVB4	7498	12815	0.15%	0.016%
29	10.787	1300	1309	1320	rBV	633764	1078364	12.74%	1.343%
30	11.040	1347	1352	1354	rBV6	5252	9744	0.12%	0.012%
31	11.063	1354	1356	1362	rVB7	6280	9984	0.12%	0.012%
32	11.193	1374	1378	1383	rBV6	10437	17059	0.20%	0.021%
33	11.916	1495	1501	1505	rVB5	15581	25411	0.30%	0.032%
34	12.145	1534	1540	1544	rBV7	9070	16314	0.19%	0.020%
35	12.234	1548	1555	1562	rBV2	35657	64760	0.76%	0.081%
36	12.551	1605	1609	1613	rBV5	9868	13876	0.16%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018645.D
 Acq On : 06 Dec 2023 19:45
 Operator : MA/JU
 Sample : 05473-04
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	12.616	1615	1620	1625	rBV7	4078	9483	0.11%	0.012%
38	12.863	1656	1662	1664	rBV7	5829	11997	0.14%	0.015%
39	13.057	1688	1695	1700	rBV7	10241	23269	0.27%	0.029%
40	13.140	1706	1709	1717	rVB8	7938	16397	0.19%	0.020%

41	13.210	1717	1721	1723	rBV4	6809	9472	0.11%	0.012%
42	13.310	1735	1738	1742	rVB6	6295	10359	0.12%	0.013%
43	13.387	1745	1751	1758	rBV2	41131	77469	0.92%	0.096%
44	13.475	1758	1766	1770	rVV6	12834	30404	0.36%	0.038%
45	13.522	1770	1774	1781	rVB5	7853	14878	0.18%	0.019%

46	13.675	1794	1800	1801	rBV3	6932	11208	0.13%	0.014%
47	13.722	1806	1808	1810	rBV3	6936	8914	0.11%	0.011%
48	13.792	1817	1820	1825	rBV7	7355	9916	0.12%	0.012%
49	13.851	1825	1830	1831	rBV3	9343	12708	0.15%	0.016%
50	13.898	1831	1838	1847	rVB	3456331	4697894	55.49%	5.852%

51	14.175	1874	1885	1893	rBV	3602807	5440005	64.26%	6.776%
52	14.351	1908	1915	1917	rBV6	17662	29073	0.34%	0.036%
53	14.422	1923	1927	1930	rBV6	8232	10875	0.13%	0.014%
54	14.481	1930	1937	1943	rBV	2397580	3468426	40.97%	4.320%
55	14.557	1948	1950	1958	rVB5	10397	19530	0.23%	0.024%

56	14.681	1965	1971	1981	rBV	227462	377165	4.46%	0.470%
57	14.834	1988	1997	2004	rBV7	45495	118284	1.40%	0.147%
58	14.898	2005	2008	2012	rVB5	15873	24536	0.29%	0.031%
59	15.010	2025	2027	2032	rVB6	17674	19888	0.23%	0.025%
60	15.063	2032	2036	2039	rBV2	11283	15266	0.18%	0.019%

61	15.110	2040	2044	2046	rBV5	8698	11339	0.13%	0.014%
62	15.310	2075	2078	2082	rVV3	11003	12196	0.14%	0.015%
63	15.351	2082	2085	2090	rVB2	12744	19834	0.23%	0.025%
64	15.475	2099	2106	2112	rBV	4808316	6734290	79.55%	8.388%
65	15.592	2118	2126	2134	rBV	1227227	1700613	20.09%	2.118%

66	15.663	2134	2138	2143	rVV3	54120	85087	1.01%	0.106%
67	15.745	2149	2152	2160	rVB3	47620	75704	0.89%	0.094%
68	15.804	2160	2162	2166	rBV5	9039	9537	0.11%	0.012%
69	16.169	2220	2224	2227	rBV6	7870	13688	0.16%	0.017%
70	16.198	2227	2229	2232	rVV4	11109	14171	0.17%	0.018%

71	16.263	2236	2240	2244	rVB5	18438	29433	0.35%	0.037%
72	16.369	2255	2258	2263	rVB5	21872	32033	0.38%	0.040%
73	16.733	2316	2320	2326	rVB5	36394	59382	0.70%	0.074%
74	16.798	2327	2331	2336	rVB6	21732	35761	0.42%	0.045%
75	16.892	2343	2347	2353	rVB6	31660	61276	0.72%	0.076%

76	16.992	2360	2364	2365	rBV4	9679	13438	0.16%	0.017%
----	--------	------	------	------	------	------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018645.D
 Acq On : 06 Dec 2023 19:45
 Operator : MA/JU
 Sample : 05473-04
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

77	17.104	2380	2383	2390	rVB3	31818	48320	0.57%	0.060%
78	17.228	2398	2404	2409	rBV	2642093	3675449	43.42%	4.578%
79	17.280	2409	2413	2416	rVV	229498	317590	3.75%	0.396%
80	17.328	2416	2421	2429	rVB2	4401725	6286511	74.26%	7.830%
81	17.457	2440	2443	2450	rVB5	30961	53153	0.63%	0.066%
82	17.604	2463	2468	2478	rVB3	85104	137939	1.63%	0.172%
83	18.122	2551	2556	2562	rBV	151103	216751	2.56%	0.270%
84	18.433	2605	2609	2616	rVB2	61218	86836	1.03%	0.108%
85	18.586	2631	2635	2637	rBV2	32982	45663	0.54%	0.057%
86	18.763	2661	2665	2669	rBV2	114453	133569	1.58%	0.166%
87	18.798	2669	2671	2680	rVB5	27792	44480	0.53%	0.055%
88	18.986	2699	2703	2713	rBV6	43660	74696	0.88%	0.093%
89	19.139	2726	2729	2733	rVB3	65723	81638	0.96%	0.102%
90	19.204	2735	2740	2744	rBV4	91648	154445	1.82%	0.192%
91	19.351	2761	2765	2774	rBV3	98556	151780	1.79%	0.189%
92	19.563	2795	2801	2808	rBV	5484761	7252665	85.67%	9.034%
93	19.786	2836	2839	2848	rBV	48669	84218	0.99%	0.105%
94	21.316	3094	3099	3107	rBV	3348575	4114282	48.60%	5.125%
95	23.533	3469	3476	3483	rBV2	4345269	8465815	100.00%	10.545%
96	23.686	3496	3502	3511	rVB	2209141	4357352	51.47%	5.427%




Sum of corrected areas: 80283421

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018645.D
Acq On : 06 Dec 2023 19:45
Operator : MA/JU
Sample : 05473-04
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

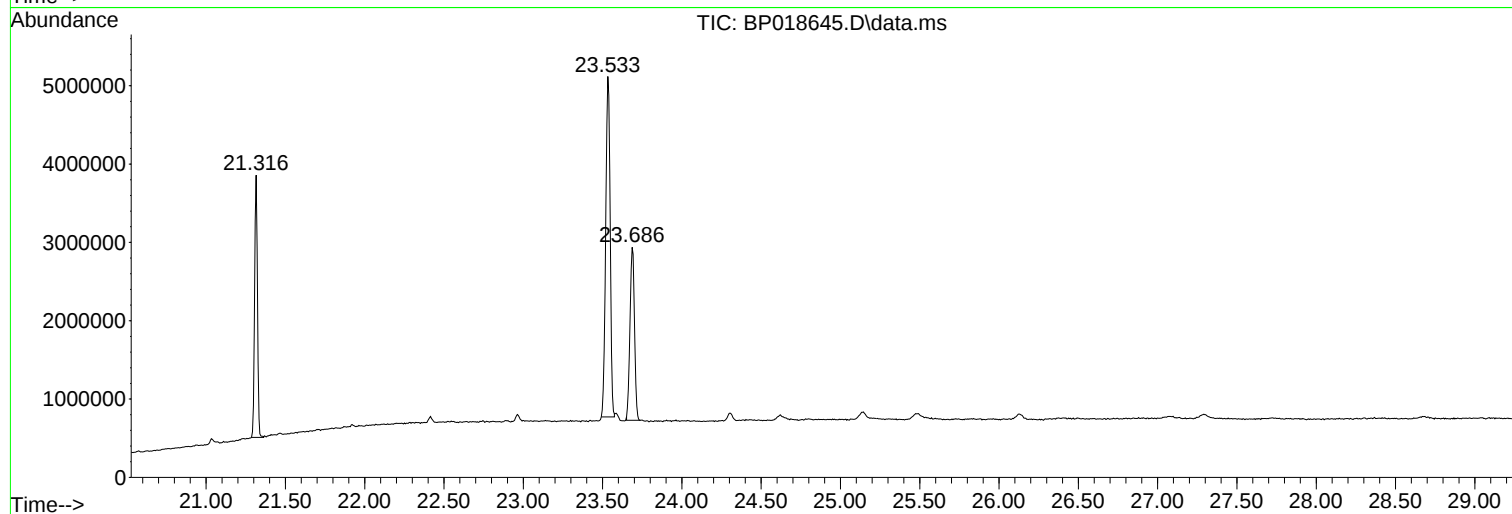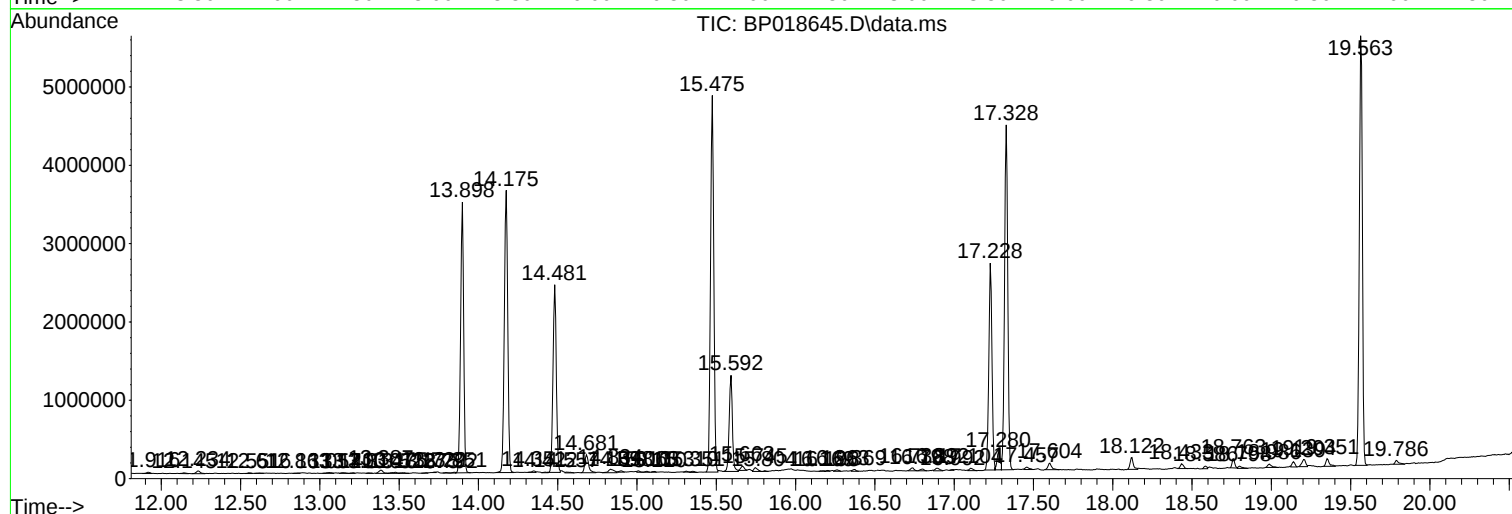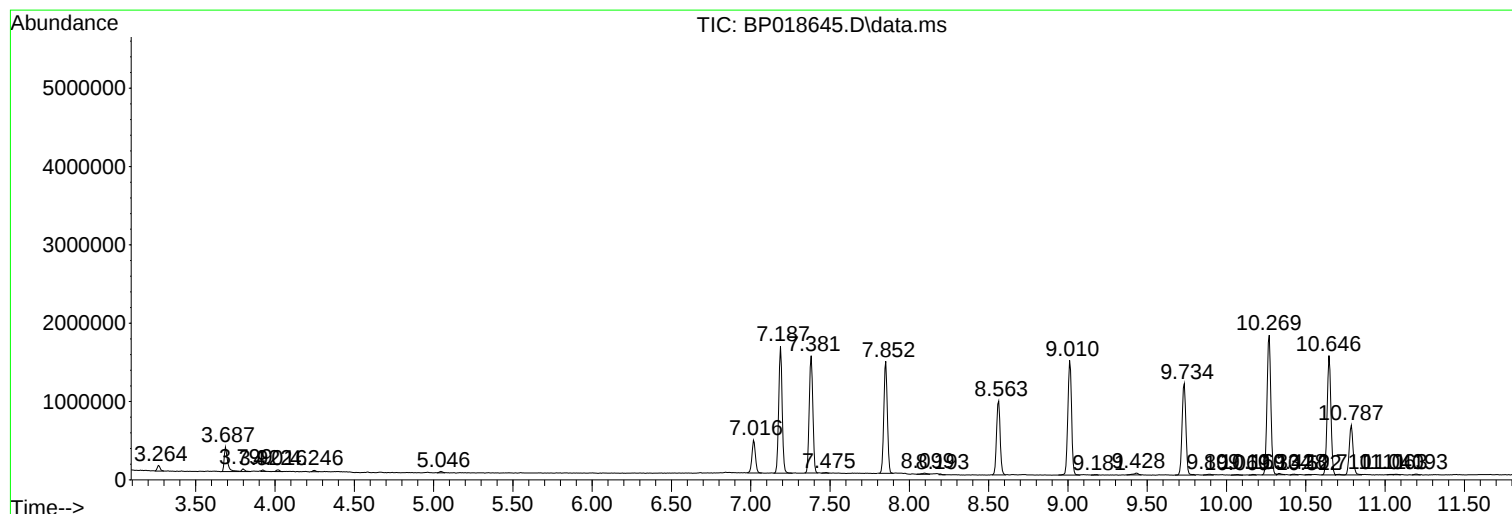

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018645.D
Acq On : 06 Dec 2023 19:45
Operator : MA/JU
Sample : 05473-04
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018645.D
Acq On : 06 Dec 2023 19:45
Operator : MA/JU
Sample : 05473-04
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc