

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018647.D
 Acq On : 06 Dec 2023 20:53
 Operator : MA/JU
 Sample : 05439-14
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018647.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	37	rVB	70622	89327	0.97%	0.120%
2	3.687	99	102	112	rBV	365805	504756	5.49%	0.680%
3	4.017	155	158	166	rVB	25154	32203	0.35%	0.043%
4	5.852	466	470	471	rBV	13448	14912	0.16%	0.020%
5	7.016	663	668	675	rVB	271038	399055	4.34%	0.537%
6	7.187	691	697	704	rBV	935393	1379519	14.99%	1.858%
7	7.305	714	717	718	rBV	8275	9423	0.10%	0.013%
8	7.381	723	730	738	rVV	1043334	1662024	18.07%	2.238%
9	7.469	740	745	753	rVB4	18852	40194	0.44%	0.054%
10	7.852	803	810	819	rBV	1235828	1916648	20.83%	2.581%
11	8.563	924	931	942	rBV	766857	1222501	13.29%	1.646%
12	9.010	1000	1007	1017	rBV	1238679	1998670	21.72%	2.692%
13	9.428	1074	1078	1083	rVB3	16624	26710	0.29%	0.036%
14	9.734	1123	1130	1138	rBV	913589	1495377	16.25%	2.014%
15	10.269	1213	1221	1231	rBV	1418482	2319208	25.21%	3.123%
16	10.646	1278	1285	1294	rVB	1545316	2551520	27.73%	3.436%
17	10.787	1302	1309	1321	rVB	1117552	1847420	20.08%	2.488%
18	11.922	1499	1502	1507	rVB4	15367	21334	0.23%	0.029%
19	12.228	1550	1554	1559	rBV2	27638	48228	0.52%	0.065%
20	13.381	1745	1750	1756	rBV3	35992	63350	0.69%	0.085%
21	13.440	1756	1760	1761	rBV	12244	16528	0.18%	0.022%
22	13.898	1831	1838	1844	rBV	2465155	3533979	38.41%	4.759%
23	14.175	1878	1885	1893	rBV	2950536	4328518	47.05%	5.829%
24	14.481	1930	1937	1946	rBV	2242617	3225189	35.06%	4.344%
25	14.681	1965	1971	1979	rBV	196219	324005	3.52%	0.436%
26	15.475	2099	2106	2115	rBV	3867230	5593403	60.80%	7.533%
27	15.592	2120	2126	2138	rVV	977157	1372539	14.92%	1.848%
28	15.710	2144	2146	2155	rVB3	21168	32157	0.35%	0.043%
29	16.251	2236	2238	2243	rVB6	8748	10767	0.12%	0.015%
30	17.228	2398	2404	2414	rBV	2706292	3808342	41.39%	5.129%
31	17.328	2414	2421	2431	rBV	4506664	6348049	69.00%	8.549%
32	18.116	2551	2555	2560	rBV	102375	135555	1.47%	0.183%
33	18.433	2606	2609	2614	rVB3	25074	38034	0.41%	0.051%
34	18.581	2631	2634	2640	rBV5	22147	36604	0.40%	0.049%
35	19.139	2725	2729	2735	rBV3	66588	93264	1.01%	0.126%
36	19.204	2736	2740	2745	rBV	74958	109305	1.19%	0.147%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018647.D
Acq On : 06 Dec 2023 20:53
Operator : MA/JU
Sample : 05439-14
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.351	2762	2765	2771	rBV4	36266	38832	0.42%	0.052%
38	19.563	2795	2801	2807	rBV	6167003	8156532	88.66%	10.985%
39	21.033	3048	3051	3061	rBV3	122122	193304	2.10%	0.260%
40	21.316	3093	3099	3105	rBV	3649836	4777026	51.92%	6.433%
41	23.533	3468	3476	3483	rBV2	4594628	9200070	100.00%	12.390%
42	23.686	3495	3502	3512	rVB	2723698	5238794	56.94%	7.055%




Sum of corrected areas: 74253175

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018647.D
Acq On : 06 Dec 2023 20:53
Operator : MA/JU
Sample : 05439-14
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

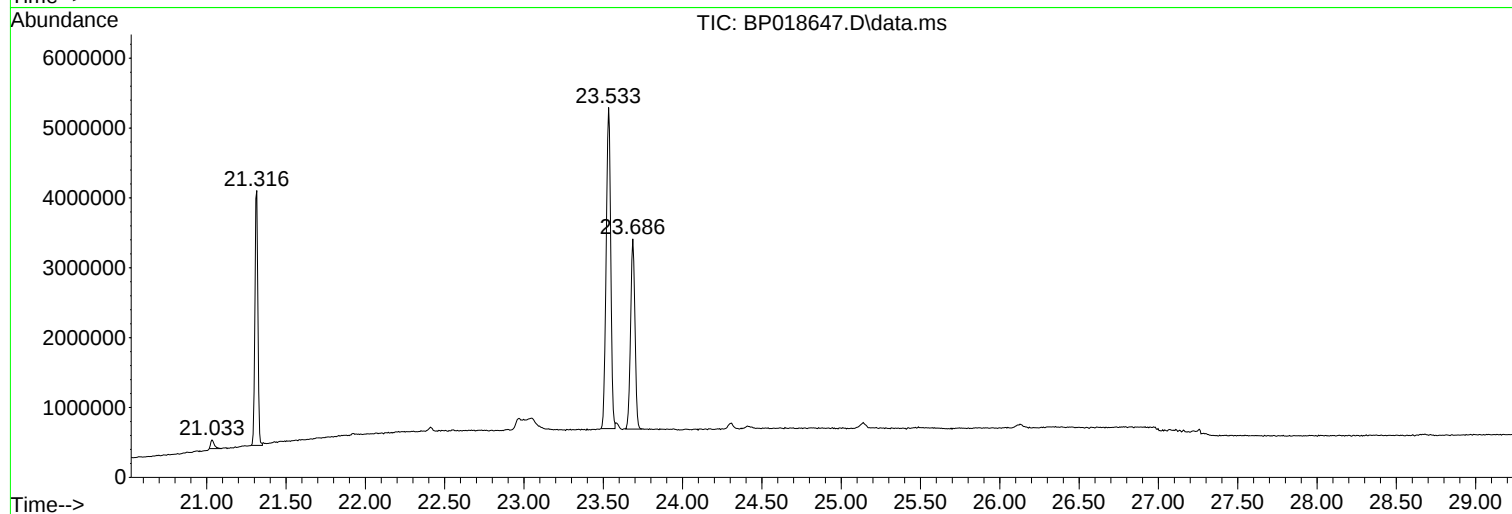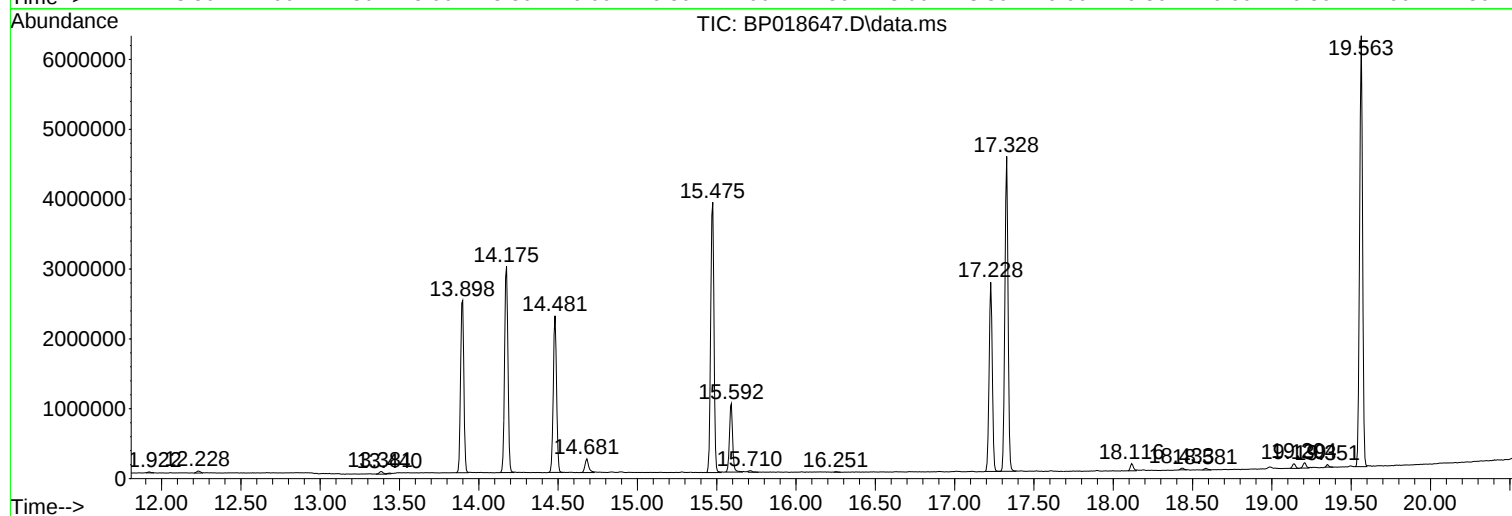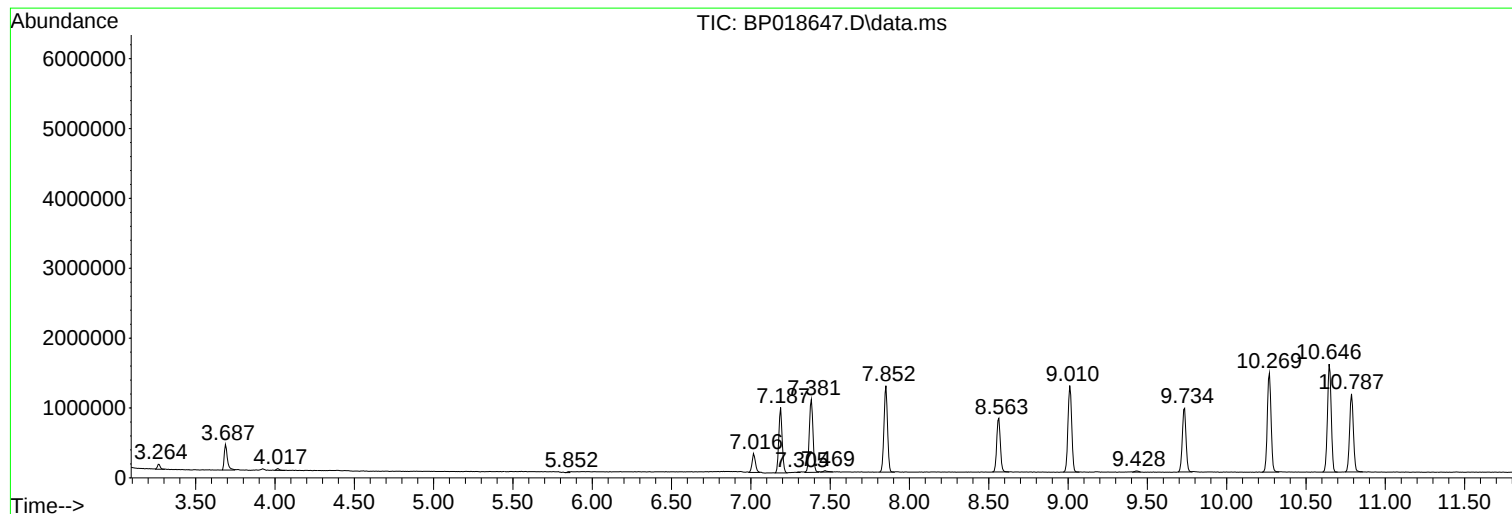

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018647.D
Acq On : 06 Dec 2023 20:53
Operator : MA/JU
Sample : 05439-14
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018647.D
Acq On : 06 Dec 2023 20:53
Operator : MA/JU
Sample : 05439-14
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc