

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018648.D
 Acq On : 06 Dec 2023 21:27
 Operator : MA/JU
 Sample : 05439-15
 Misc :
 ALS Vial : 85 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	27	30	37	rVB	67726	80985	1.03%	0.098%
2	3.546	76	78	83	rVB	7962	9882	0.13%	0.012%
3	3.687	98	102	111	rBV	174705	256367	3.25%	0.311%
4	3.793	115	120	124	rBV2	15841	35825	0.45%	0.043%
5	3.922	137	142	147	rVB3	22213	50901	0.65%	0.062%
6	4.016	152	158	163	rBV2	37773	71090	0.90%	0.086%
7	4.304	200	207	208	rBV2	11769	23926	0.30%	0.029%
8	5.222	357	363	367	rBV	11237	27607	0.35%	0.033%
9	5.869	468	473	476	rBV	7583	10940	0.14%	0.013%
10	5.981	487	492	494	rBV	12782	16683	0.21%	0.020%
11	6.516	579	583	585	rBV2	5893	8107	0.10%	0.010%
12	7.016	662	668	678	rVB	311481	492792	6.25%	0.598%
13	7.187	691	697	707	rBV	1240140	1910816	24.23%	2.318%
14	7.381	722	730	737	rBV	1143743	1771808	22.46%	2.149%
15	7.469	740	745	750	rBV2	16220	24864	0.32%	0.030%
16	7.851	802	810	817	rBV	1353096	2078301	26.35%	2.521%
17	8.563	924	931	940	rBV	915642	1492397	18.92%	1.810%
18	9.010	999	1007	1019	rVB	1483864	2435284	30.87%	2.954%
19	9.134	1022	1028	1029	rBV6	5794	9022	0.11%	0.011%
20	9.181	1032	1036	1041	rVV5	7560	16547	0.21%	0.020%
21	9.251	1046	1048	1053	rBV2	5522	10324	0.13%	0.013%
22	9.434	1075	1079	1085	rVB4	16076	25265	0.32%	0.031%
23	9.734	1122	1130	1139	rBV	1097488	1819075	23.06%	2.207%
24	10.269	1213	1221	1234	rBV	1733560	2903556	36.81%	3.522%
25	10.645	1278	1285	1295	rVB	1917474	3163669	40.11%	3.837%
26	10.786	1302	1309	1325	rVB	1079208	1811110	22.96%	2.197%
27	11.433	1416	1419	1428	rBV3	10758	23162	0.29%	0.028%
28	11.922	1499	1502	1508	rVB3	13932	22329	0.28%	0.027%
29	12.233	1550	1555	1559	rBV	36260	55881	0.71%	0.068%
30	12.375	1578	1579	1582	rVB	12601	10990	0.14%	0.013%
31	12.457	1584	1593	1595	rBV9	10997	23150	0.29%	0.028%
32	13.386	1745	1751	1756	rVB2	50183	79301	1.01%	0.096%
33	13.451	1760	1762	1767	rVB3	6557	8851	0.11%	0.011%
34	13.898	1830	1838	1844	rBV	3658026	5209418	66.05%	6.319%
35	14.174	1875	1885	1895	rBV	4058423	5873429	74.46%	7.124%
36	14.480	1930	1937	1944	rBV	2944347	4352367	55.18%	5.279%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018648.D
 Acq On : 06 Dec 2023 21:27
 Operator : MA/JU
 Sample : 05439-15
 Misc :
 ALS Vial : 85 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	14.569	1948	1952	1955	rVV3	5896	9425	0.12%	0.011%
38	14.680	1965	1971	1981	rBV2	222173	360521	4.57%	0.437%
39	14.839	1993	1998	2002	rVB5	9098	13473	0.17%	0.016%
40	14.898	2003	2008	2012	rVB8	13188	22082	0.28%	0.027%
41	15.474	2099	2106	2114	rBV	5285433	7676433	97.32%	9.311%
42	15.592	2119	2126	2140	rVV	1216517	1763546	22.36%	2.139%
43	15.710	2142	2146	2158	rVB3	30857	66680	0.85%	0.081%
44	16.251	2235	2238	2244	rBV7	8668	13833	0.18%	0.017%
45	16.910	2346	2350	2354	rVB2	9648	16396	0.21%	0.020%
46	17.227	2397	2404	2414	rBV	3197296	4617374	58.54%	5.601%
47	17.327	2414	2421	2432	rVV	5493653	7604396	96.41%	9.224%
48	18.115	2550	2555	2561	rBV2	114592	163375	2.07%	0.198%
49	18.192	2565	2568	2573	rVV3	10500	16979	0.22%	0.021%
50	18.433	2606	2609	2614	rBV4	20533	27250	0.35%	0.033%
51	18.586	2632	2635	2640	rVB4	19606	22438	0.28%	0.027%
52	19.139	2725	2729	2733	rBV	70614	92900	1.18%	0.113%
53	19.204	2736	2740	2744	rBV	74744	112028	1.42%	0.136%
54	19.351	2762	2765	2772	rBV	75132	89416	1.13%	0.108%
55	19.562	2795	2801	2812	rBV	6139999	7887585	100.00%	9.568%
56	21.315	3094	3099	3104	rBV	3028889	3912734	49.61%	4.746%
57	23.533	3469	3476	3494	rVB2	3856181	7579283	96.09%	9.194%
58	23.686	3495	3502	3515	rVB	2074418	4157216	52.71%	5.043%




Sum of corrected areas: 82441384

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018648.D
Acq On : 06 Dec 2023 21:27
Operator : MA/JU
Sample : 05439-15
Misc :
ALS Vial : 85 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

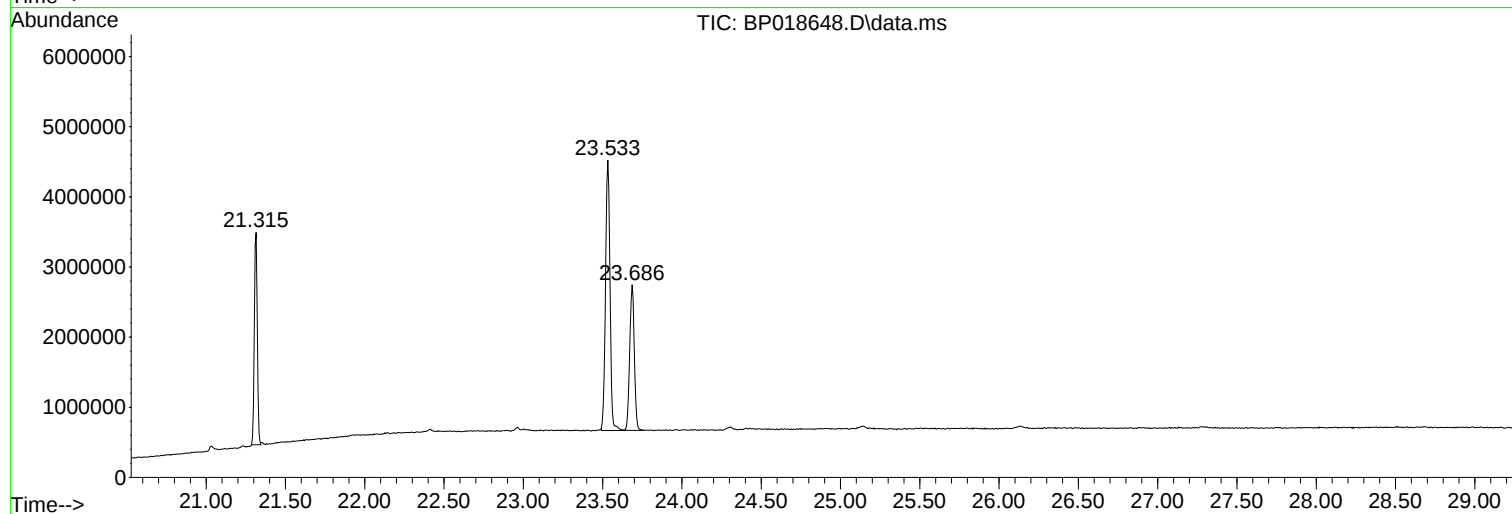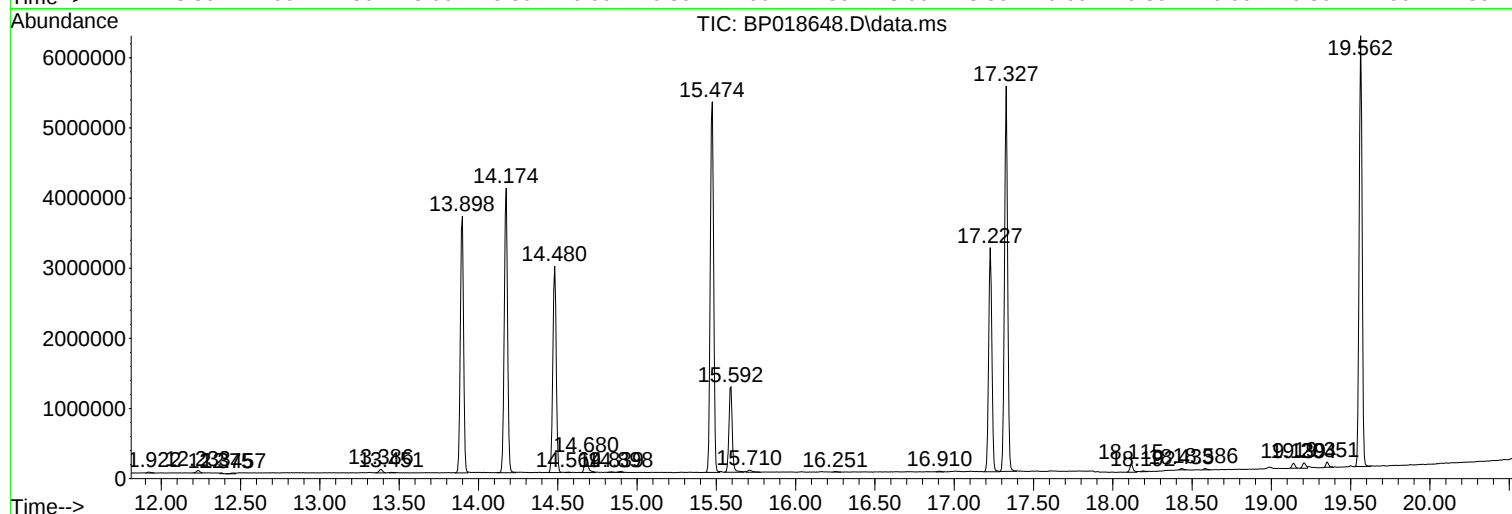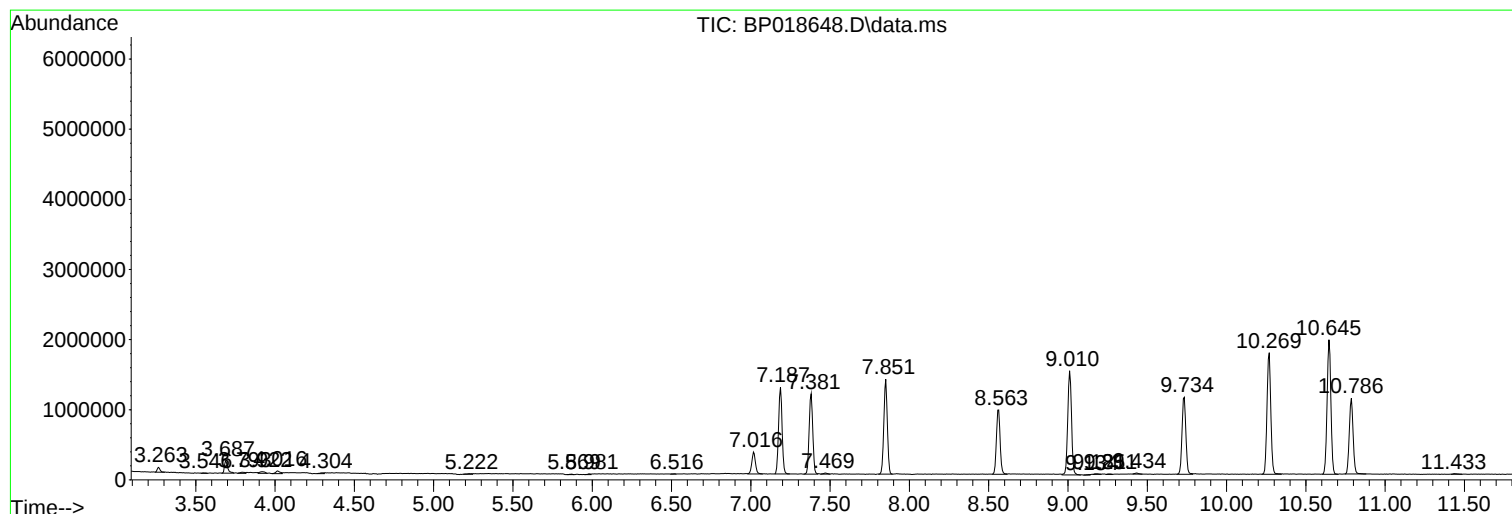

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018648.D
Acq On : 06 Dec 2023 21:27
Operator : MA/JU
Sample : 05439-15
Misc :
ALS Vial : 85 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018648.D
Acq On : 06 Dec 2023 21:27
Operator : MA/JU
Sample : 05439-15
Misc :
ALS Vial : 85 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
