

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018649.D
 Acq On : 06 Dec 2023 22:01
 Operator : MA/JU
 Sample : 05439-16
 Misc :
 ALS Vial : 86 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018649.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	40	rVB	76494	99421	1.34%	0.123%
2	3.687	98	102	118	rBV	413178	601131	8.10%	0.741%
3	3.922	139	142	147	rVB2	20450	25109	0.34%	0.031%
4	4.017	155	158	162	rVB	22458	25069	0.34%	0.031%
5	5.128	344	347	352	rVB	14034	20344	0.27%	0.025%
6	5.269	367	371	372	rBV	10242	10304	0.14%	0.013%
7	6.840	636	638	642	rVB	8747	10718	0.14%	0.013%
8	7.016	662	668	677	rVB	342703	529027	7.13%	0.652%
9	7.187	690	697	705	rBV	1346616	2082568	28.08%	2.567%
10	7.381	723	730	738	rBV	1214951	1903847	25.67%	2.346%
11	7.469	742	745	752	rVB4	18074	32114	0.43%	0.040%
12	7.852	801	810	818	rBV	1156648	1839616	24.80%	2.267%
13	7.916	818	821	826	rBV6	6002	11489	0.15%	0.014%
14	8.563	922	931	939	rBV	765829	1254544	16.91%	1.546%
15	9.010	1000	1007	1016	rBV	1235576	1977541	26.66%	2.437%
16	9.434	1075	1079	1085	rVB5	9895	14826	0.20%	0.018%
17	9.734	1122	1130	1138	rBV	936996	1565897	21.11%	1.930%
18	10.269	1212	1221	1229	rBV	1450599	2425309	32.70%	2.989%
19	10.522	1258	1264	1265	rBV5	7236	10337	0.14%	0.013%
20	10.646	1278	1285	1292	rBV	1619054	2691174	36.28%	3.317%
21	10.787	1301	1309	1323	rBV	1249047	2069511	27.90%	2.551%
22	11.440	1410	1420	1422	rBV8	7391	13732	0.19%	0.017%
23	12.234	1548	1555	1561	rBV2	31143	54188	0.73%	0.067%
24	13.387	1746	1751	1756	rVB2	52877	89385	1.21%	0.110%
25	13.451	1758	1762	1766	rBV4	6599	11923	0.16%	0.015%
26	13.763	1807	1815	1816	rBV2	9694	21577	0.29%	0.027%
27	13.898	1831	1838	1847	rBV	3744857	5120948	69.04%	6.311%
28	14.175	1878	1885	1895	rBV	4036944	6017378	81.12%	7.416%
29	14.481	1930	1937	1947	rBV	3277640	4703856	63.41%	5.797%
30	14.681	1965	1971	1981	rBV	220004	356180	4.80%	0.439%
31	14.834	1995	1997	2004	rVB6	12941	16775	0.23%	0.021%
32	14.898	2004	2008	2014	rVB9	12345	19028	0.26%	0.023%
33	15.475	2099	2106	2116	rBV	5079744	7417778	100.00%	9.142%
34	15.592	2120	2126	2141	rVV	1167557	1692932	22.82%	2.086%
35	15.710	2143	2146	2158	rVB4	25927	50987	0.69%	0.063%
36	17.228	2397	2404	2411	rBV	3468872	4823044	65.02%	5.944%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018649.D
Acq On : 06 Dec 2023 22:01
Operator : MA/JU
Sample : 05439-16
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	17.328	2414	2421	2432	rVV2	4879650	7110801	95.86%	8.763%
38	18.116	2551	2555	2561	rBV2	150895	208663	2.81%	0.257%
39	19.139	2726	2729	2734	rVB2	63287	80956	1.09%	0.100%
40	19.204	2736	2740	2748	rBV	71993	106124	1.43%	0.131%
41	19.351	2762	2765	2769	rBV3	38256	40951	0.55%	0.050%
42	19.563	2795	2801	2807	rBV	5508444	7408028	99.87%	9.130%
43	21.033	3048	3051	3058	rBV3	145146	254361	3.43%	0.313%
44	21.316	3094	3099	3104	rBV	3519666	4288636	57.82%	5.285%
45	23.533	3469	3476	3484	rBV2	3829871	7338621	98.93%	9.044%
46	23.686	3496	3502	3512	rVB	2413250	4694488	63.29%	5.786%




Sum of corrected areas: 81141236

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018649.D
Acq On : 06 Dec 2023 22:01
Operator : MA/JU
Sample : 05439-16
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

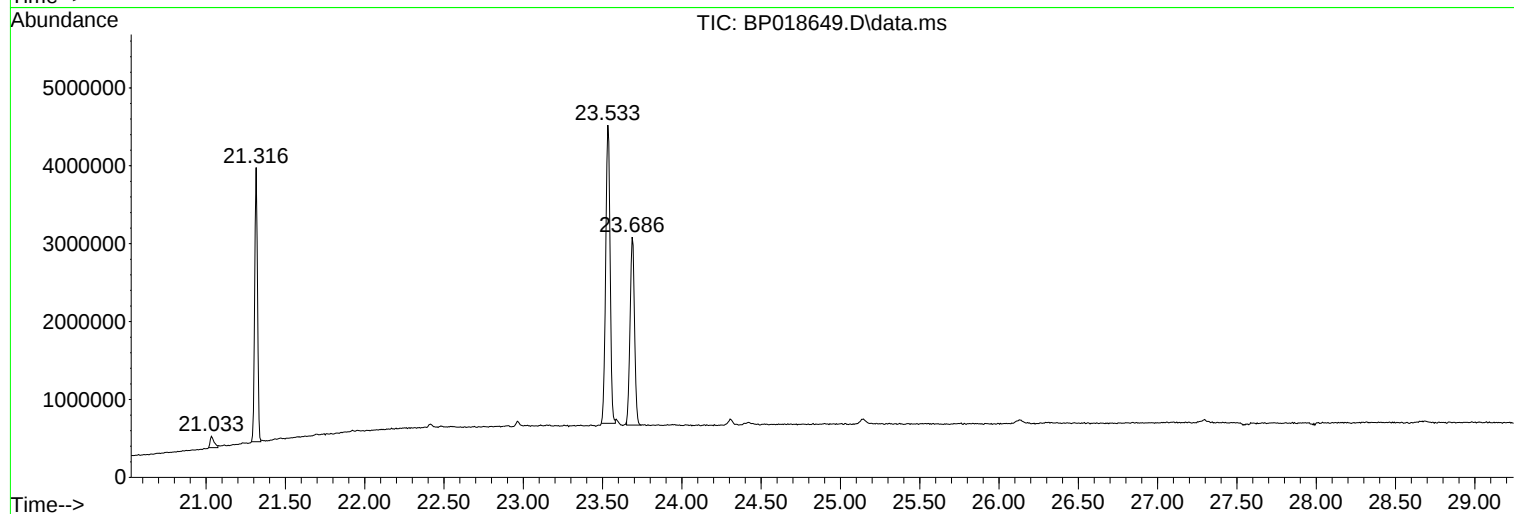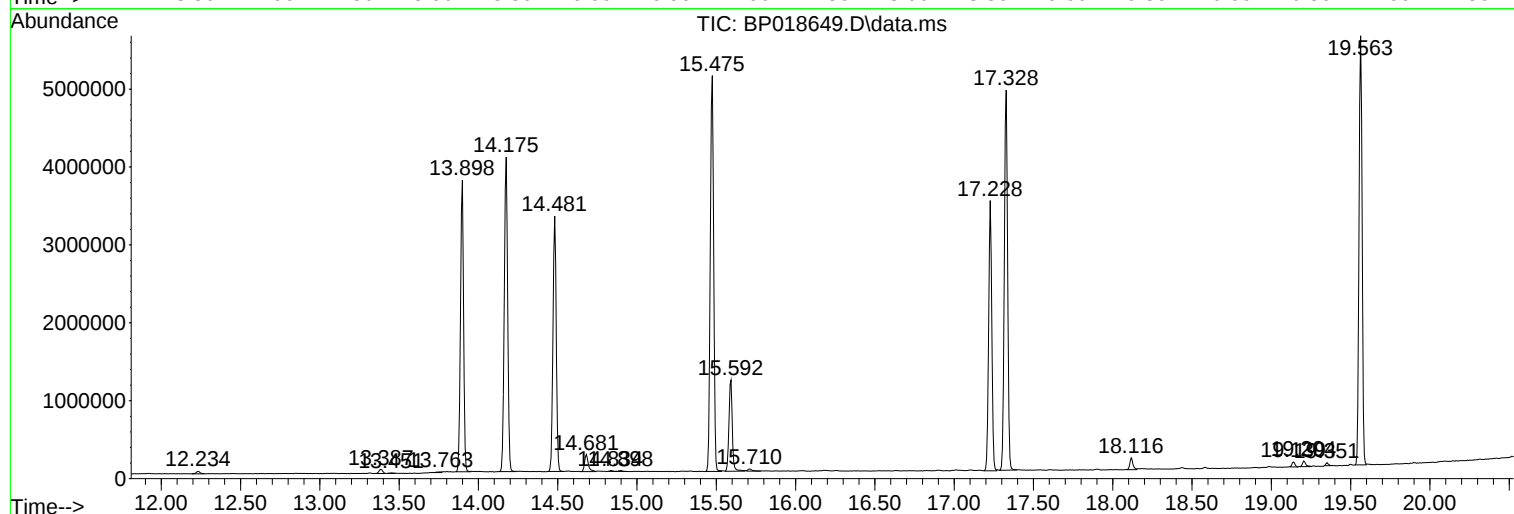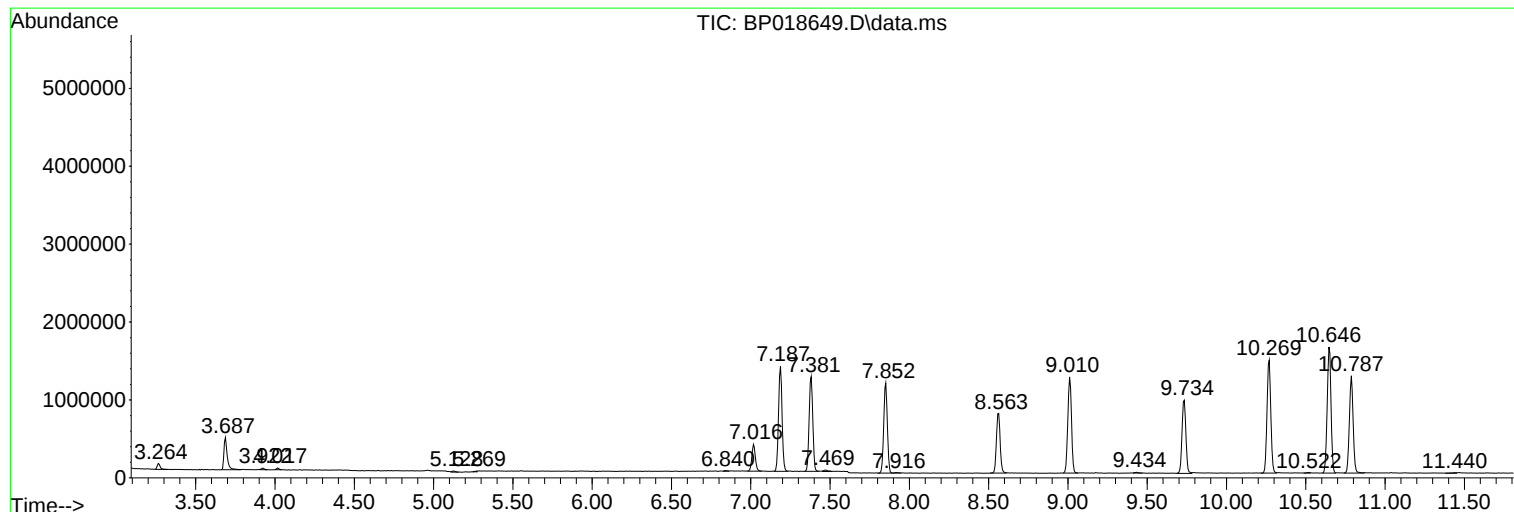

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018649.D
Acq On : 06 Dec 2023 22:01
Operator : MA/JU
Sample : 05439-16
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018649.D
Acq On : 06 Dec 2023 22:01
Operator : MA/JU
Sample : 05439-16
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc