

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018650.D
 Acq On : 06 Dec 2023 22:35
 Operator : MA/JU
 Sample : 05439-17
 Misc :
 ALS Vial : 87 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018650.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	42	rVB	94013	135257	1.66%	0.152%
2	3.687	98	102	115	rBV	343797	495315	6.06%	0.556%
3	3.922	137	142	147	rBV2	21614	34770	0.43%	0.039%
4	4.017	155	158	162	rVB	21957	24301	0.30%	0.027%
5	4.581	251	254	258	rVB3	5818	8500	0.10%	0.010%
6	6.452	567	572	575	rBV4	6023	11761	0.14%	0.013%
7	6.840	633	638	640	rBV2	10181	15222	0.19%	0.017%
8	7.016	661	668	678	rVB	410913	641247	7.85%	0.720%
9	7.187	690	697	708	rVB	1406617	2127925	26.05%	2.388%
10	7.381	722	730	739	rBV	1367177	2138136	26.18%	2.399%
11	7.463	739	744	751	rVV3	30900	54867	0.67%	0.062%
12	7.852	803	810	817	rVB	1455253	2269315	27.79%	2.546%
13	7.899	817	818	825	rVB2	9197	13155	0.16%	0.015%
14	7.975	825	831	832	rBV	8479	13455	0.16%	0.015%
15	8.557	922	930	942	rBV	1127282	1845299	22.59%	2.071%
16	8.734	956	960	964	rBV3	6246	10551	0.13%	0.012%
17	9.010	999	1007	1015	rBV	1624784	2599572	31.83%	2.917%
18	9.128	1025	1027	1032	rVB5	8714	9807	0.12%	0.011%
19	9.428	1071	1078	1084	rVB4	19730	39223	0.48%	0.044%
20	9.734	1121	1130	1137	rBV	1338100	2214708	27.12%	2.485%
21	9.957	1165	1168	1170	rBV2	8091	9718	0.12%	0.011%
22	10.269	1213	1221	1234	rBV	2045717	3438934	42.11%	3.859%
23	10.510	1258	1262	1266	rBV3	16936	24625	0.30%	0.028%
24	10.646	1277	1285	1293	rBV	2060353	3419485	41.87%	3.837%
25	10.787	1300	1309	1327	rBV	1563770	2690367	32.94%	3.019%
26	11.040	1345	1352	1361	rBV	16989	63244	0.77%	0.071%
27	11.299	1393	1396	1398	rBV2	6489	8519	0.10%	0.010%
28	11.463	1411	1424	1431	rBV2	58867	127540	1.56%	0.143%
29	11.922	1498	1502	1508	rVB3	19512	29427	0.36%	0.033%
30	12.093	1529	1531	1537	rVB2	6793	11431	0.14%	0.013%
31	12.234	1549	1555	1561	rVB3	36938	68964	0.84%	0.077%
32	12.422	1583	1587	1590	rBV3	6949	11637	0.14%	0.013%
33	12.610	1613	1619	1621	rBV6	9004	15528	0.19%	0.017%
34	13.381	1746	1750	1758	rVB2	31709	49678	0.61%	0.056%
35	13.451	1758	1762	1764	rBV2	9621	13179	0.16%	0.015%
36	13.710	1801	1806	1808	rBV5	7825	10374	0.13%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018650.D
 Acq On : 06 Dec 2023 22:35
 Operator : MA/JU
 Sample : 05439-17
 Misc :
 ALS Vial : 87 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	13.898	1831	1838	1849	rBV	3668136	5151108	63.07%	5.780%
38	14.004	1852	1856	1862	rVB6	6880	12072	0.15%	0.014%
39	14.175	1875	1885	1892	rBV	4460508	6300606	77.15%	7.070%
40	14.381	1919	1920	1925	rVB3	8399	8249	0.10%	0.009%
41	14.481	1927	1937	1944	rBV	3239349	4630038	56.69%	5.195%
42	14.563	1949	1951	1957	rVB6	8337	10382	0.13%	0.012%
43	14.681	1964	1971	1982	rBV	304021	489977	6.00%	0.550%
44	14.834	1994	1997	2002	rVB2	20973	32789	0.40%	0.037%
45	14.898	2004	2008	2012	rVB6	16279	27006	0.33%	0.030%
46	15.275	2066	2072	2075	rBV3	9383	23978	0.29%	0.027%
47	15.475	2099	2106	2119	rBV	5467115	7956793	97.42%	8.928%
48	15.592	2119	2126	2136	rBV	1474794	2079757	25.46%	2.334%
49	15.710	2143	2146	2150	rVB2	23587	30838	0.38%	0.035%
50	17.016	2358	2368	2372	rBV3	27239	81869	1.00%	0.092%
51	17.104	2380	2383	2385	rBV3	12104	13728	0.17%	0.015%
52	17.228	2398	2404	2410	rBV	3371352	4738769	58.02%	5.317%
53	17.275	2410	2412	2415	rVV4	29233	38468	0.47%	0.043%
54	17.328	2415	2421	2433	rVB	5295551	7386929	90.45%	8.289%
55	17.598	2463	2467	2475	rBV4	19451	36653	0.45%	0.041%
56	17.904	2516	2519	2523	rVB2	27280	32529	0.40%	0.037%
57	18.116	2551	2555	2565	rBV	137192	201746	2.47%	0.226%
58	18.433	2605	2609	2619	rVB2	47181	72469	0.89%	0.081%
59	18.586	2631	2635	2638	rBV3	36011	44966	0.55%	0.050%
60	18.986	2700	2703	2705	rBV4	29617	38658	0.47%	0.043%
61	19.039	2709	2712	2716	rVB4	31074	39403	0.48%	0.044%
62	19.139	2725	2729	2734	rVB	76299	96922	1.19%	0.109%
63	19.204	2736	2740	2744	rBV2	89885	130513	1.60%	0.146%
64	19.351	2762	2765	2770	rBV3	69459	85330	1.04%	0.096%
65	19.563	2795	2801	2809	rBV	6414827	8167137	100.00%	9.164%
66	21.316	3094	3099	3104	rBV	3327137	4128896	50.55%	4.633%
67	23.533	3469	3476	3483	rBV2	4174379	7861069	96.25%	8.821%
68	23.686	3496	3502	3515	rVB	2269347	4475445	54.80%	5.022%




Sum of corrected areas: 89120128

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018650.D
Acq On : 06 Dec 2023 22:35
Operator : MA/JU
Sample : 05439-17
Misc :
ALS Vial : 87 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

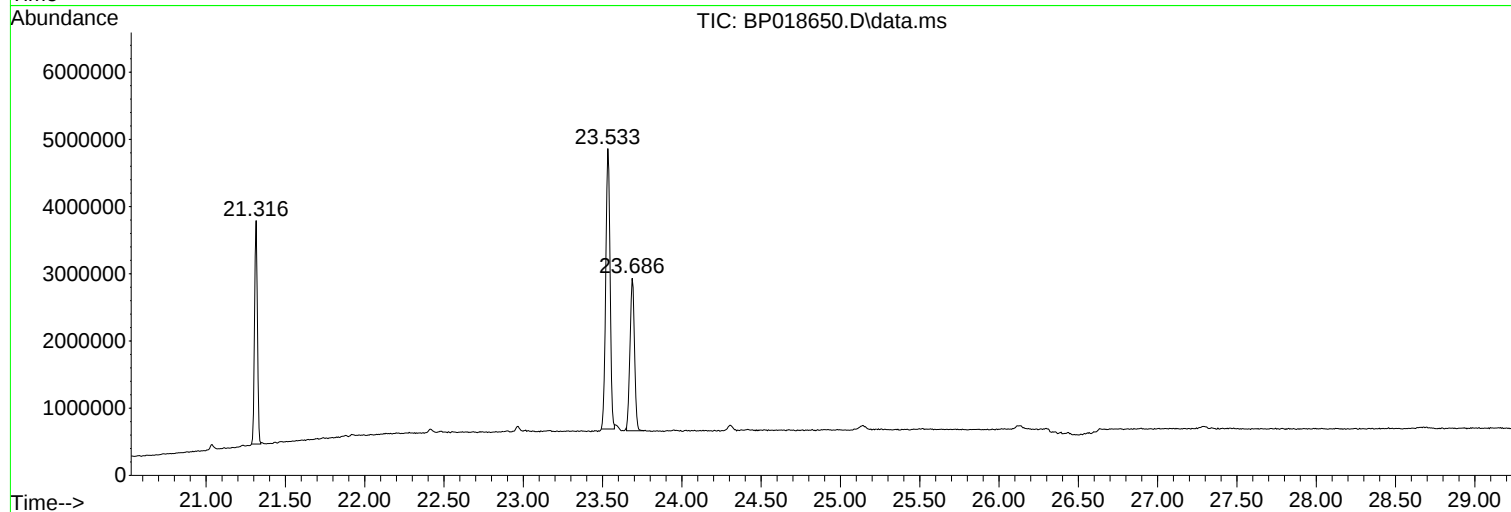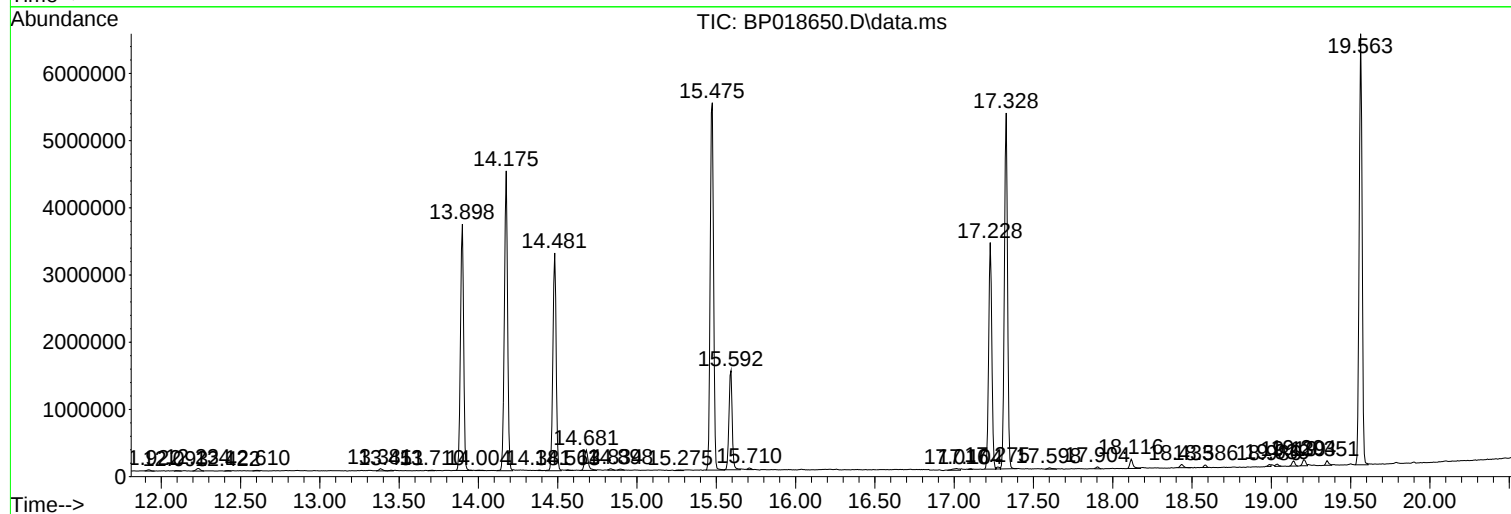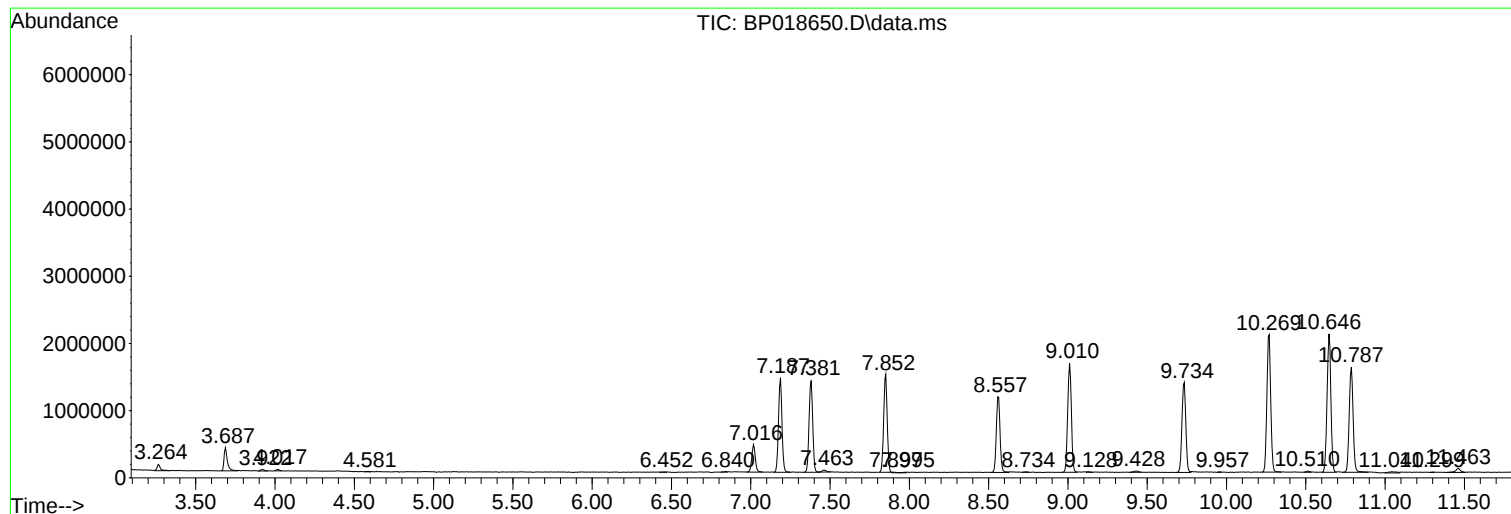

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018650.D
Acq On : 06 Dec 2023 22:35
Operator : MA/JU
Sample : 05439-17
Misc :
ALS Vial : 87 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018650.D
Acq On : 06 Dec 2023 22:35
Operator : MA/JU
Sample : 05439-17
Misc :
ALS Vial : 87 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc