

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018651.D
 Acq On : 06 Dec 2023 23:09
 Operator : MA/JU
 Sample : 05439-18
 Misc :
 ALS Vial : 88 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COAE0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018651.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	40	rVB	77687	107327	1.31%	0.126%
2	3.687	98	102	115	rBV	430774	612314	7.50%	0.717%
3	4.017	154	158	163	rVB	28726	39908	0.49%	0.047%
4	7.016	662	668	678	rVB	339863	540590	6.62%	0.633%
5	7.187	690	697	709	rVB	1349749	2075144	25.42%	2.429%
6	7.381	723	730	738	rBV	1186151	1844994	22.60%	2.160%
7	7.458	739	743	751	rVB2	42415	73425	0.90%	0.086%
8	7.852	803	810	818	rVV	1368736	2179049	26.69%	2.551%
9	7.916	818	821	825	rVB3	7351	10335	0.13%	0.012%
10	8.557	924	930	939	rBV	1008046	1620463	19.85%	1.897%
11	9.010	1000	1007	1016	rBV	1566548	2507098	30.71%	2.935%
12	9.434	1077	1079	1083	rVB4	7564	8874	0.11%	0.010%
13	9.734	1122	1130	1139	rBV	911788	1530088	18.74%	1.791%
14	10.269	1212	1221	1229	rBV	1455966	2463303	30.17%	2.884%
15	10.434	1242	1249	1251	rBV	8514	19840	0.24%	0.023%
16	10.646	1278	1285	1294	rVB	1972579	3256938	39.89%	3.813%
17	10.787	1302	1309	1323	rBV	1703791	2873483	35.20%	3.364%
18	11.434	1417	1419	1426	rVB2	6399	10094	0.12%	0.012%
19	11.916	1498	1501	1508	rVB4	14437	23470	0.29%	0.027%
20	12.234	1549	1555	1561	rBV3	36554	60833	0.75%	0.071%
21	13.304	1735	1737	1743	rVB3	5885	9055	0.11%	0.011%
22	13.381	1745	1750	1758	rBV2	45366	75658	0.93%	0.089%
23	13.451	1758	1762	1767	rVV4	5252	9389	0.12%	0.011%
24	13.710	1803	1806	1810	rVB3	9503	10073	0.12%	0.012%
25	13.892	1831	1837	1849	rBV	3602948	5138003	62.94%	6.015%
26	14.169	1878	1884	1892	rBV2	3928419	6037588	73.95%	7.068%
27	14.481	1930	1937	1945	rBV	3064373	4508450	55.22%	5.278%
28	14.604	1955	1958	1962	rVB4	14962	16015	0.20%	0.019%
29	14.681	1965	1971	1981	rBV	198173	340313	4.17%	0.398%
30	14.839	1994	1998	2003	rVB6	11134	17406	0.21%	0.020%
31	14.898	2005	2008	2012	rVB4	17339	22700	0.28%	0.027%
32	15.469	2098	2105	2113	rBV	5200740	7803333	95.58%	9.135%
33	15.586	2119	2125	2133	rBV	1187247	1600988	19.61%	1.874%
34	15.710	2142	2146	2153	rVB2	28262	48473	0.59%	0.057%
35	16.039	2196	2202	2207	rBV10	11300	23051	0.28%	0.027%
36	16.386	2258	2261	2267	rVB3	21994	30189	0.37%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018651.D
 Acq On : 06 Dec 2023 23:09
 Operator : MA/JU
 Sample : 05439-18
 Misc :
 ALS Vial : 88 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AE0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.228	2397	2404	2410	rBV	3396821	4734787	58.00%	5.543%
38	17.328	2414	2421	2433	rVB	5356118	7721962	94.59%	9.040%
39	17.898	2516	2518	2522	rVB4	24748	30665	0.38%	0.036%
40	18.116	2551	2555	2561	rBV2	144000	188271	2.31%	0.220%
41	18.433	2606	2609	2613	rBV3	21728	30527	0.37%	0.036%
42	19.033	2709	2711	2717	rVB6	41973	50615	0.62%	0.059%
43	19.139	2725	2729	2733	rBV	73484	92293	1.13%	0.108%
44	19.204	2736	2740	2745	rBV	80103	111288	1.36%	0.130%
45	19.351	2762	2765	2770	rBV4	48251	61483	0.75%	0.072%
46	19.563	2795	2801	2807	rBV	6223571	8163905	100.00%	9.558%
47	21.316	3093	3099	3108	rBV	3196214	4217147	51.66%	4.937%
48	23.533	3468	3476	3483	rBV	4145407	7935557	97.20%	9.290%
49	23.686	3495	3502	3512	rVB	2253258	4531395	55.51%	5.305%




Sum of corrected areas: 85418149

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018651.D
Acq On : 06 Dec 2023 23:09
Operator : MA/JU
Sample : 05439-18
Misc :
ALS Vial : 88 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

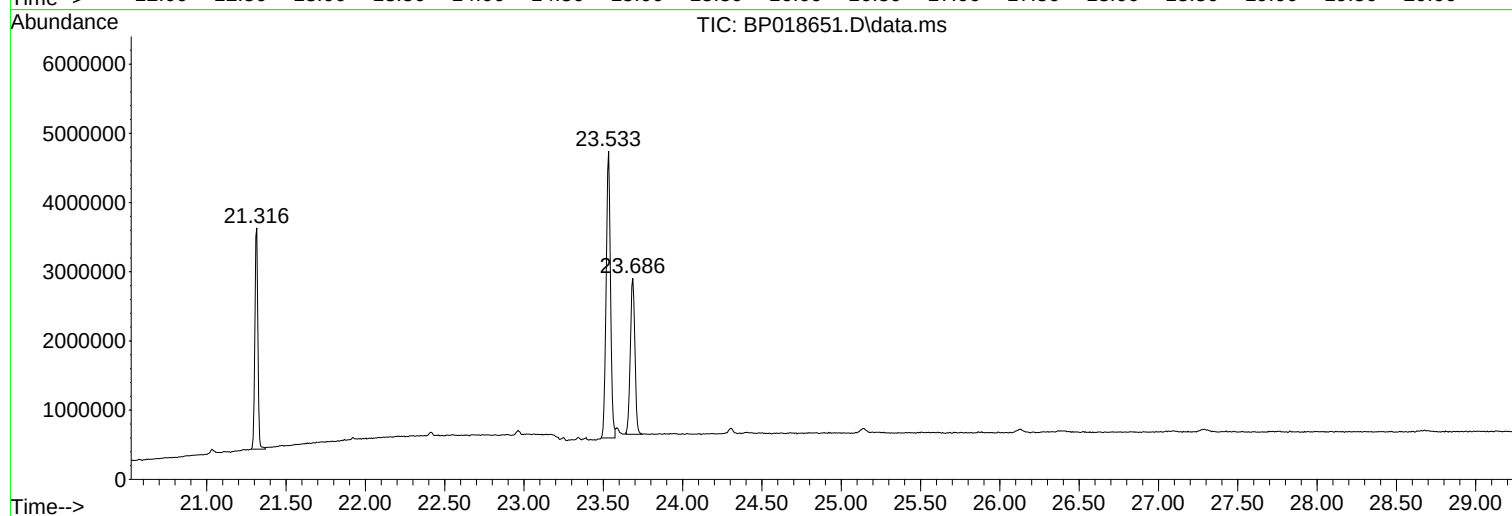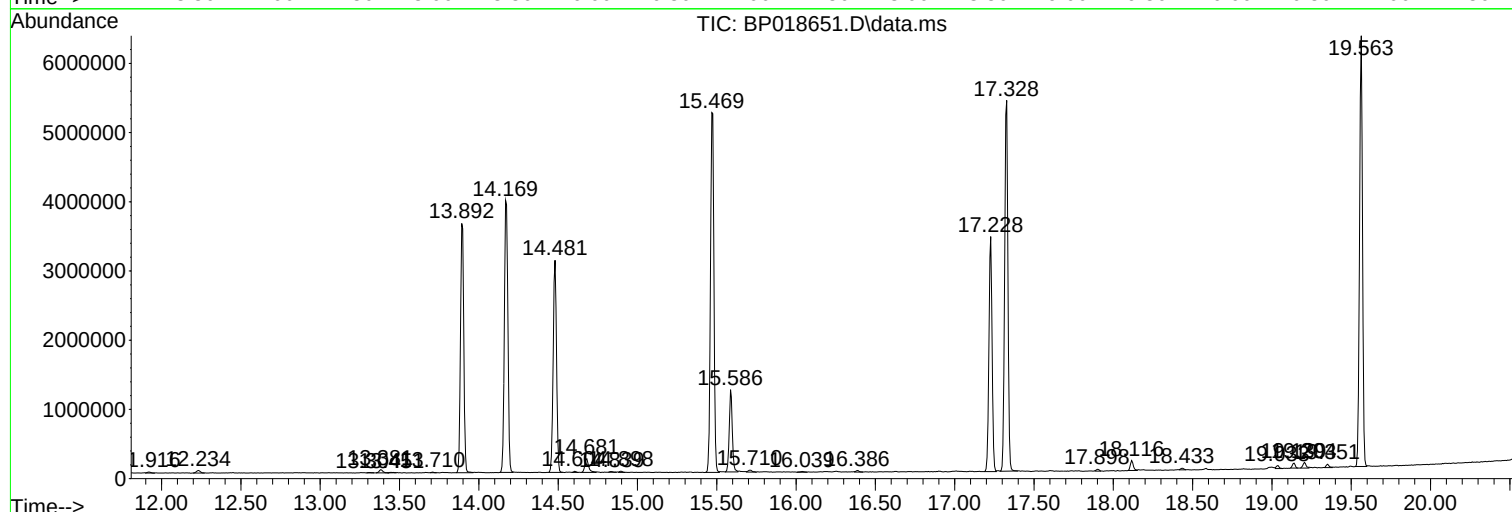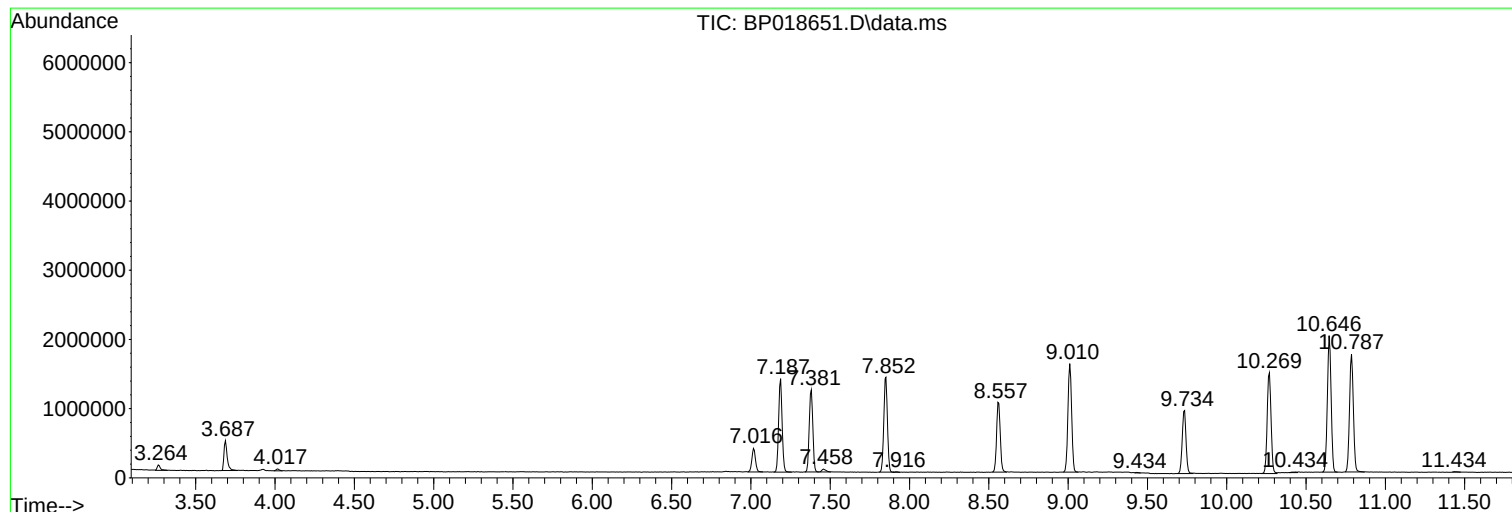

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018651.D
Acq On : 06 Dec 2023 23:09
Operator : MA/JU
Sample : 05439-18
Misc :
ALS Vial : 88 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018651.D
Acq On : 06 Dec 2023 23:09
Operator : MA/JU
Sample : 05439-18
Misc :
ALS Vial : 88 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc