

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018652.D
 Acq On : 06 Dec 2023 23:42
 Operator : MA/JU
 Sample : 05439-07
 Misc :
 ALS Vial : 89 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018652.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	37	rVB	83082	105100	1.26%	0.137%
2	3.687	98	102	115	rBV	352253	500299	6.00%	0.652%
3	3.922	138	142	146	rVB	19855	27438	0.33%	0.036%
4	4.016	155	158	162	rVB2	22989	28006	0.34%	0.036%
5	6.940	651	655	657	rBV3	7646	12641	0.15%	0.016%
6	7.016	662	668	677	rVB	312507	478528	5.74%	0.623%
7	7.187	690	697	706	rBV	1328890	2037983	24.46%	2.655%
8	7.381	723	730	737	rVB	1171595	1849726	22.20%	2.410%
9	7.463	740	744	751	rVB3	18230	33798	0.41%	0.044%
10	7.851	803	810	818	rVB	1384020	2191874	26.30%	2.856%
11	8.081	843	849	850	rBV3	6327	9943	0.12%	0.013%
12	8.175	863	865	870	rVB	6471	9532	0.11%	0.012%
13	8.251	870	878	882	rVB	10775	27996	0.34%	0.036%
14	8.557	920	930	939	rBV	686430	1113168	13.36%	1.450%
15	9.010	998	1007	1015	rBV	1165141	1894354	22.73%	2.468%
16	9.428	1076	1078	1083	rVB4	8905	12215	0.15%	0.016%
17	9.728	1122	1129	1142	rBV	907938	1498409	17.98%	1.952%
18	10.269	1214	1221	1230	rBV	1314533	2238367	26.86%	2.916%
19	10.545	1266	1268	1271	rBV2	6408	9549	0.11%	0.012%
20	10.587	1271	1275	1277	rVV	13174	19381	0.23%	0.025%
21	10.645	1277	1285	1296	rVV	1892318	3134400	37.62%	4.083%
22	10.787	1301	1309	1321	rVV	1394712	2339761	28.08%	3.048%
23	11.422	1414	1417	1419	rBV	6114	8700	0.10%	0.011%
24	12.234	1550	1555	1560	rBV2	30167	47100	0.57%	0.061%
25	13.110	1699	1704	1709	rBV2	12510	20856	0.25%	0.027%
26	13.386	1745	1751	1759	rBV	38040	67325	0.81%	0.088%
27	13.451	1759	1762	1768	rBV3	9883	15025	0.18%	0.020%
28	13.892	1831	1837	1849	rBV	3060099	4292841	51.52%	5.593%
29	14.175	1878	1885	1894	rBV	3460486	5156581	61.88%	6.718%
30	14.481	1930	1937	1945	rBV	2671477	3845194	46.15%	5.009%
31	14.681	1965	1971	1978	rBV2	172745	279899	3.36%	0.365%
32	14.898	2004	2008	2013	rVB8	12222	18606	0.22%	0.024%
33	15.475	2099	2106	2114	rBV	4294232	6323588	75.89%	8.238%
34	15.586	2119	2125	2134	rBV	1029798	1463479	17.56%	1.907%
35	15.710	2143	2146	2152	rVB3	22910	34402	0.41%	0.045%
36	17.227	2397	2404	2414	rBV	2726575	3912525	46.95%	5.097%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018652.D
Acq On : 06 Dec 2023 23:42
Operator : MA/JU
Sample : 05439-07
Misc :
ALS Vial : 89 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	17.327	2414	2421	2433	rVV	4360505	6336651	76.05%	8.255%
38	18.116	2551	2555	2563	rBV2	147355	203308	2.44%	0.265%
39	18.433	2607	2609	2617	rVB3	24288	33689	0.40%	0.044%
40	18.580	2631	2634	2638	rBV3	19822	23579	0.28%	0.031%
41	19.139	2725	2729	2734	rBV2	60730	81193	0.97%	0.106%
42	19.204	2736	2740	2747	rBV	74246	114700	1.38%	0.149%
43	19.351	2761	2765	2772	rBV3	102071	144164	1.73%	0.188%
44	19.563	2795	2801	2807	rBV	5586035	7396332	88.76%	9.636%
45	21.315	3094	3099	3105	rBV	3317180	4168219	50.02%	5.430%
46	23.533	3469	3476	3484	rBV2	4308951	8332596	100.00%	10.856%
47	23.686	3495	3502	3511	rVB	2424191	4865488	58.39%	6.339%




Sum of corrected areas: 76758508

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018652.D
Acq On : 06 Dec 2023 23:42
Operator : MA/JU
Sample : 05439-07
Misc :
ALS Vial : 89 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

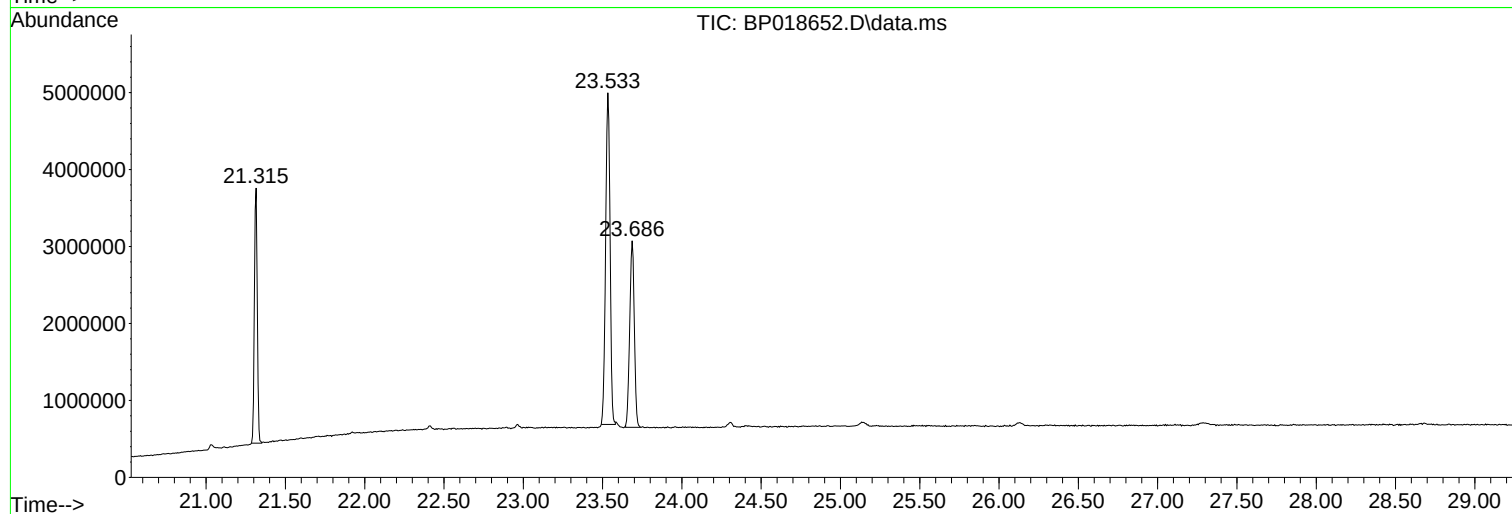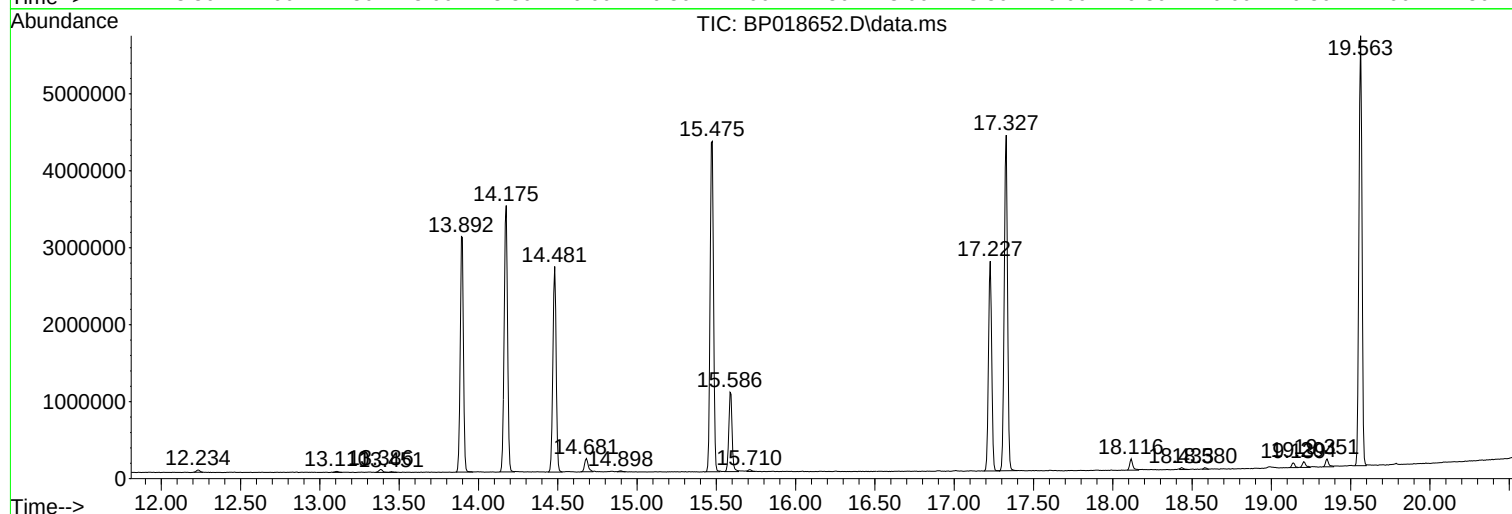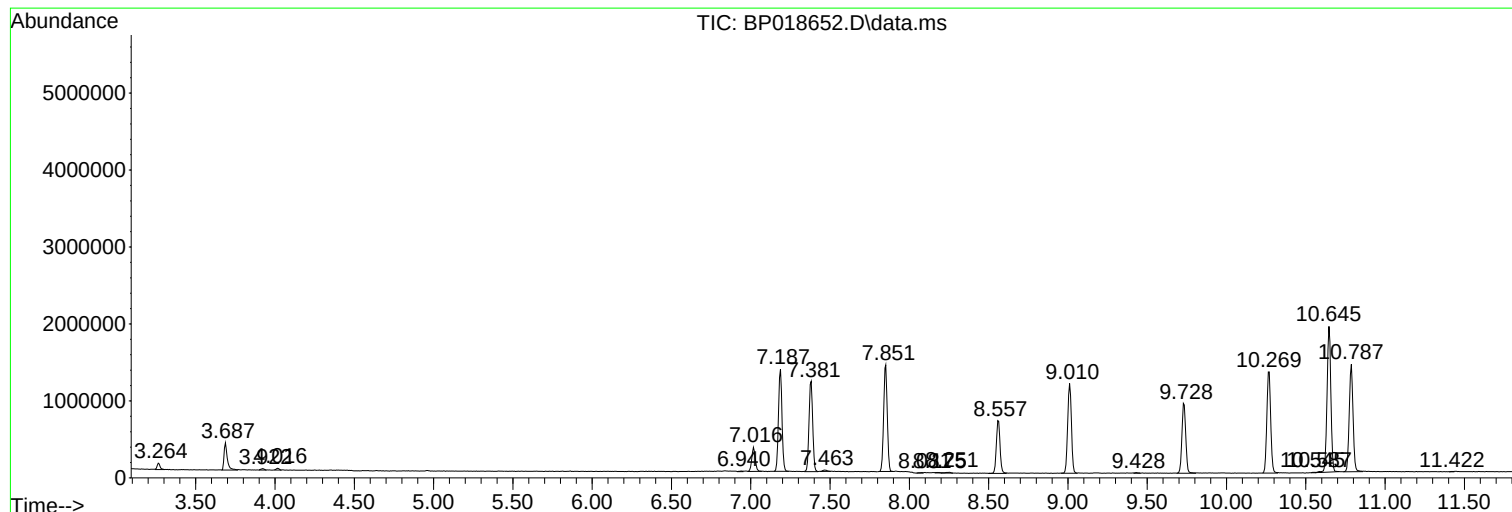

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018652.D
Acq On : 06 Dec 2023 23:42
Operator : MA/JU
Sample : 05439-07
Misc :
ALS Vial : 89 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018652.D
Acq On : 06 Dec 2023 23:42
Operator : MA/JU
Sample : 05439-07
Misc :
ALS Vial : 89 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
