

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018653.D
 Acq On : 07 Dec 2023 00:16
 Operator : MA/JU
 Sample : 05439-08
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018653.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	36	rVB	85852	107910	1.45%	0.129%
2	3.687	98	102	112	rBV	353403	508562	6.82%	0.607%
3	3.923	138	142	146	rVB2	21706	29082	0.39%	0.035%
4	4.017	154	158	162	rBV2	26893	36763	0.49%	0.044%
5	4.958	317	318	324	rVB4	8737	10205	0.14%	0.012%
6	7.016	662	668	678	rVB	376159	585850	7.86%	0.699%
7	7.187	690	697	709	rVB	1490440	2308478	30.98%	2.754%
8	7.381	723	730	738	rBV	1336452	2103050	28.22%	2.509%
9	7.464	740	744	752	rVB3	22076	42657	0.57%	0.051%
10	7.611	765	769	772	rBV	6861	12109	0.16%	0.014%
11	7.852	803	810	817	rVV	1596570	2533128	33.99%	3.022%
12	7.916	817	821	828	rVB3	8472	16522	0.22%	0.020%
13	8.558	922	930	941	rBV	1065462	1720190	23.08%	2.052%
14	9.010	999	1007	1015	rBV	1741163	2769891	37.17%	3.305%
15	9.434	1075	1079	1084	rVB3	15182	25472	0.34%	0.030%
16	9.546	1095	1098	1100	rBV	8953	13391	0.18%	0.016%
17	9.728	1122	1129	1136	rBV	1276569	2117069	28.41%	2.526%
18	10.263	1213	1220	1230	rBV	1937932	3248486	43.59%	3.876%
19	10.646	1278	1285	1293	rVB	2272140	3711051	49.80%	4.428%
20	10.787	1301	1309	1320	rBV	1475404	2477689	33.25%	2.956%
21	11.916	1493	1501	1510	rVB4	14018	35736	0.48%	0.043%
22	12.034	1520	1521	1525	rVB	12203	8344	0.11%	0.010%
23	12.099	1529	1532	1533	rBV	7860	8943	0.12%	0.011%
24	12.234	1549	1555	1562	rVB3	39782	68234	0.92%	0.081%
25	13.104	1699	1703	1709	rVB2	20157	35665	0.48%	0.043%
26	13.310	1735	1738	1741	rVB5	9049	10905	0.15%	0.013%
27	13.387	1744	1751	1757	rBV2	52129	87989	1.18%	0.105%
28	13.451	1759	1762	1766	rVB5	6821	10983	0.15%	0.013%
29	13.898	1830	1838	1847	rBV	3812991	5214409	69.97%	6.221%
30	14.175	1876	1885	1896	rBV	4051604	6218163	83.44%	7.419%
31	14.481	1929	1937	1945	rBV	3315668	4805728	64.49%	5.734%
32	14.681	1964	1971	1984	rBV	212843	366390	4.92%	0.437%
33	14.840	1991	1998	2002	rBV6	11099	22647	0.30%	0.027%
34	14.893	2003	2007	2014	rVB8	13087	25808	0.35%	0.031%
35	15.469	2099	2105	2113	rBV	5059243	7451851	100.00%	8.891%
36	15.592	2119	2126	2142	rBV	1195370	1709420	22.94%	2.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018653.D
 Acq On : 07 Dec 2023 00:16
 Operator : MA/JU
 Sample : 05439-08
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.710	2142	2146	2152	rVB3	28430	45343	0.61%	0.054%
38	16.257	2234	2239	2244	rVB3	9735	17938	0.24%	0.021%
39	16.628	2299	2302	2306	rBV4	5735	10711	0.14%	0.013%
40	16.687	2310	2312	2319	rBV3	4264	9673	0.13%	0.012%
41	16.904	2346	2349	2353	rVB6	7285	10691	0.14%	0.013%
42	17.104	2381	2383	2387	rVB3	7545	8858	0.12%	0.011%
43	17.228	2397	2404	2411	rBV	3432886	4751427	63.76%	5.669%
44	17.328	2414	2421	2431	rVV	4995066	7122508	95.58%	8.498%
45	17.734	2488	2490	2492	rVB	17507	13047	0.18%	0.016%
46	17.910	2515	2520	2524	rBV2	11542	19671	0.26%	0.023%
47	18.116	2552	2555	2562	rVB2	56368	68774	0.92%	0.082%
48	18.434	2604	2609	2614	rBV4	22495	41028	0.55%	0.049%
49	18.581	2630	2634	2639	rVB4	21573	30719	0.41%	0.037%
50	18.986	2700	2703	2710	rBV9	14303	25274	0.34%	0.030%
51	19.139	2724	2729	2734	rBV2	53913	72651	0.97%	0.087%
52	19.204	2736	2740	2746	rBV	62113	90949	1.22%	0.109%
53	19.351	2762	2765	2768	rBV2	23523	23737	0.32%	0.028%
54	19.563	2795	2801	2808	rBV	4628798	6162205	82.69%	7.352%
55	21.316	3094	3099	3104	rBV	2933857	3668929	49.24%	4.377%
56	23.533	3468	3476	3484	rBV2	3523600	6939851	93.13%	8.280%
57	23.686	3495	3502	3511	rVB	2232482	4220918	56.64%	5.036%




Sum of corrected areas: 83813672

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018653.D
Acq On : 07 Dec 2023 00:16
Operator : MA/JU
Sample : 05439-08
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

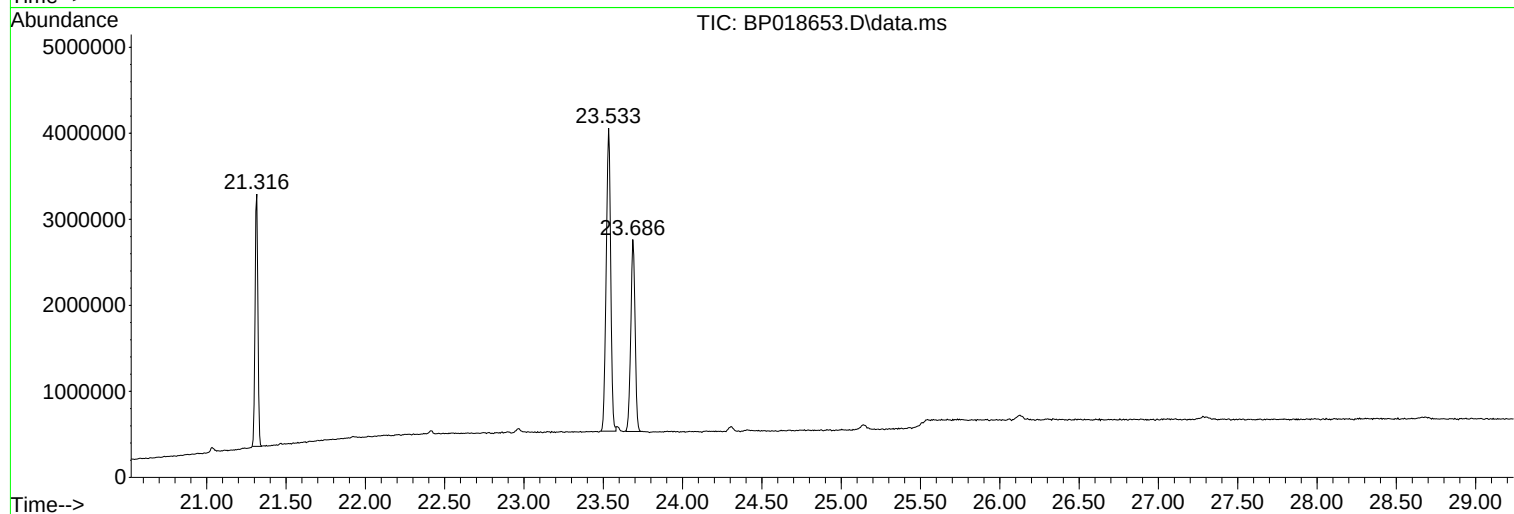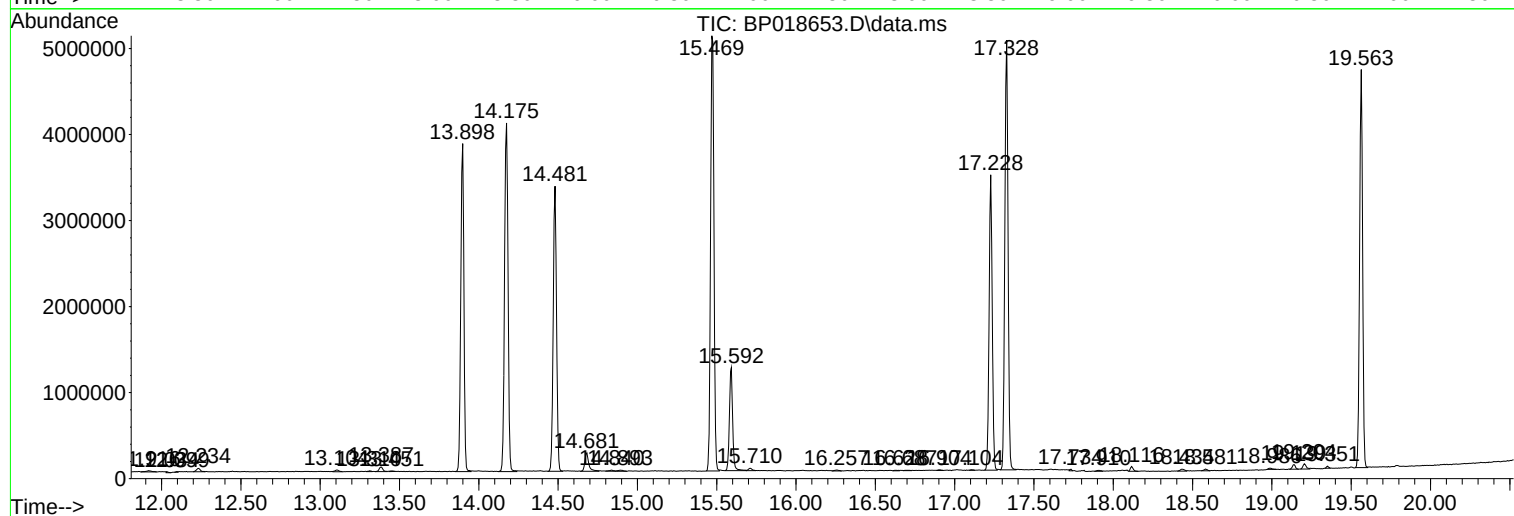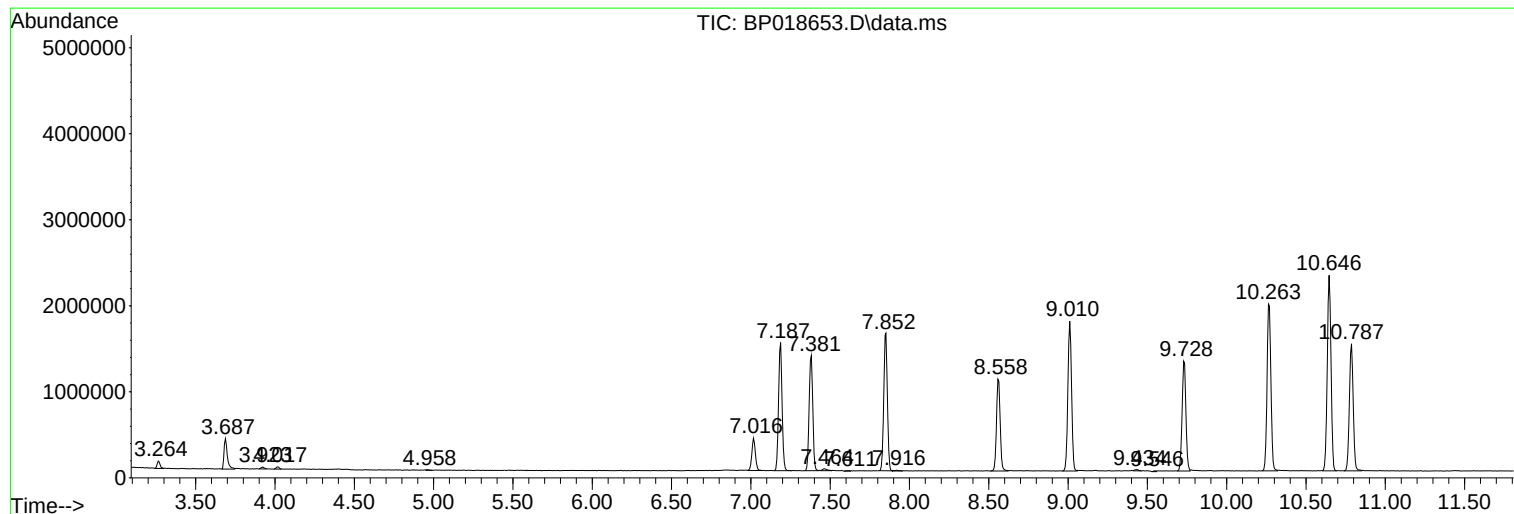

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018653.D
Acq On : 07 Dec 2023 00:16
Operator : MA/JU
Sample : 05439-08
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018653.D
Acq On : 07 Dec 2023 00:16
Operator : MA/JU
Sample : 05439-08
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc