

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018654.D
 Acq On : 07 Dec 2023 00:50
 Operator : MA/JU
 Sample : 05439-11
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018654.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	27	30	37	rVB	72730	92784	1.00%	0.122%
2	3.687	98	102	117	rBV	420644	601145	6.45%	0.788%
3	3.928	137	143	150	rVB2	18074	36438	0.39%	0.048%
4	4.016	155	158	163	rVB2	24245	30703	0.33%	0.040%
5	7.016	661	668	675	rVB	269634	422589	4.53%	0.554%
6	7.187	690	697	705	rBV	1219207	1878183	20.15%	2.462%
7	7.381	722	730	739	rBV	1046278	1663281	17.85%	2.180%
8	7.469	742	745	750	rVB4	13589	22617	0.24%	0.030%
9	7.851	800	810	817	rBV	1328384	2116743	22.71%	2.775%
10	7.916	817	821	829	rVB3	7153	16752	0.18%	0.022%
11	8.557	923	930	940	rBV	782360	1252616	13.44%	1.642%
12	9.010	1000	1007	1015	rBV	1353243	2170823	23.30%	2.845%
13	9.428	1073	1078	1083	rVB3	19434	36565	0.39%	0.048%
14	9.734	1122	1130	1143	rBV	940714	1555725	16.69%	2.039%
15	10.269	1211	1221	1229	rBV	1431092	2411529	25.88%	3.161%
16	10.645	1278	1285	1293	rVB	1729994	2840680	30.48%	3.723%
17	10.786	1300	1309	1322	rVB	1253477	2118985	22.74%	2.777%
18	11.928	1498	1503	1506	rBV3	9568	14718	0.16%	0.019%
19	12.233	1549	1555	1561	rVB3	27039	47056	0.50%	0.062%
20	13.098	1700	1702	1704	rBV2	9593	9550	0.10%	0.013%
21	13.310	1735	1738	1743	rVB5	7975	10703	0.11%	0.014%
22	13.380	1746	1750	1757	rVB3	29703	49004	0.53%	0.064%
23	13.892	1831	1837	1845	rBV	2615928	3665369	39.33%	4.804%
24	14.174	1875	1885	1894	rBV	3188539	4540326	48.72%	5.951%
25	14.480	1930	1937	1944	rBV	2378558	3419991	36.70%	4.483%
26	14.680	1965	1971	1982	rBV2	161581	279849	3.00%	0.367%
27	14.833	1995	1997	2002	rVV4	6544	10539	0.11%	0.014%
28	14.892	2004	2007	2013	rVB6	11074	21124	0.23%	0.028%
29	15.469	2099	2105	2112	rBV	3957235	5715458	61.33%	7.492%
30	15.521	2112	2114	2119	rVB3	13400	19795	0.21%	0.026%
31	15.586	2119	2125	2138	rBV	968273	1343299	14.41%	1.761%
32	15.710	2142	2146	2150	rBV3	17574	26716	0.29%	0.035%
33	16.527	2280	2285	2288	rVB3	15710	22113	0.24%	0.029%
34	17.010	2365	2367	2373	rVB	7711	10256	0.11%	0.013%
35	17.227	2398	2404	2410	rBV	2751870	3801114	40.79%	4.982%
36	17.327	2415	2421	2433	rVV	4472569	6248511	67.05%	8.190%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018654.D
 Acq On : 07 Dec 2023 00:50
 Operator : MA/JU
 Sample : 05439-11
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.633	2470	2473	2477	rVB2	13170	16045	0.17%	0.021%
38	17.845	2506	2509	2512	rBV2	7213	12363	0.13%	0.016%
39	17.904	2516	2519	2525	rVB6	9365	13890	0.15%	0.018%
40	18.115	2550	2555	2561	rBV4	77294	113298	1.22%	0.149%
41	18.192	2564	2568	2572	rVV2	18968	28698	0.31%	0.038%
42	18.439	2606	2610	2614	rVB3	24117	36088	0.39%	0.047%
43	18.586	2631	2635	2638	rBV5	16789	22298	0.24%	0.029%
44	18.986	2699	2703	2706	rBV6	23767	42220	0.45%	0.055%
45	19.139	2725	2729	2734	rBV2	64024	86243	0.93%	0.113%
46	19.204	2736	2740	2743	rBV	71044	98750	1.06%	0.129%
47	19.233	2743	2745	2751	rVB2	36767	49803	0.53%	0.065%
48	19.351	2762	2765	2771	rBV3	37794	44061	0.47%	0.058%
49	19.562	2795	2801	2810	rBV	5966755	7933412	85.13%	10.399%
50	21.315	3093	3099	3104	rBV	3722561	4686243	50.29%	6.142%
51	23.533	3469	3476	3483	rBV2	4718263	9318765	100.00%	12.215%
52	23.686	3495	3502	3510	rVB	2710866	5266568	56.52%	6.903%




Sum of corrected areas: 76292394

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018654.D
Acq On : 07 Dec 2023 00:50
Operator : MA/JU
Sample : 05439-11
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

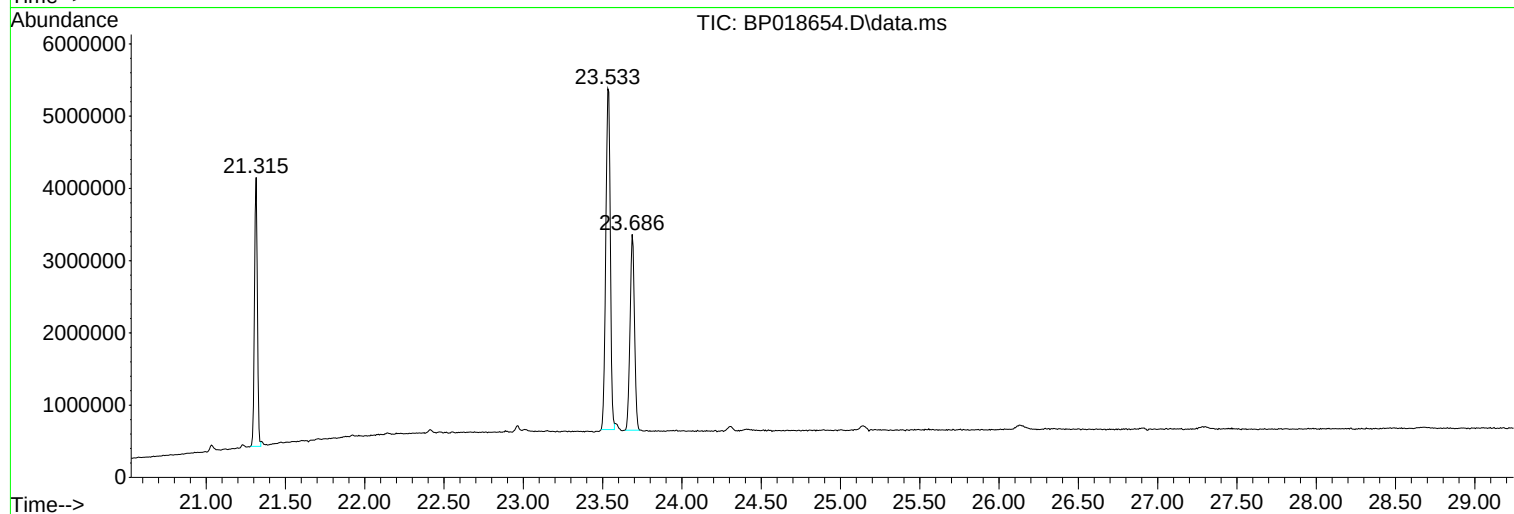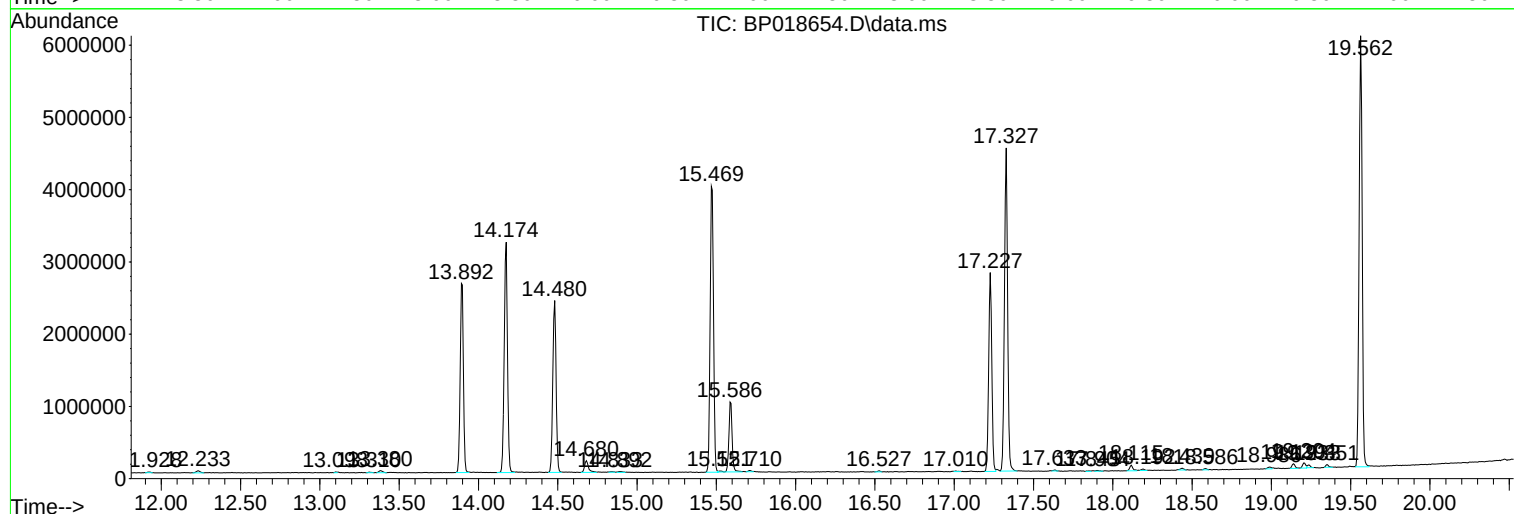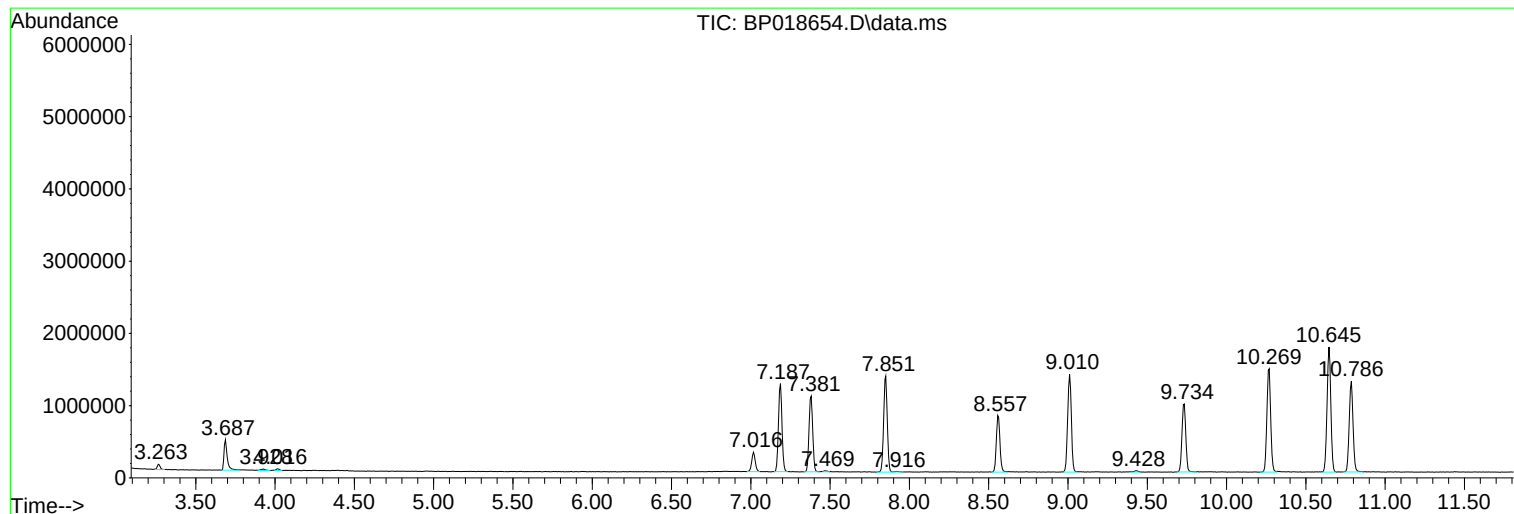

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018654.D
Acq On : 07 Dec 2023 00:50
Operator : MA/JU
Sample : 05439-11
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018654.D
Acq On : 07 Dec 2023 00:50
Operator : MA/JU
Sample : 05439-11
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc