

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018655.D
 Acq On : 07 Dec 2023 01:24
 Operator : MA/JU
 Sample : 05439-12
 Misc :
 ALS Vial : 92 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018655.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	37	rVB	73129	95073	0.87%	0.116%
2	3.687	98	102	113	rBV	426894	603138	5.50%	0.738%
3	3.922	138	142	146	rVB2	20801	33020	0.30%	0.040%
4	4.017	154	158	164	rBV2	22790	37116	0.34%	0.045%
5	5.211	359	361	363	rBV	11188	11022	0.10%	0.013%
6	5.799	457	461	463	rBV	11646	19321	0.18%	0.024%
7	6.899	646	648	652	rVB	10772	14198	0.13%	0.017%
8	7.016	662	668	677	rBV	263333	413792	3.77%	0.506%
9	7.105	681	683	686	rVB	12137	12965	0.12%	0.016%
10	7.187	689	697	705	rBV	933262	1445579	13.17%	1.768%
11	7.381	721	730	740	rBV	1008036	1667538	15.19%	2.040%
12	7.469	740	745	755	rVB3	22478	58913	0.54%	0.072%
13	7.846	803	809	818	rVV	1233971	1962610	17.88%	2.401%
14	7.916	818	821	826	rVB2	5834	11128	0.10%	0.014%
15	8.557	924	930	939	rBV	840925	1330014	12.12%	1.627%
16	9.010	1000	1007	1014	rBV	1315327	2119012	19.31%	2.592%
17	9.428	1074	1078	1084	rVB4	19614	32029	0.29%	0.039%
18	9.728	1122	1129	1138	rBV	981411	1588677	14.47%	1.943%
19	10.263	1213	1220	1233	rBV	1504778	2508420	22.85%	3.068%
20	10.646	1277	1285	1294	rVB	1559339	2585449	23.56%	3.162%
21	10.787	1302	1309	1322	rBV	1264067	2169664	19.77%	2.654%
22	11.922	1498	1502	1506	rBV3	11882	14066	0.13%	0.017%
23	12.234	1550	1555	1560	rVB2	31178	51748	0.47%	0.063%
24	13.381	1746	1750	1754	rBV2	21864	32025	0.29%	0.039%
25	13.892	1831	1837	1849	rBV	2757899	3912613	35.65%	4.786%
26	14.169	1878	1884	1893	rBV	3068629	4678929	42.63%	5.723%
27	14.481	1930	1937	1946	rBV	2165351	3262331	29.72%	3.990%
28	14.681	1965	1971	1981	rBV	239626	405315	3.69%	0.496%
29	14.898	2006	2008	2013	rVB5	11946	13986	0.13%	0.017%
30	15.281	2069	2073	2079	rVB2	27441	36070	0.33%	0.044%
31	15.469	2097	2105	2112	rBV	3593488	5192186	47.31%	6.351%
32	15.587	2118	2125	2137	rBV	1132980	1539358	14.03%	1.883%
33	15.710	2142	2146	2149	rBV2	20618	24552	0.22%	0.030%
34	16.057	2199	2205	2208	rBV	18322	41655	0.38%	0.051%
35	17.104	2379	2383	2388	rBV6	8996	14111	0.13%	0.017%
36	17.228	2397	2404	2410	rBV	2883742	4072573	37.11%	4.981%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018655.D
 Acq On : 07 Dec 2023 01:24
 Operator : MA/JU
 Sample : 05439-12
 Misc :
 ALS Vial : 92 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AD4

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.328	2414	2421	2433	rVV	5070136	7338507	66.86%	8.976%
38	18.116	2551	2555	2561	rBV3	106485	138865	1.27%	0.170%
39	18.433	2606	2609	2615	rVB5	29356	42928	0.39%	0.053%
40	18.580	2631	2634	2638	rBV2	23794	28827	0.26%	0.035%
41	18.992	2700	2704	2711	rBV10	21219	43700	0.40%	0.053%
42	19.139	2725	2729	2735	rVB2	77849	100547	0.92%	0.123%
43	19.204	2736	2740	2745	rBV	88707	126406	1.15%	0.155%
44	19.351	2762	2765	2769	rBV5	36936	38361	0.35%	0.047%
45	19.563	2795	2801	2808	rBV	7622189	9716633	88.53%	11.885%
46	21.033	3048	3051	3058	rBV4	104919	178938	1.63%	0.219%
47	21.227	3082	3084	3088	rVB	107460	104766	0.95%	0.128%
48	21.316	3094	3099	3104	rBV	4160484	5139493	46.83%	6.286%
49	23.533	3469	3476	3484	rBV2	5705801	10975642	100.00%	13.425%
50	23.686	3495	3502	3515	rVB	2955539	5771724	52.59%	7.060%




Sum of corrected areas: 81755533

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018655.D
Acq On : 07 Dec 2023 01:24
Operator : MA/JU
Sample : 05439-12
Misc :
ALS Vial : 92 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

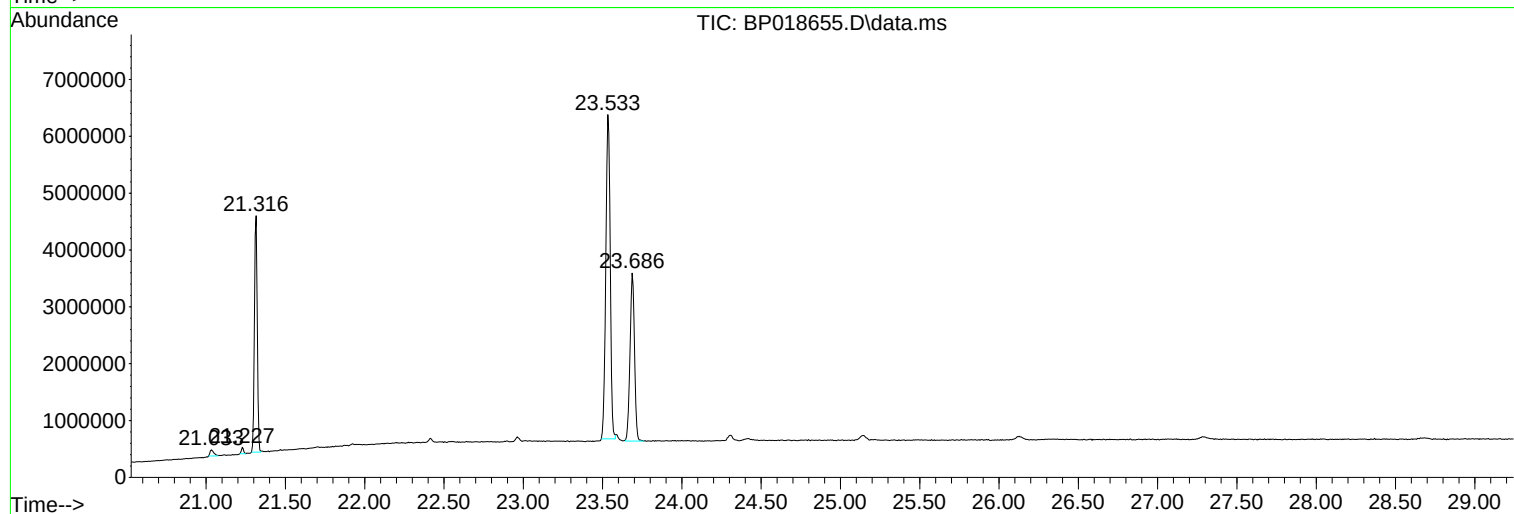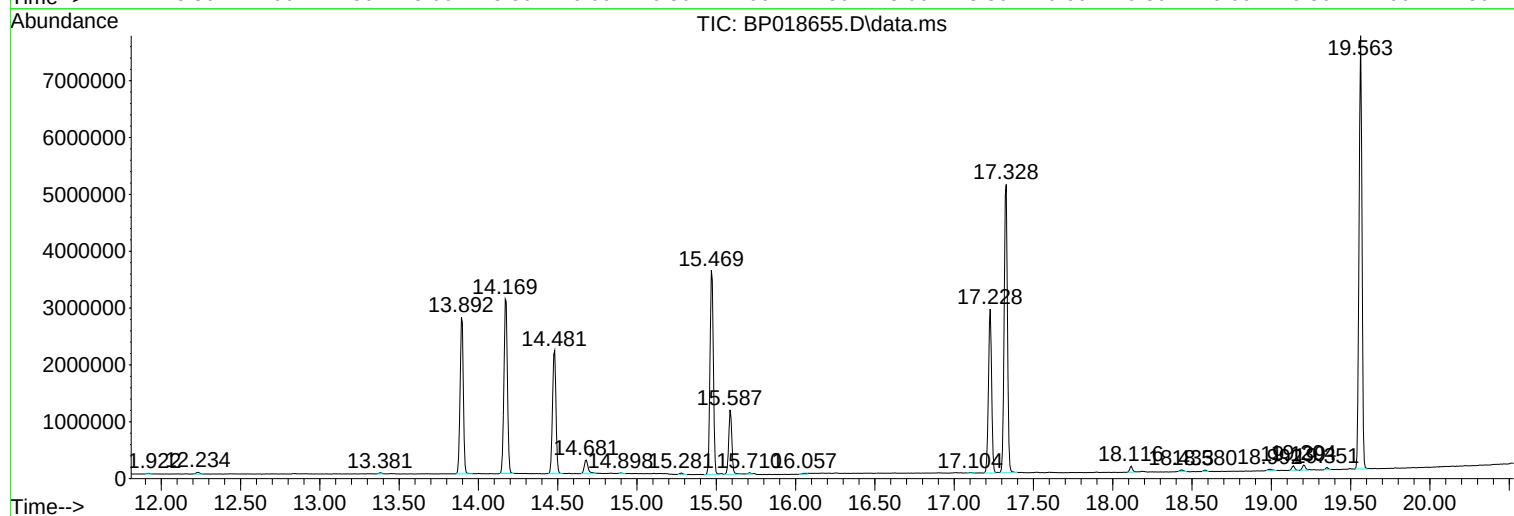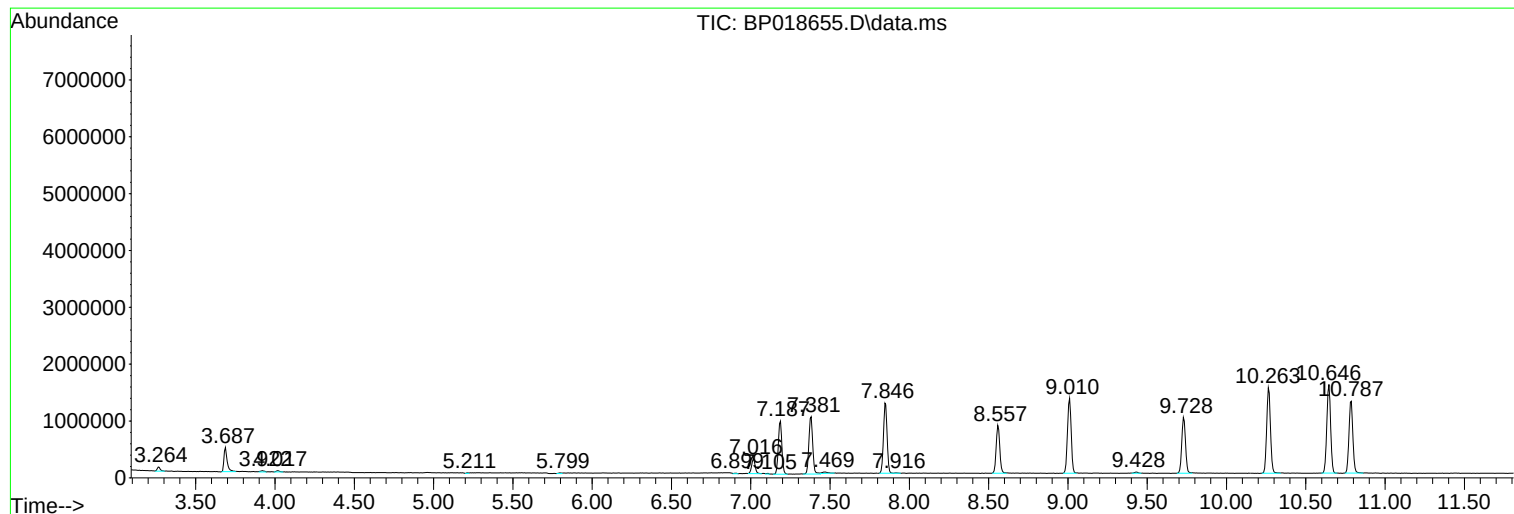

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018655.D
Acq On : 07 Dec 2023 01:24
Operator : MA/JU
Sample : 05439-12
Misc :
ALS Vial : 92 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018655.D
Acq On : 07 Dec 2023 01:24
Operator : MA/JU
Sample : 05439-12
Misc :
ALS Vial : 92 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------