

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018656.D
 Acq On : 07 Dec 2023 01:58
 Operator : MA/JU
 Sample : 05439-13
 Misc :
 ALS Vial : 93 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018656.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	36	rVB	77393	90288	0.97%	0.096%
2	3.687	98	102	114	rBV	335306	496047	5.32%	0.526%
3	3.923	139	142	146	rVB2	19593	26191	0.28%	0.028%
4	4.017	155	158	163	rVB	26847	32065	0.34%	0.034%
5	7.016	662	668	676	rVB	342590	518606	5.56%	0.549%
6	7.187	690	697	707	rVB	1493892	2278540	24.44%	2.414%
7	7.381	722	730	739	rBV	1269621	2036963	21.85%	2.158%
8	7.469	742	745	749	rVB4	12935	16522	0.18%	0.018%
9	7.764	793	795	798	rBV	6796	10539	0.11%	0.011%
10	7.846	803	809	818	rVB	1482124	2277914	24.44%	2.414%
11	7.916	818	821	827	rVB5	7387	11328	0.12%	0.012%
12	8.558	922	930	940	rBV	771886	1247324	13.38%	1.322%
13	9.011	999	1007	1015	rBV	1303831	2113804	22.68%	2.240%
14	9.428	1074	1078	1083	rVB	27090	41659	0.45%	0.044%
15	9.728	1121	1129	1142	rBV	1035725	1678753	18.01%	1.779%
16	10.263	1212	1220	1229	rBV	1535807	2598011	27.87%	2.753%
17	10.593	1271	1276	1277	rBV3	6121	9804	0.11%	0.010%
18	10.646	1277	1285	1294	rVB	1776157	2972544	31.89%	3.150%
19	10.787	1301	1309	1317	rBV	1214304	2028048	21.76%	2.149%
20	11.922	1496	1502	1508	rBV4	21592	37076	0.40%	0.039%
21	12.234	1549	1555	1564	rVB3	32871	57966	0.62%	0.061%
22	12.804	1646	1652	1655	rVV2	24770	51426	0.55%	0.054%
23	12.846	1656	1659	1660	rVV2	22652	28095	0.30%	0.030%
24	12.869	1660	1663	1671	rVB2	36960	69751	0.75%	0.074%
25	13.310	1734	1738	1744	rVB5	15521	24882	0.27%	0.026%
26	13.381	1746	1750	1759	rBV3	51591	100894	1.08%	0.107%
27	13.481	1764	1767	1772	rVV2	25372	40618	0.44%	0.043%
28	13.540	1773	1777	1783	rVB2	25183	43593	0.47%	0.046%
29	13.898	1831	1838	1847	rBV	4240573	6001722	64.38%	6.359%
30	14.169	1877	1884	1897	rBV	4444592	6775012	72.68%	7.178%
31	14.481	1929	1937	1944	rVV	3508504	5376842	57.68%	5.697%
32	14.675	1965	1970	1982	rBV2	237488	400590	4.30%	0.424%
33	14.893	2005	2007	2013	rVB6	14862	20684	0.22%	0.022%
34	15.281	2068	2073	2079	rVV	72141	94973	1.02%	0.101%
35	15.328	2079	2081	2088	rVB4	8302	11055	0.12%	0.012%
36	15.469	2099	2105	2116	rVB	6094698	8818514	94.60%	9.344%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018656.D
 Acq On : 07 Dec 2023 01:58
 Operator : MA/JU
 Sample : 05439-13
 Misc :
 ALS Vial : 93 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AD5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.587	2119	2125	2138	rBV	1511593	2142384	22.98%	2.270%
38	15.710	2142	2146	2152	rVB3	29332	46234	0.50%	0.049%
39	17.228	2397	2404	2411	rBV	3907866	5592347	59.99%	5.925%
40	17.328	2414	2421	2432	rVV	6019030	8848334	94.92%	9.375%
41	18.116	2550	2555	2560	rBV2	123062	162290	1.74%	0.172%
42	18.434	2606	2609	2613	rVB4	23239	31209	0.33%	0.033%
43	18.581	2631	2634	2640	rVB4	21421	29093	0.31%	0.031%
44	19.139	2725	2729	2735	rVB	87138	105252	1.13%	0.112%
45	19.204	2736	2740	2749	rBV	87283	134590	1.44%	0.143%
46	19.351	2762	2765	2769	rBV2	55219	61526	0.66%	0.065%
47	19.563	2795	2801	2807	rBV	7047133	9321845	100.00%	9.877%
48	21.033	3048	3051	3059	rBV3	107232	182306	1.96%	0.193%
49	21.316	3094	3099	3104	rBV	4007872	4857651	52.11%	5.147%
50	23.533	3468	3476	3483	rBV2	4659463	9192030	98.61%	9.739%
51	23.686	3495	3502	3512	rVB	2603304	5233571	56.14%	5.545%




Sum of corrected areas: 94379305

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018656.D
Acq On : 07 Dec 2023 01:58
Operator : MA/JU
Sample : 05439-13
Misc :
ALS Vial : 93 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

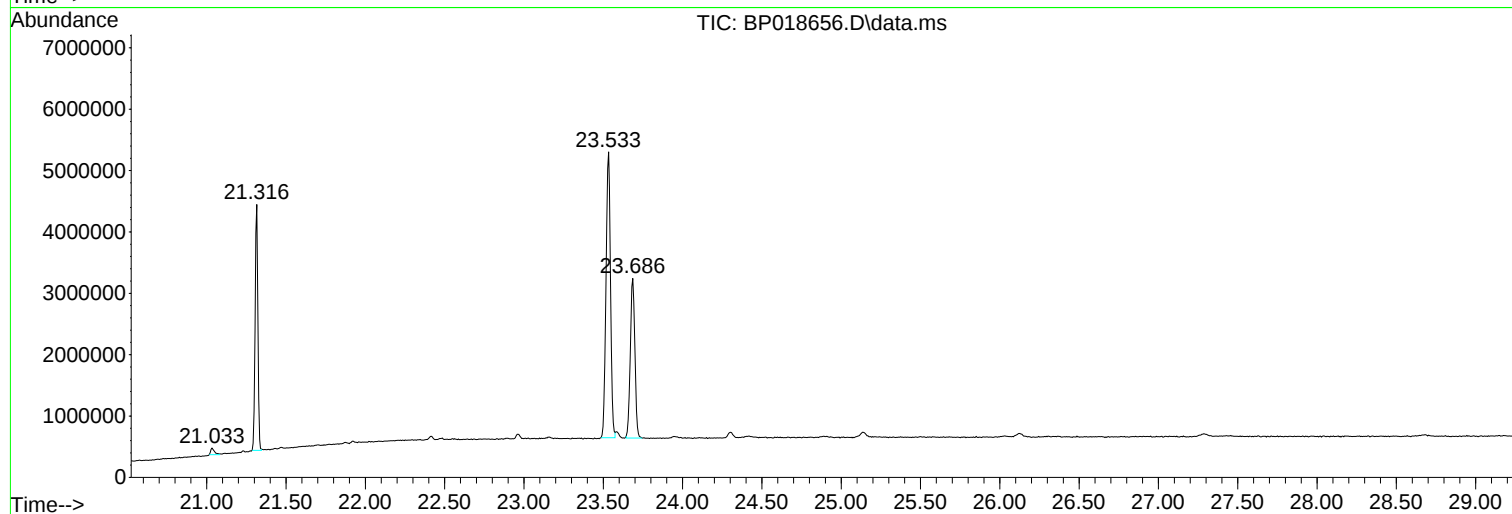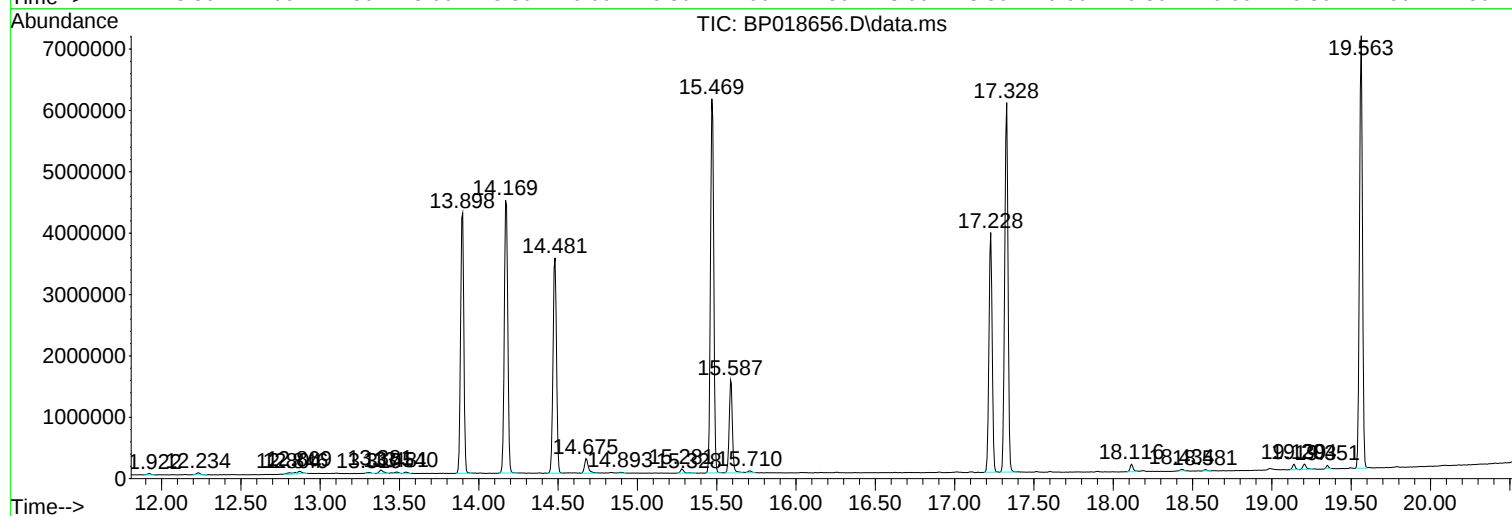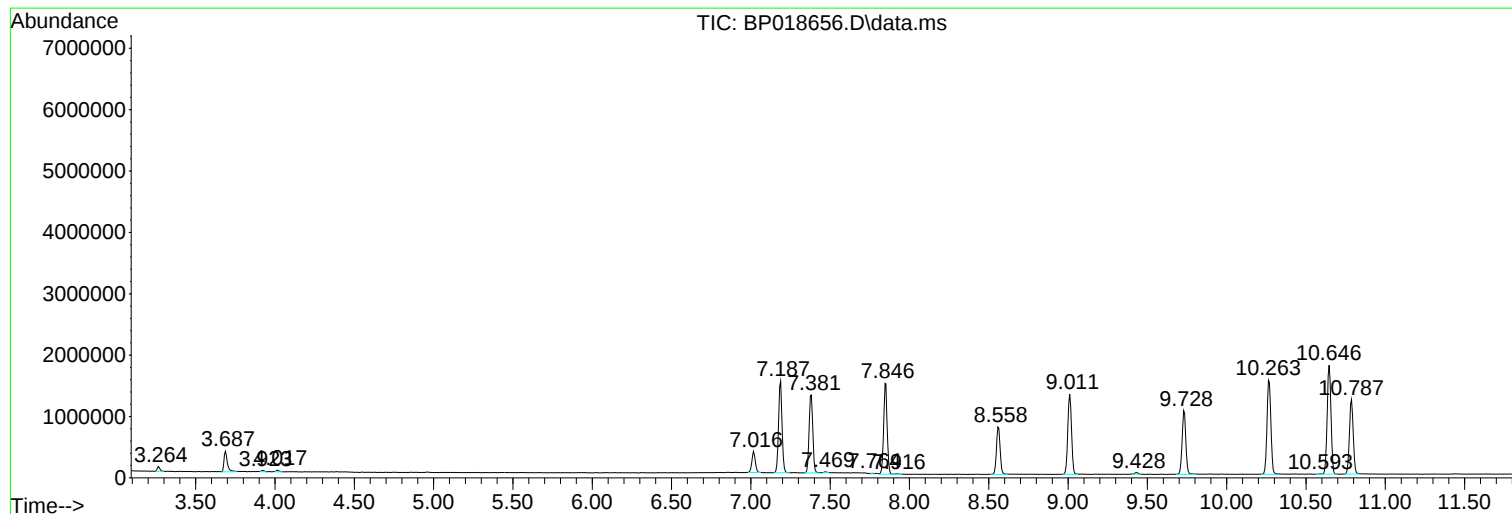

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018656.D
Acq On : 07 Dec 2023 01:58
Operator : MA/JU
Sample : 05439-13
Misc :
ALS Vial : 93 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018656.D
Acq On : 07 Dec 2023 01:58
Operator : MA/JU
Sample : 05439-13
Misc :
ALS Vial : 93 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AD5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc