

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018658.D
 Acq On : 07 Dec 2023 03:40
 Operator : MA/JU
 Sample : PB157356BL
 Misc :
 ALS Vial : 96 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK356

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018658.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	42	rVB	145744	190771	2.19%	0.210%
2	3.681	97	101	116	rBV	1543720	2127559	24.42%	2.347%
3	4.017	154	158	163	rBV	25716	34026	0.39%	0.038%
4	6.758	621	624	625	rBV	9801	9723	0.11%	0.011%
5	7.016	661	668	681	rVB	1776349	2791854	32.04%	3.080%
6	7.187	690	697	705	rVB	1539023	2327187	26.71%	2.568%
7	7.381	722	730	740	rBV	1807556	2825171	32.43%	3.117%
8	7.852	803	810	817	rVB	1458654	2311446	26.53%	2.550%
9	8.493	918	919	924	rVB	10273	9719	0.11%	0.011%
10	8.563	924	931	941	rBV	1759848	2824227	32.42%	3.116%
11	9.011	997	1007	1015	rBV	1454762	2322090	26.65%	2.562%
12	9.128	1023	1027	1030	rBV6	11272	21960	0.25%	0.024%
13	9.734	1122	1130	1137	rBV	1289727	2125869	24.40%	2.346%
14	10.263	1213	1220	1233	rBV	2036867	3442634	39.51%	3.798%
15	10.646	1277	1285	1296	rVB	1975106	3251534	37.32%	3.588%
16	10.787	1301	1309	1323	rBV	1594905	2673323	30.68%	2.950%
17	12.228	1550	1554	1561	rVB2	38122	65992	0.76%	0.073%
18	13.381	1744	1750	1756	rBV4	14149	33443	0.38%	0.037%
19	13.446	1758	1761	1767	rVV6	6606	12297	0.14%	0.014%
20	13.893	1831	1837	1845	rBV	3251797	4565412	52.40%	5.037%
21	14.169	1878	1884	1894	rBV	3691501	5710900	65.55%	6.301%
22	14.481	1930	1937	1946	rBV	2745105	3995043	45.85%	4.408%
23	14.681	1964	1971	1986	rBV	1267669	1940619	22.27%	2.141%
24	15.469	2098	2105	2115	rBV	4578314	6749856	77.47%	7.447%
25	15.587	2118	2125	2138	rVV	1096415	1532475	17.59%	1.691%
26	15.710	2140	2146	2153	rVB2	24819	49467	0.57%	0.055%
27	17.228	2397	2404	2412	rBV	2859666	4118688	47.27%	4.544%
28	17.328	2414	2421	2434	rVV	4391697	6505384	74.67%	7.178%
29	18.110	2552	2554	2560	rVB7	9758	12592	0.14%	0.014%
30	18.434	2607	2609	2613	rBV5	11782	14990	0.17%	0.017%
31	19.139	2725	2729	2734	rBV	60373	78240	0.90%	0.086%
32	19.204	2736	2740	2745	rBV	58622	84836	0.97%	0.094%
33	19.563	2795	2801	2807	rBV	5735781	7448323	85.49%	8.218%
34	21.310	3094	3098	3104	rBV	3525112	4479391	51.41%	4.942%
35	23.533	3468	3476	3483	rBV2	4415636	8712531	100.00%	9.613%
36	23.686	3495	3502	3512	rVB	2697751	5234861	60.08%	5.776%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018658.D
Acq On : 07 Dec 2023 03:40
Operator : MA/JU
Sample : PB157356BL
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK356

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 90634433

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018658.D
Acq On : 07 Dec 2023 03:40
Operator : MA/JU
Sample : PB157356BL
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK356

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

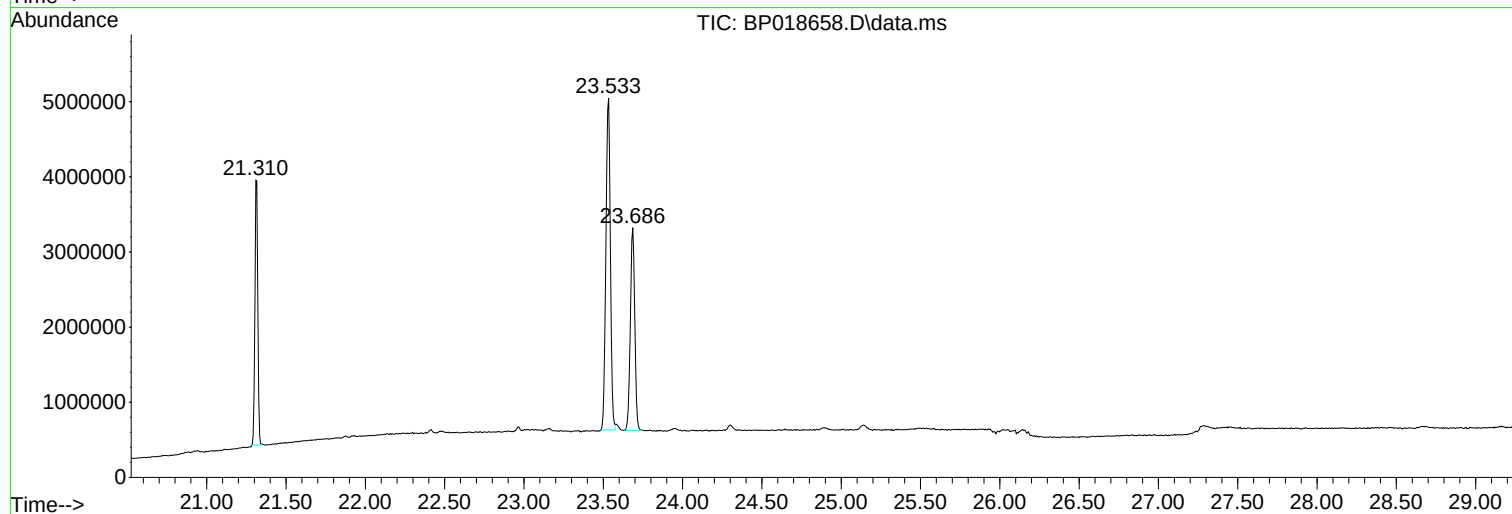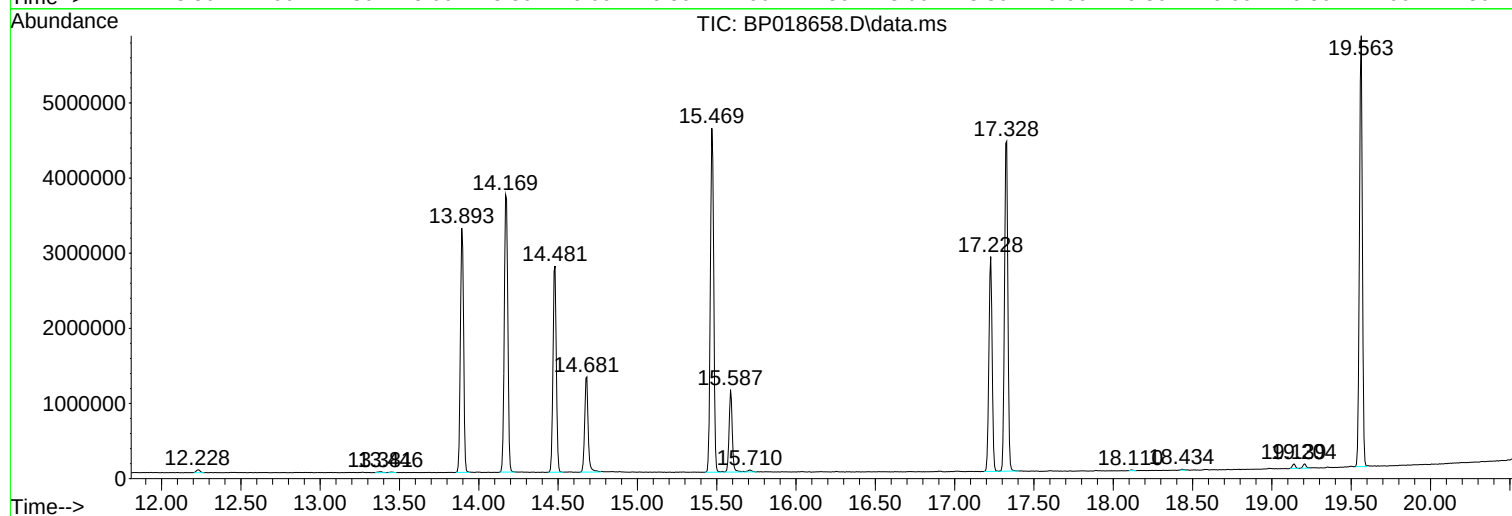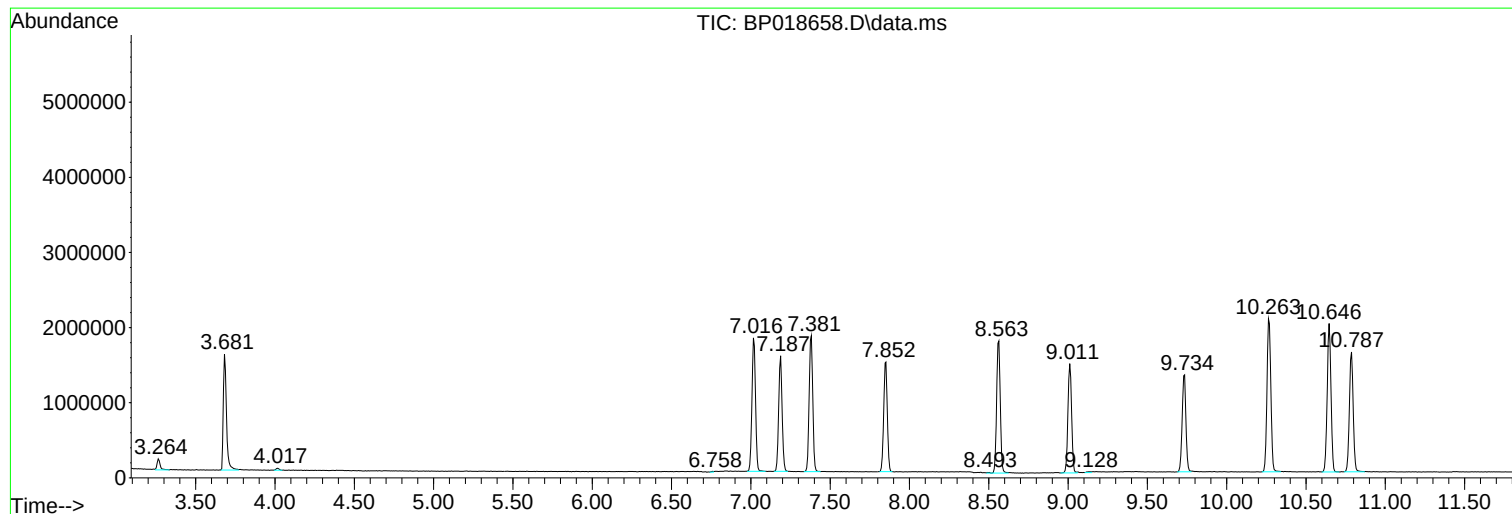

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018658.D
Acq On : 07 Dec 2023 03:40
Operator : MA/JU
Sample : PB157356BL
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK356

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018658.D
Acq On : 07 Dec 2023 03:40
Operator : MA/JU
Sample : PB157356BL
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK356

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------