

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018661.D
 Acq On : 07 Dec 2023 05:21
 Operator : MA/JU
 Sample : 05473-01
 Misc :
 ALS Vial : 104 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018661.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	36	rVB	79300	96670	0.90%	0.117%
2	3.687	98	102	117	rVB	417761	602004	5.63%	0.729%
3	3.923	140	142	147	rVB2	22873	27062	0.25%	0.033%
4	4.017	154	158	163	rBV2	24888	31947	0.30%	0.039%
5	7.017	662	668	679	rVB	327251	506217	4.73%	0.613%
6	7.181	689	696	705	rBV	1304202	2067208	19.33%	2.504%
7	7.375	722	729	739	rBV	1204774	1895637	17.73%	2.296%
8	7.846	801	809	818	rBV	1211322	1916253	17.92%	2.321%
9	8.558	923	930	942	rBV	914033	1430063	13.37%	1.732%
10	9.011	999	1007	1014	rBV	1478146	2373789	22.20%	2.875%
11	9.728	1121	1129	1138	rBV	1078172	1746871	16.34%	2.116%
12	10.263	1211	1220	1235	rBV	1675263	2761046	25.82%	3.344%
13	10.646	1277	1285	1296	rVB	1535531	2579150	24.12%	3.124%
14	10.781	1300	1308	1321	rBV	1270836	2184902	20.43%	2.646%
15	11.140	1363	1369	1370	rBV	11269	13532	0.13%	0.016%
16	12.234	1548	1555	1563	rBV3	32335	57618	0.54%	0.070%
17	13.381	1743	1750	1754	rBV2	21716	37358	0.35%	0.045%
18	13.446	1759	1761	1767	rVB4	9543	13089	0.12%	0.016%
19	13.893	1831	1837	1847	rBV	2983719	4101463	38.35%	4.968%
20	14.169	1875	1884	1892	rBV2	3419191	5078721	47.49%	6.151%
21	14.475	1930	1936	1944	rBV	2192245	3228631	30.19%	3.910%
22	14.675	1964	1970	1981	rBV2	190262	333563	3.12%	0.404%
23	14.893	2003	2007	2012	rVB6	11284	19380	0.18%	0.023%
24	15.469	2098	2105	2114	rBV	4653236	6461545	60.42%	7.826%
25	15.587	2119	2125	2137	rVV	1129210	1520939	14.22%	1.842%
26	15.704	2142	2145	2151	rVB3	23899	40066	0.37%	0.049%
27	16.898	2345	2348	2354	rBV4	8932	13606	0.13%	0.016%
28	17.228	2397	2404	2410	rBV	2625895	3888980	36.37%	4.710%
29	17.322	2414	2420	2429	rVV2	5071505	7161243	66.97%	8.674%
30	17.598	2465	2467	2475	rVB5	10438	16610	0.16%	0.020%
31	18.116	2550	2555	2560	rBV2	66414	90447	0.85%	0.110%
32	18.222	2570	2573	2575	rBV2	9910	11864	0.11%	0.014%
33	18.434	2606	2609	2613	rVB3	21333	24059	0.22%	0.029%
34	18.575	2631	2633	2640	rVB7	14515	23058	0.22%	0.028%
35	19.134	2724	2728	2734	rBV2	70487	102743	0.96%	0.124%
36	19.204	2736	2740	2744	rBV	80335	109717	1.03%	0.133%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018661.D
Acq On : 07 Dec 2023 05:21
Operator : MA/JU
Sample : 05473-01
Misc :
ALS Vial : 104 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.345	2761	2764	2772	rBV4	56591	78807	0.74%	0.095%
38	19.563	2795	2801	2807	rBV	6822506	9137509	85.45%	11.067%
39	21.310	3093	3098	3108	rBV	3756584	4774494	44.65%	5.783%
40	23.533	3468	3476	3493	rVB2	5305586	10693691	100.00%	12.952%
41	23.686	3495	3502	3517	rVB	2633068	5311669	49.67%	6.433%




Sum of corrected areas: 82563221

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018661.D
Acq On : 07 Dec 2023 05:21
Operator : MA/JU
Sample : 05473-01
Misc :
ALS Vial : 104 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

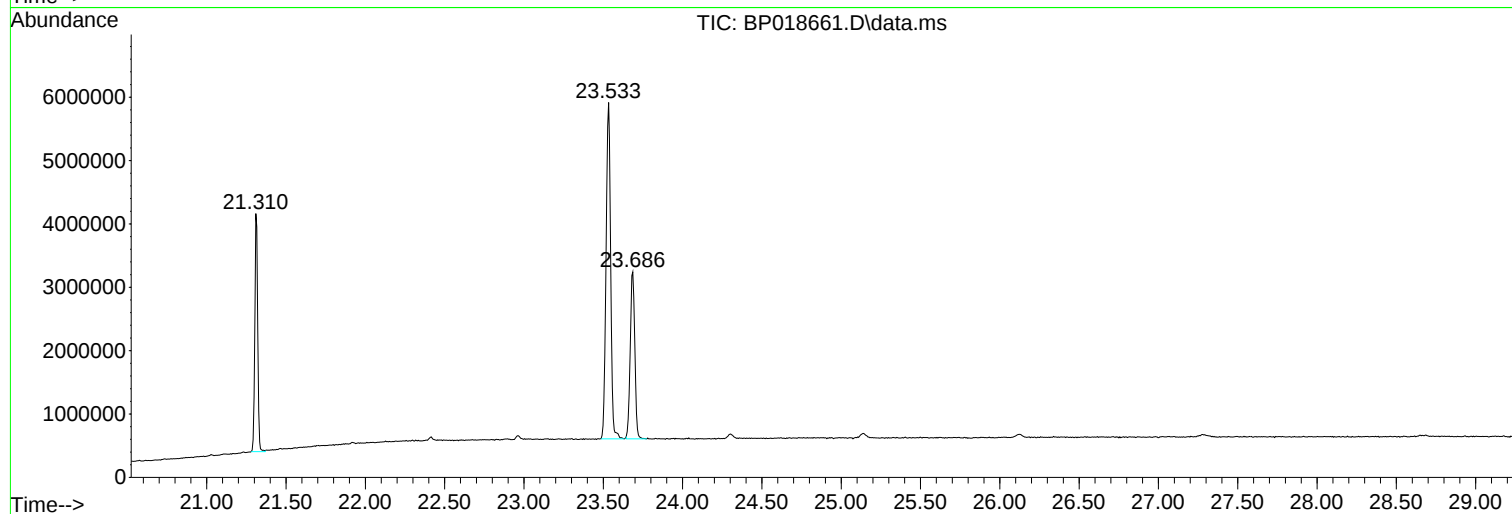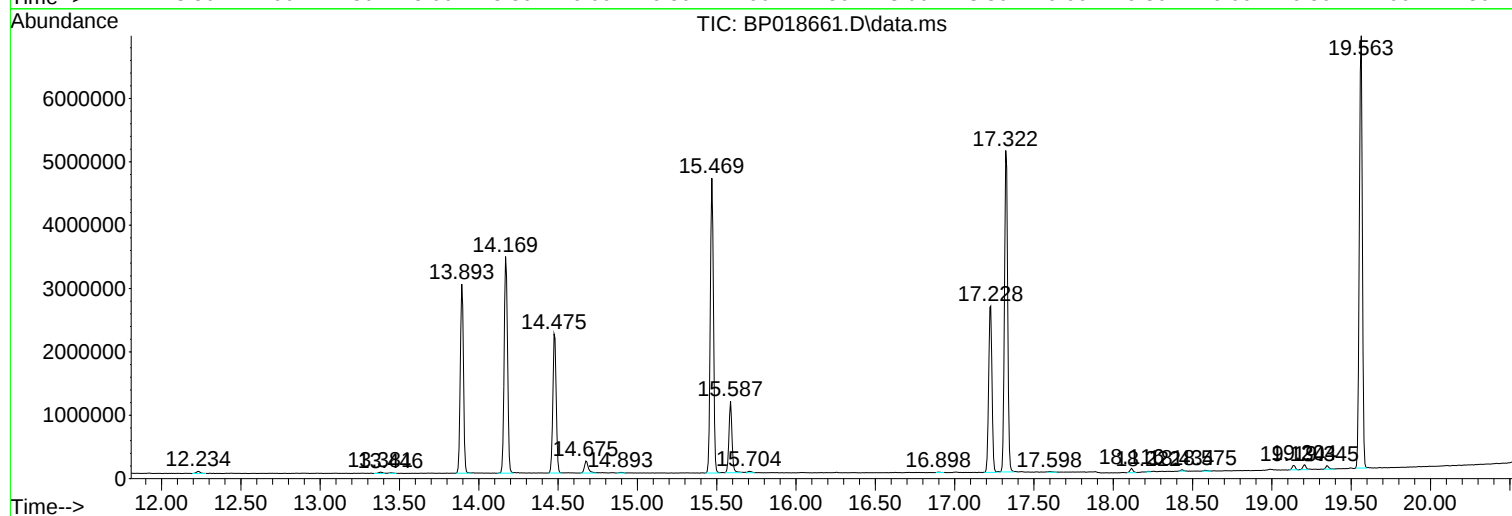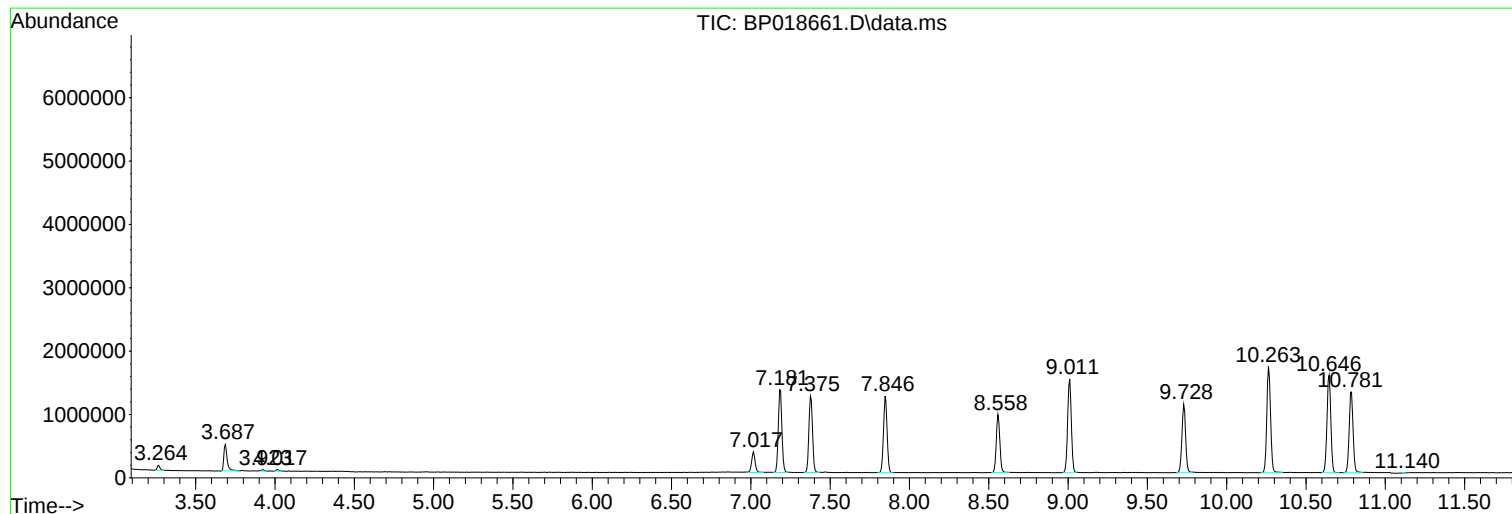

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018661.D
Acq On : 07 Dec 2023 05:21
Operator : MA/JU
Sample : 05473-01
Misc :
ALS Vial : 104 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018661.D
Acq On : 07 Dec 2023 05:21
Operator : MA/JU
Sample : 05473-01
Misc :
ALS Vial : 104 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------