


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP120519\
Data File : BP001202.D
Acq On : 05 Dec 2019 10:27
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 17:15:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 05 12:34:47 2019
Response via : Initial Calibration

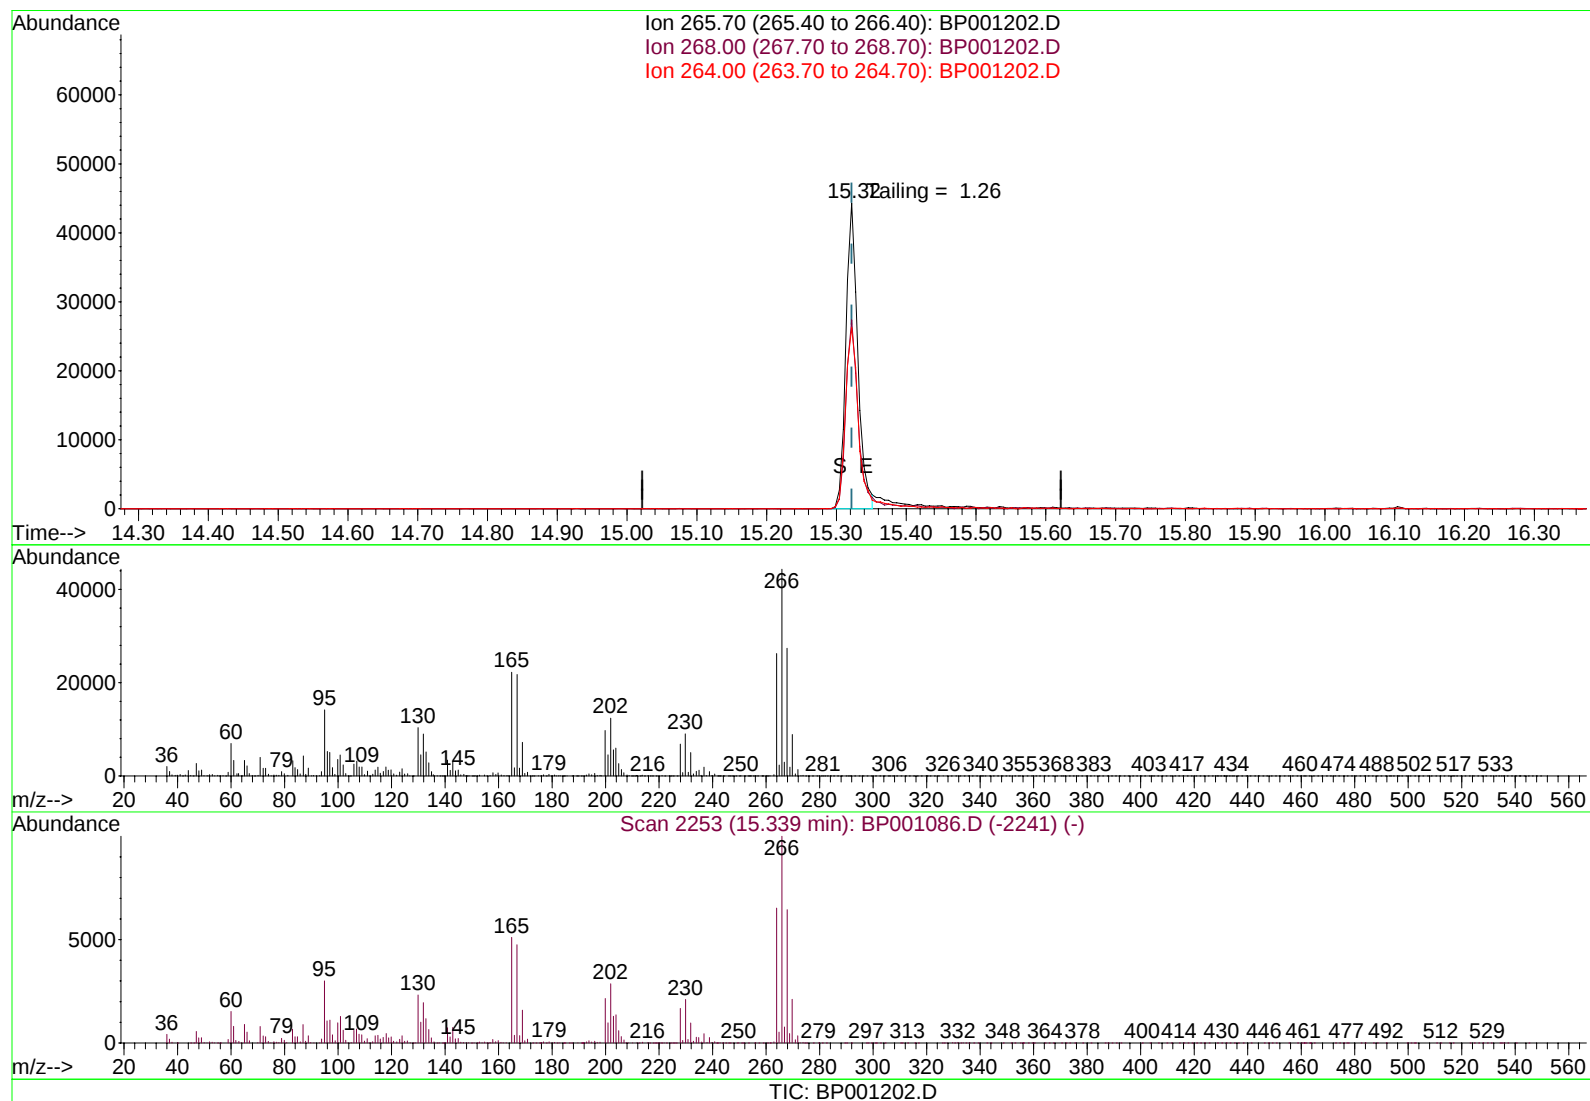

(70) Pentachlorophenol (C)




15.322min (-0.000) 704342.38ng

response 52579

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	61.76
264.00	62.40	59.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP120519\
Data File : BP001202.D
Acq On : 05 Dec 2019 10:27
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 17:15:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 05 12:34:47 2019
Response via : Initial Calibration

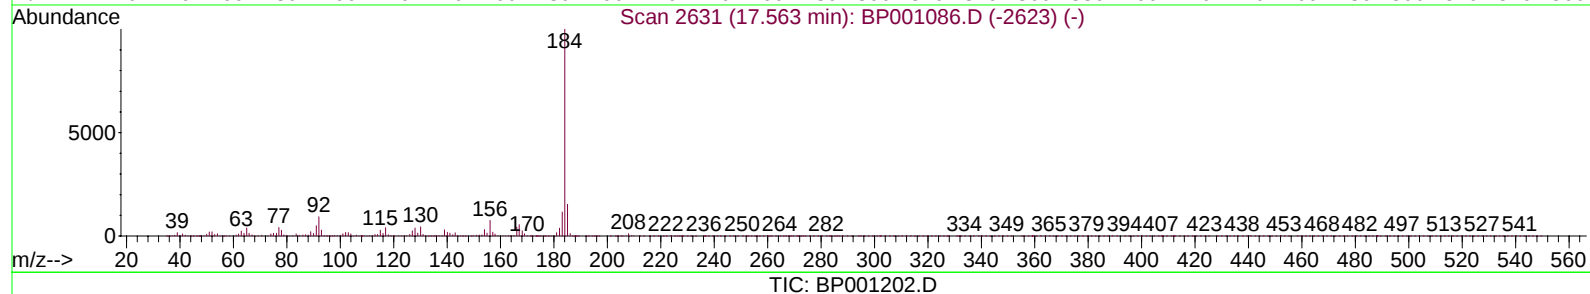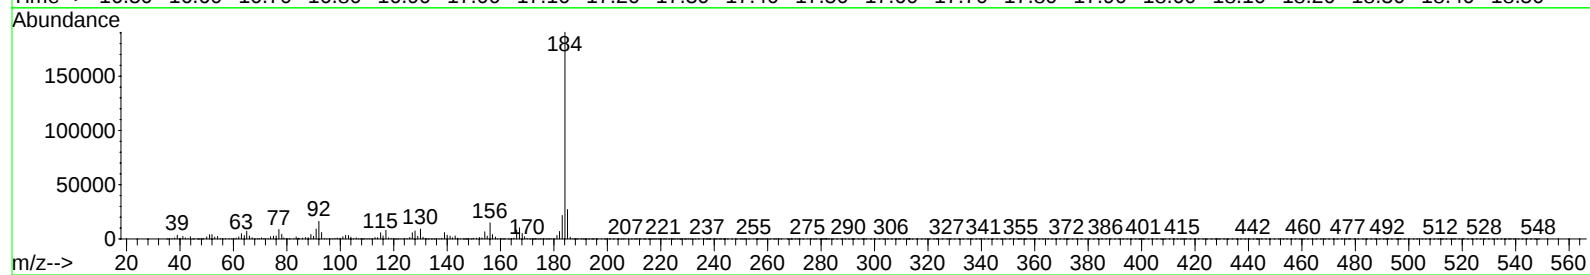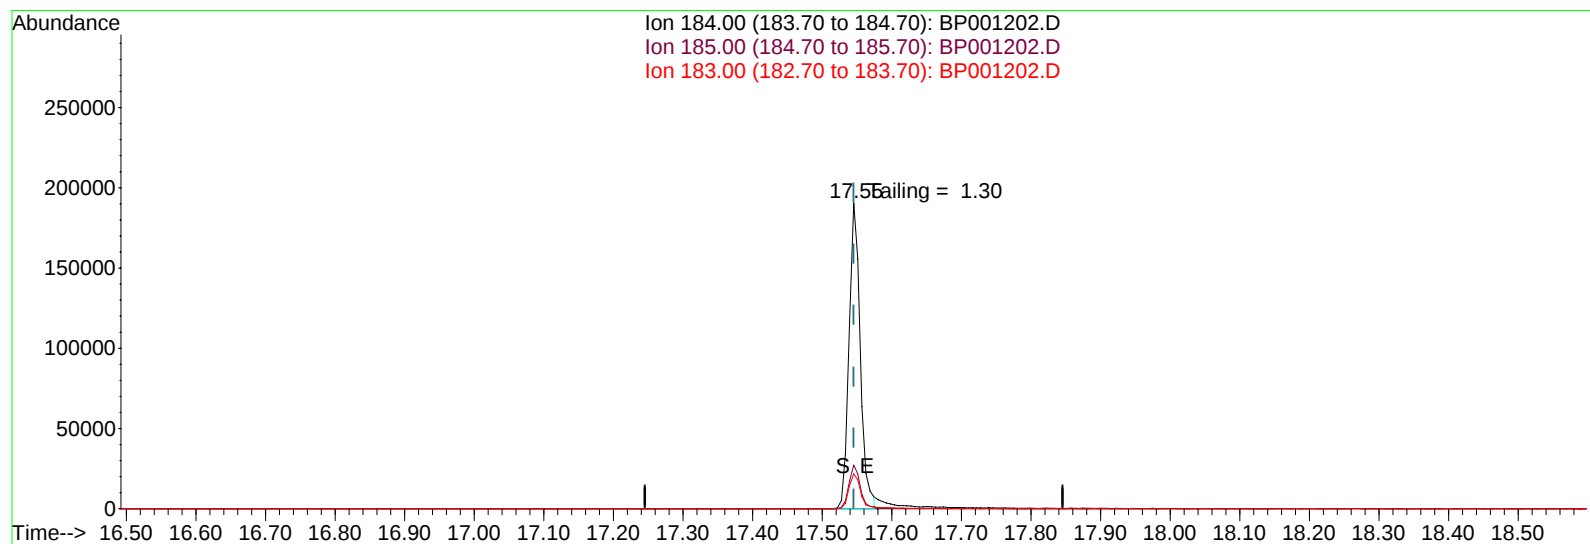

(77) Benzidine

17.545min (-0.000) 120523.47ng

response 211604

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.28
183.00	11.20	11.40
0.00	0.00	0.00