

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP120519\
 Data File : BP001206.D
 Acq On : 05 Dec 2019 12:30
 Operator : JU
 Sample : PB125191BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB125191BL

Quant Time: Dec 05 13:46:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 05 12:34:47 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.31	152	78724	20.00	ng	0.00
21) Naphthalene-d8	10.35	136	287316	20.00	ng	0.00
39) Acenaphthene-d10	13.21	164	163171	20.00	ng	0.00
64) Phenanthrene-d10	15.60	188	332542	20.00	ng	0.00
76) Chrysene-d12	19.24	240	276805	20.00	ng	-0.01
87) Perylene-d12	21.02	264	291019	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	6.22	112	471939	99.46	ng	0.00
7) Phenol-d6	7.75	99	396768	62.76	ng	-0.01
23) Nitrobenzene-d5	9.19	82	705900	106.59	ng	0.00
42) 2,4,6-Tribromophenol	14.50	330	281941	180.27	ng	0.00
45) 2-Fluorobiphenyl	12.13	172	1168636	104.82	ng	0.00
79) Terphenyl-d14	17.89	244	1612831	107.80	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP120519\
Data File : BP001206.D
Acq On : 05 Dec 2019 12:30
Operator : JU
Sample : PB125191BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB125191BL

Quant Time: Dec 05 13:46:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 05 12:34:47 2019
Response via : Initial Calibration

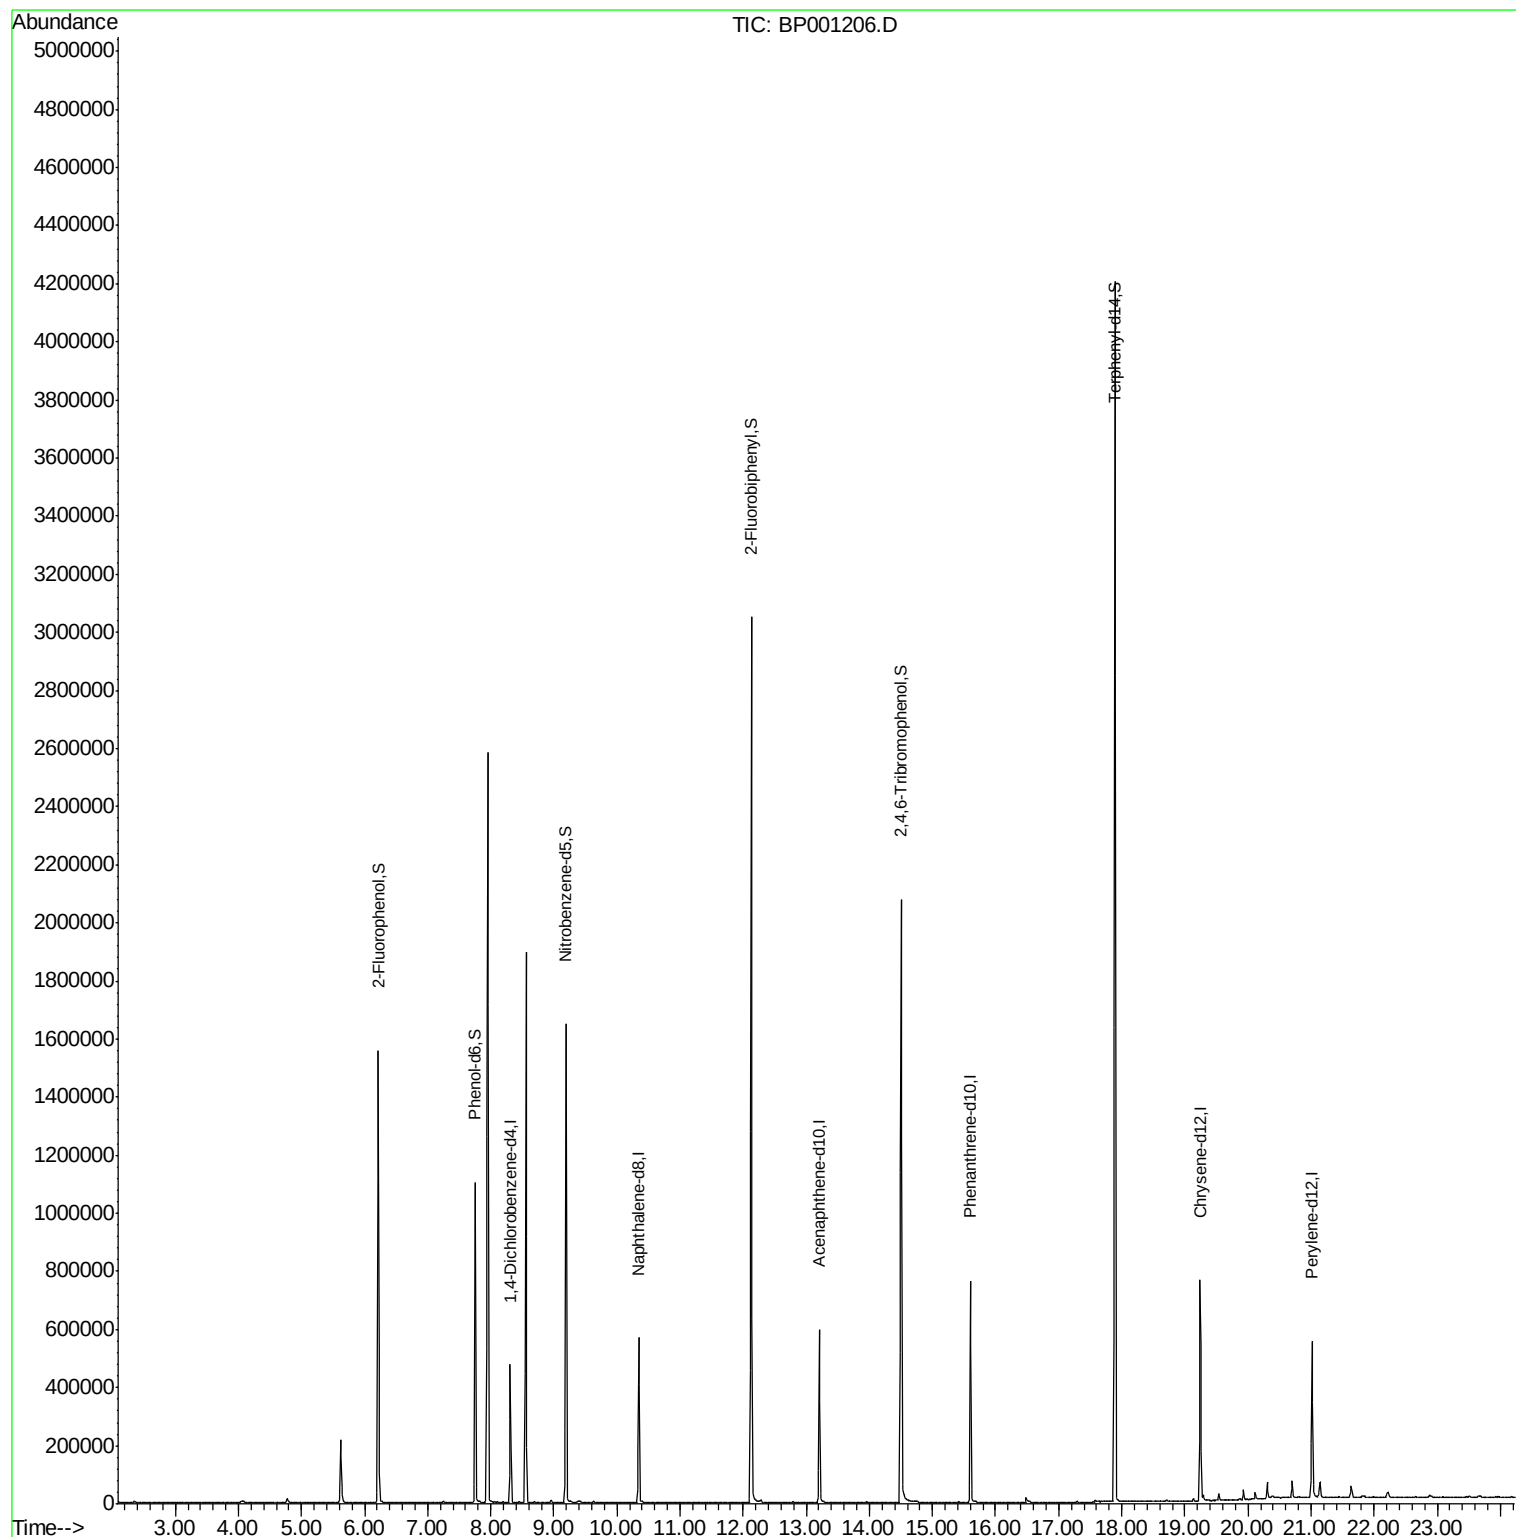

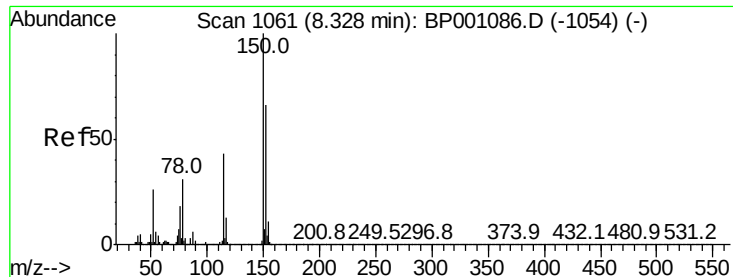

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.31 min Scan# 1058

Delta R.T. -0.00 min

Lab File: BP001206.D

Acq: 05 Dec 2019 12:30

Instrument :

BNA_P

ClientSampleId :

PB125191BL


Tot Ion:152 Resp: 78724

Ion Ratio Lower Upper

152 100

150 161.9 127.3 190.9

115 72.7 56.0 84.0



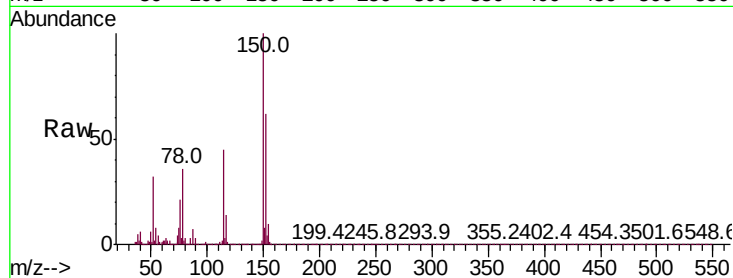


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

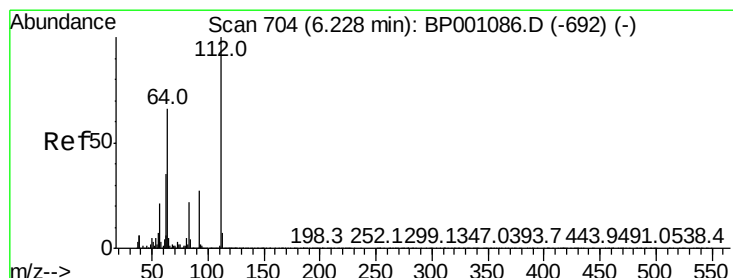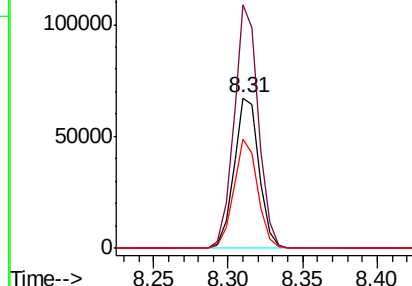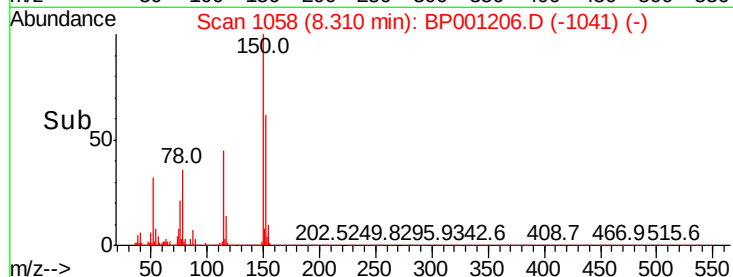

#5

2-Fluorophenol

Concen: 99.460 ng

RT: 6.22 min Scan# 702

Delta R.T. 0.01 min

Lab File: BP001206.D

Acq: 05 Dec 2019 12:30


Tgt Ion:112 Resp: 471939

Ion Ratio Lower Upper

112 100

64 70.4 56.8 85.2

63 41.2 32.2 48.2


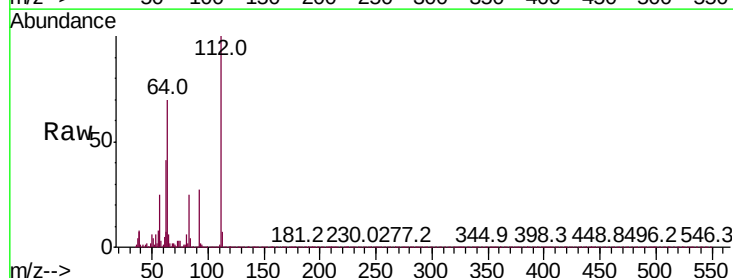



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BP0

Ion 63.00 (62.70 to 63.70): BP0

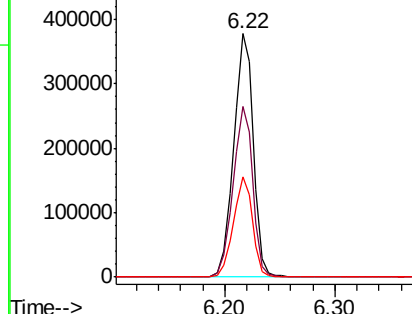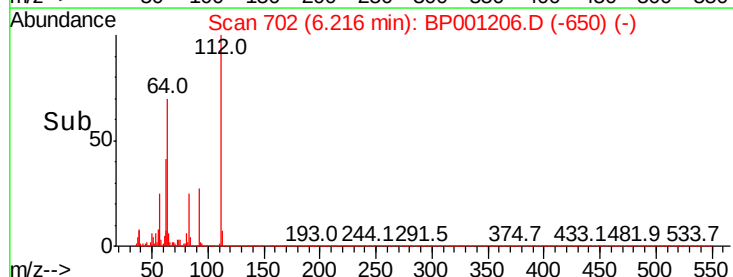

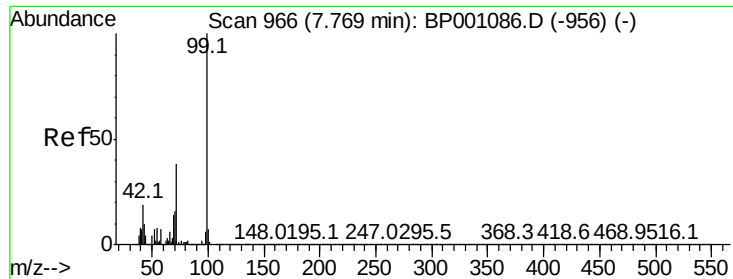

#7

Phenol-d6

Concen: 62.764 ng

RT: 7.75 min Scan# 963

Delta R.T. -0.01 min

Lab File: BP001206.D

Acq: 05 Dec 2019 12:30

Instrument :

BNA_P

ClientSampleId :

PB125191BL


Tot Ion: 99 Resp: 396768

Ion Ratio Lower Upper

99 100

42 23.5 17.6 26.4




71 44.3 33.8 50.8

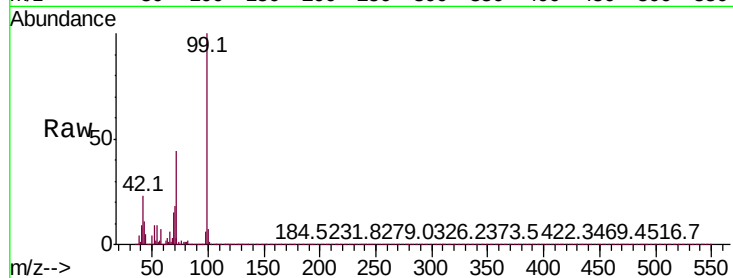

Abundance Ion 99.00 (98.70 to 99.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 71.00 (70.70 to 71.70): BP0

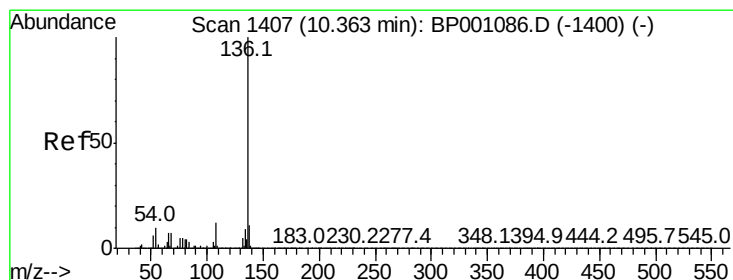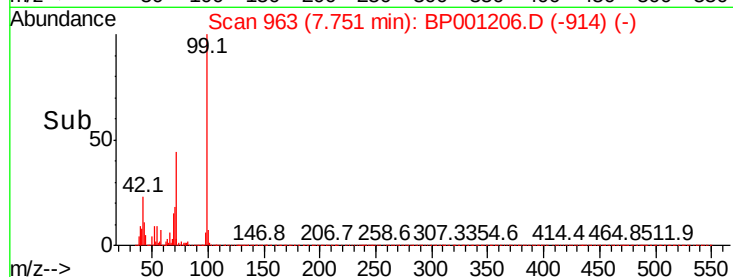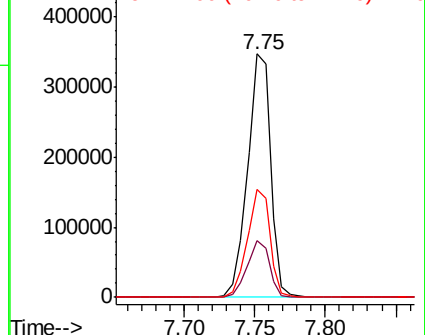

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.35 min Scan# 1404

Delta R.T. -0.01 min

Lab File: BP001206.D

Acq: 05 Dec 2019 12:30

Tgt Ion: 136 Resp: 287316


Ion Ratio Lower Upper

136 100

137 10.5 8.4 12.6

54 10.5 7.4 11.0

68 6.2 4.6 7.0


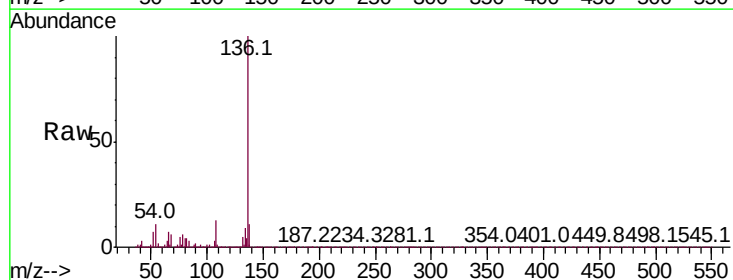



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BP0

Ion 68.00 (67.70 to 68.70): BP0



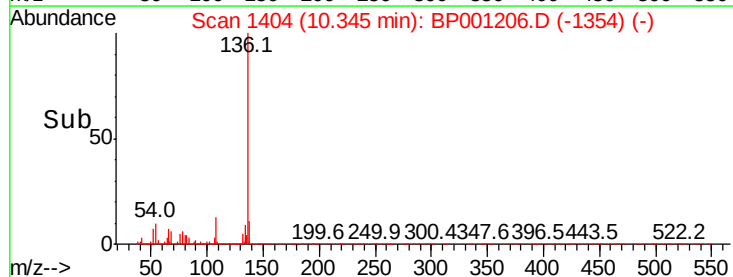
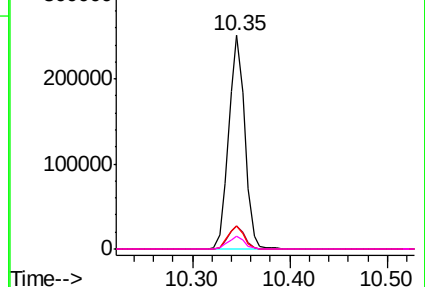


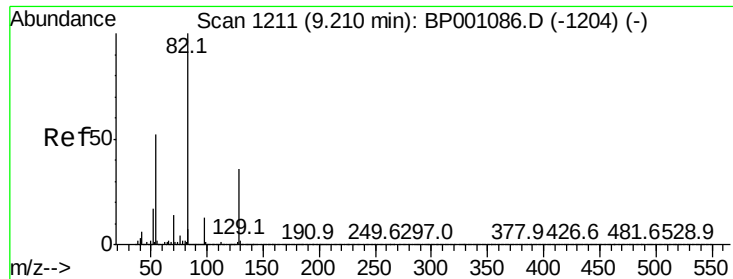

#23
 Nitrobenzene-d5
 Concen: 106.594 ng
 RT: 9.19 min Scan# 1208
 Delta R.T. -0.01 min
 Lab File: BP001206.D
 Acq: 05 Dec 2019 12:30




Instrument :
 BNA_P
 ClientSampleId :
 PB125191BL


Tot Ion	82	Resp	705900
Ion	Ratio	Lower	Upper
82	100		
128	33.7	27.5	41.3
54	57.0	45.7	68.5

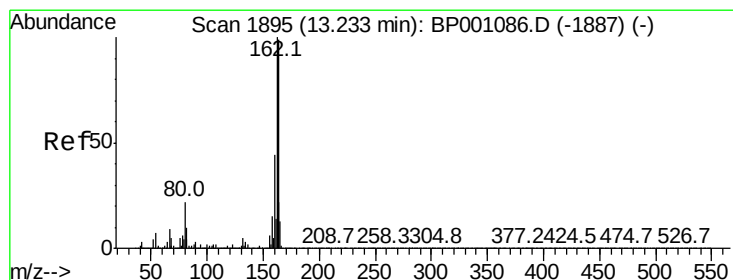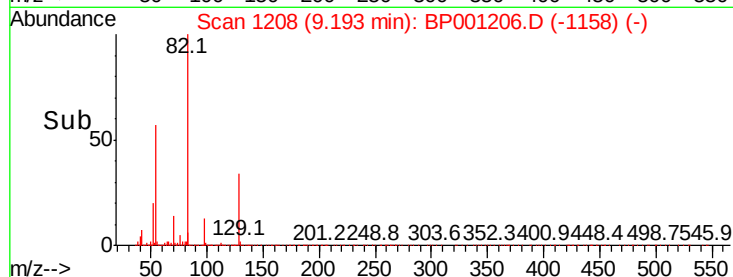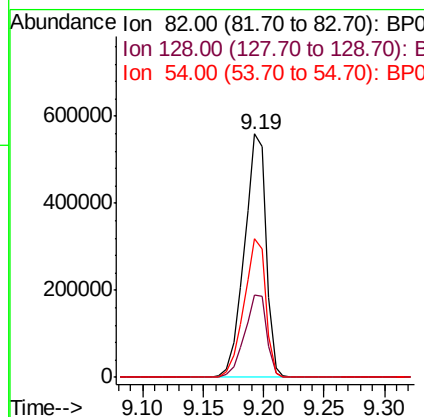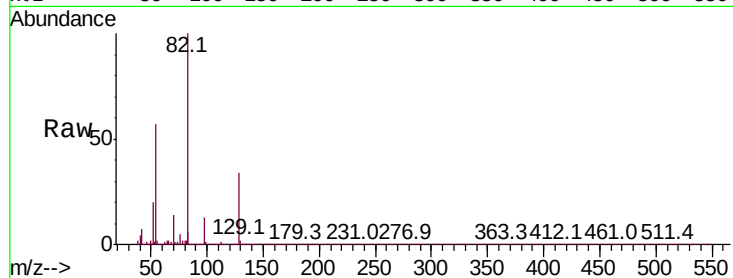

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 13.21 min Scan# 1891
 Delta R.T. -0.00 min
 Lab File: BP001206.D
 Acq: 05 Dec 2019 12:30

Tgt Ion	164	Resp	163171
Ion	Ratio	Lower	Upper
164	100		
162	102.2	80.7	121.1
160	46.9	36.3	54.5

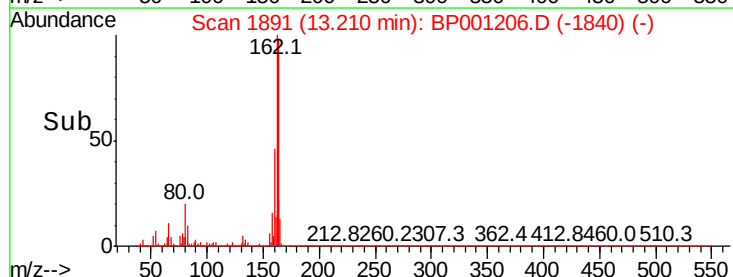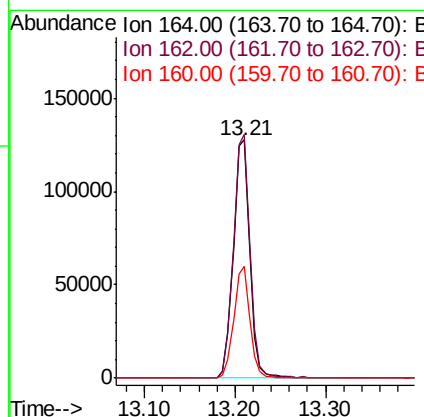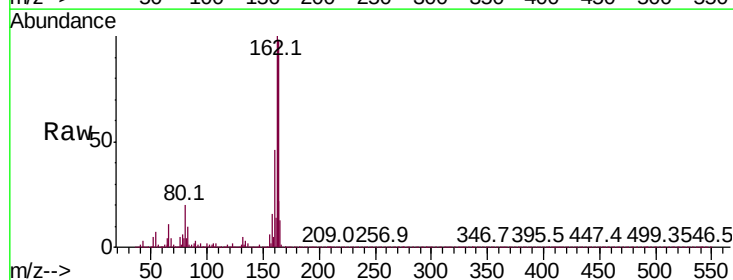


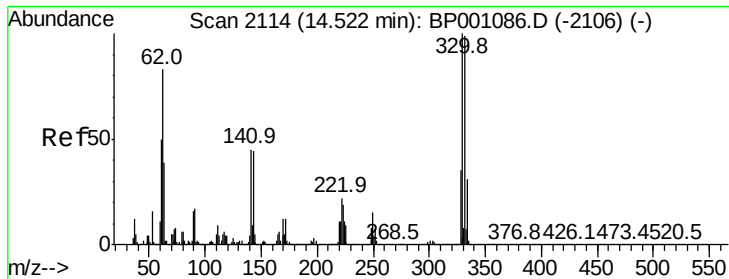

#42
2,4,6-Tribromophenol
Concen: 180.270 ng
RT: 14.50 min Scan# 2111
Delta R.T. -0.00 min
Lab File: BP001206.D
Acq: 05 Dec 2019 12:30

Instrument :
BNA_P
ClientSampleId :
PB125191BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.6	79.1	118.7
141	45.7	35.9	53.9



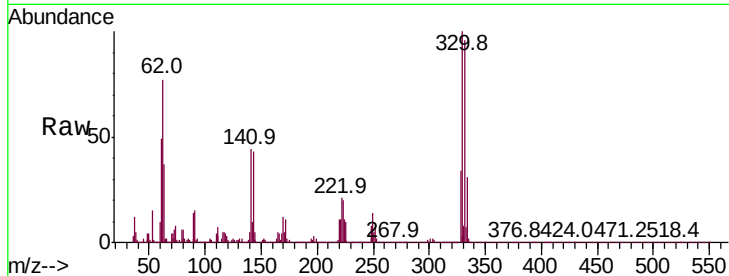


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

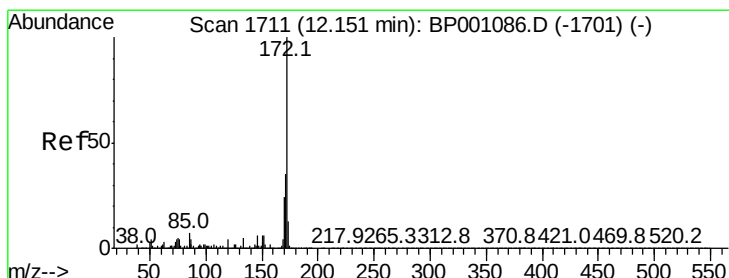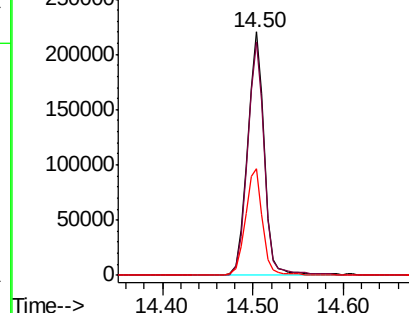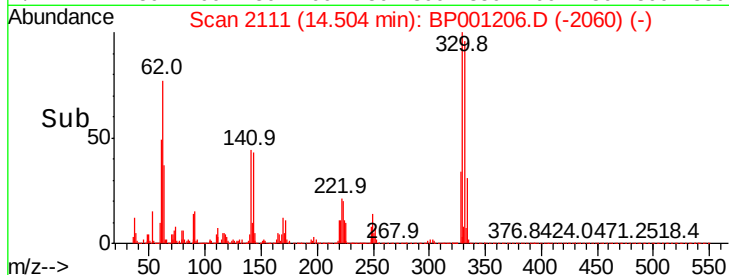

#45
2-Fluorobiphenyl
Concen: 104.822 ng
RT: 12.13 min Scan# 1707
Delta R.T. -0.01 min
Lab File: BP001206.D
Acq: 05 Dec 2019 12:30

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.6	28.7	43.1
170	23.4	19.2	28.8


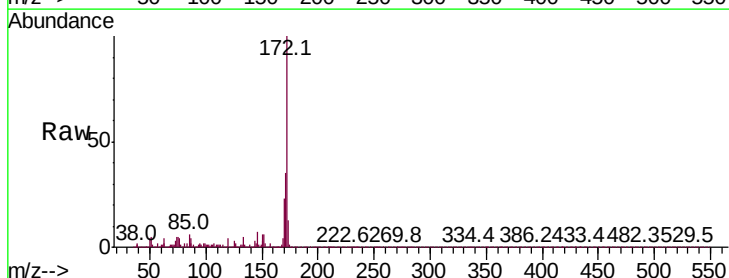



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

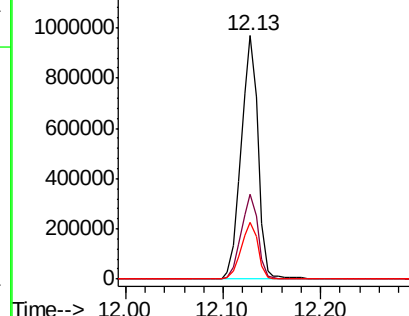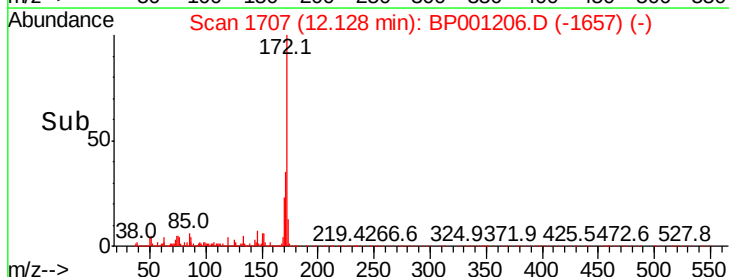

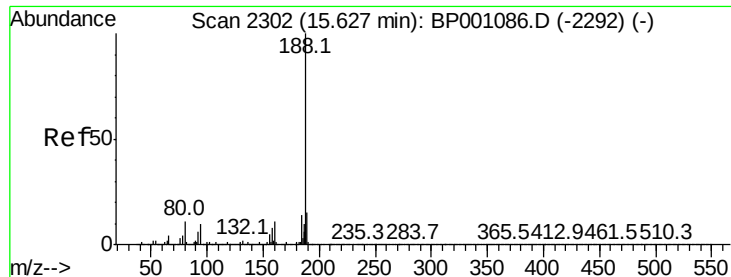

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 15.60 min Scan# 2298

Delta R.T. -0.01 min

Lab File: BP001206.D

Acq: 05 Dec 2019 12:30

Instrument :

BNA_P

ClientSampleId :

PB125191BL


Tot Ion:188 Resp: 332542

Ion Ratio Lower Upper

188 100

94 9.2 7.1 10.7




80 10.3 7.8 11.6

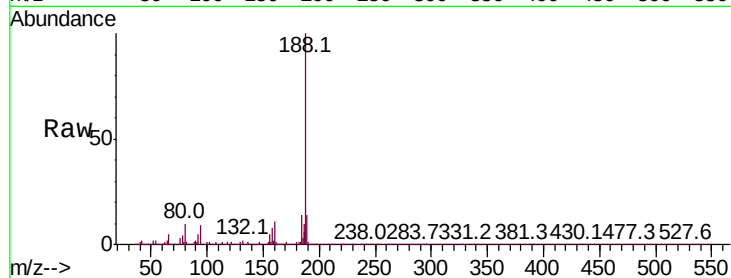

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BP0

Ion 80.00 (79.70 to 80.70): BP0

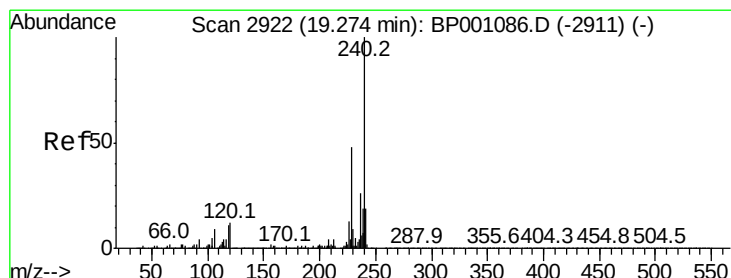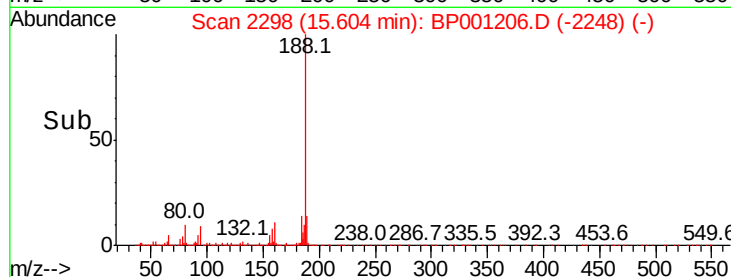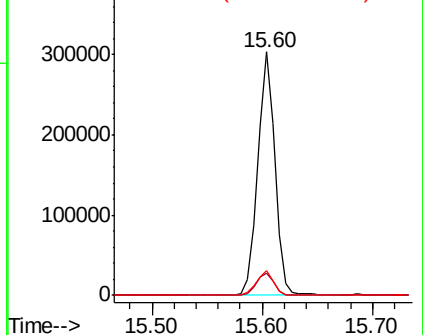

#76

Chrysene-d12

Concen: 20.000 ng

RT: 19.24 min Scan# 2917

Delta R.T. -0.01 min

Lab File: BP001206.D

Acq: 05 Dec 2019 12:30


Tgt Ion:240 Resp: 276805

Ion Ratio Lower Upper

240 100

120 10.3 7.0 10.6



236 26.3 21.7 32.5

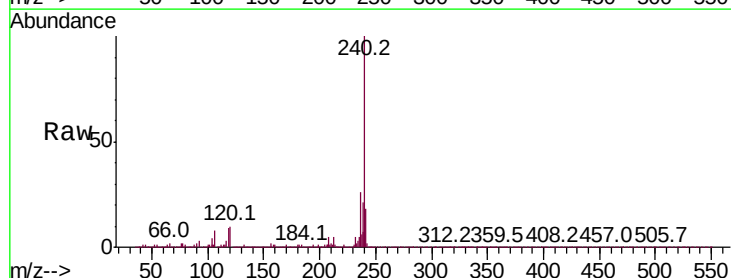


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

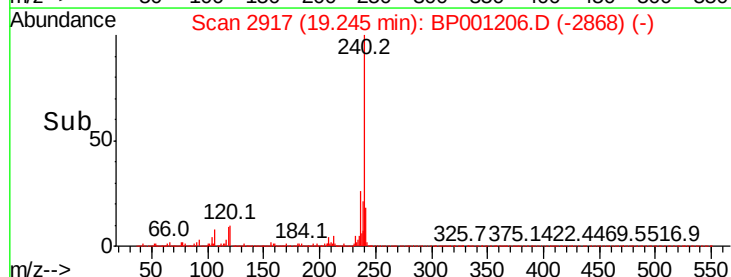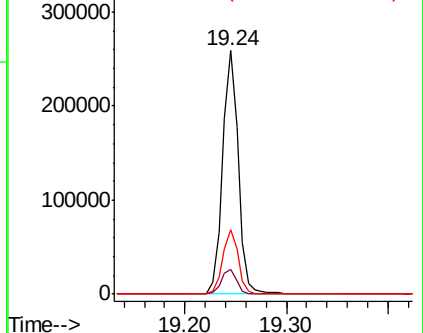

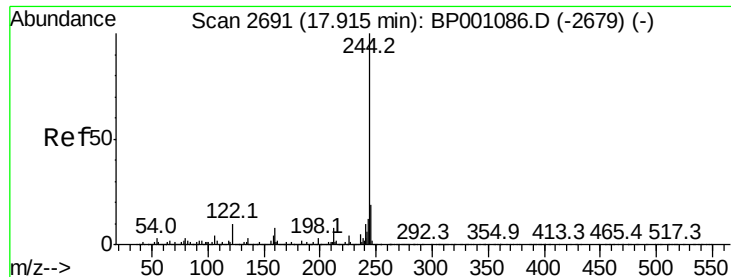

#79

Terphenyl-d14

Concen: 107.797 ng

RT: 17.89 min Scan# 2687

Delta R.T. -0.00 min

Lab File: BP001206.D

Acq: 05 Dec 2019 12:30

Instrument :

BNA_P

ClientSampleId :

PB125191BL


Tot Ion:244 Resp: 1612831

Ion Ratio Lower Upper

244 100

212 8.3 6.6 9.8




122 10.9 9.2 13.8

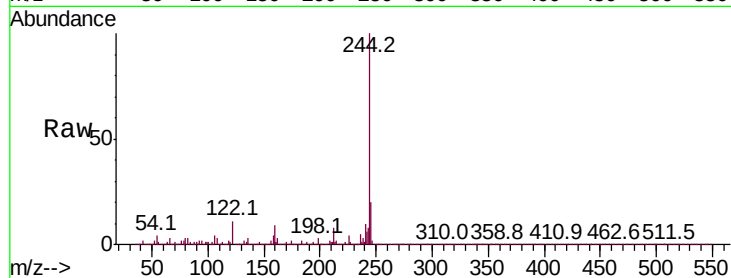

Abundance Ion 244.00 (243.70 to 244.70): E

2000000 Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

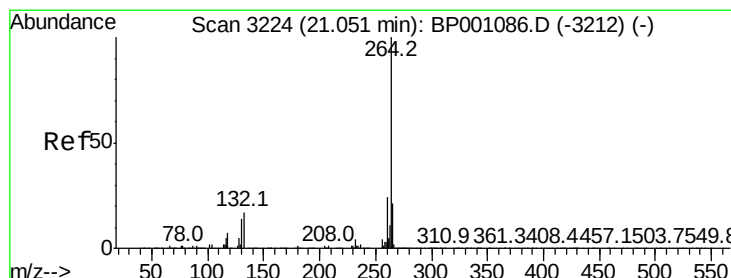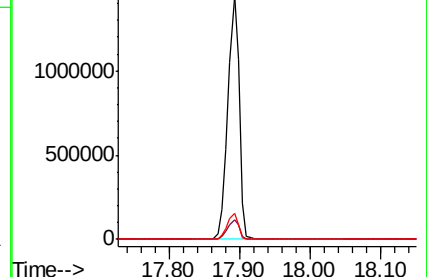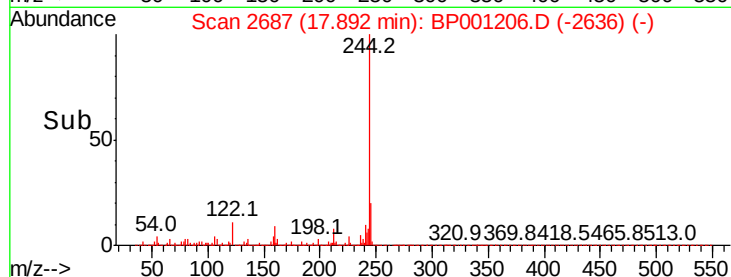

#87

Perylene-d12

Concen: 20.000 ng

RT: 21.02 min Scan# 3218

Delta R.T. -0.01 min

Lab File: BP001206.D

Acq: 05 Dec 2019 12:30


Tgt Ion:264 Resp: 291019

Ion Ratio Lower Upper

264 100

260 24.3 19.4 29.0

265 21.7 17.1 25.7

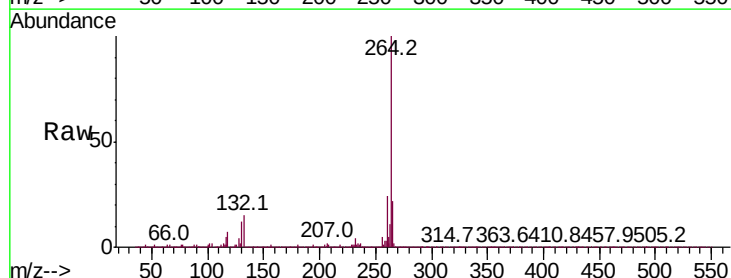

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

