


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120519\
 Data File : BP001202.D
 Acq On : 05 Dec 2019 10:27
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP112719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 05 12:34:47 2019

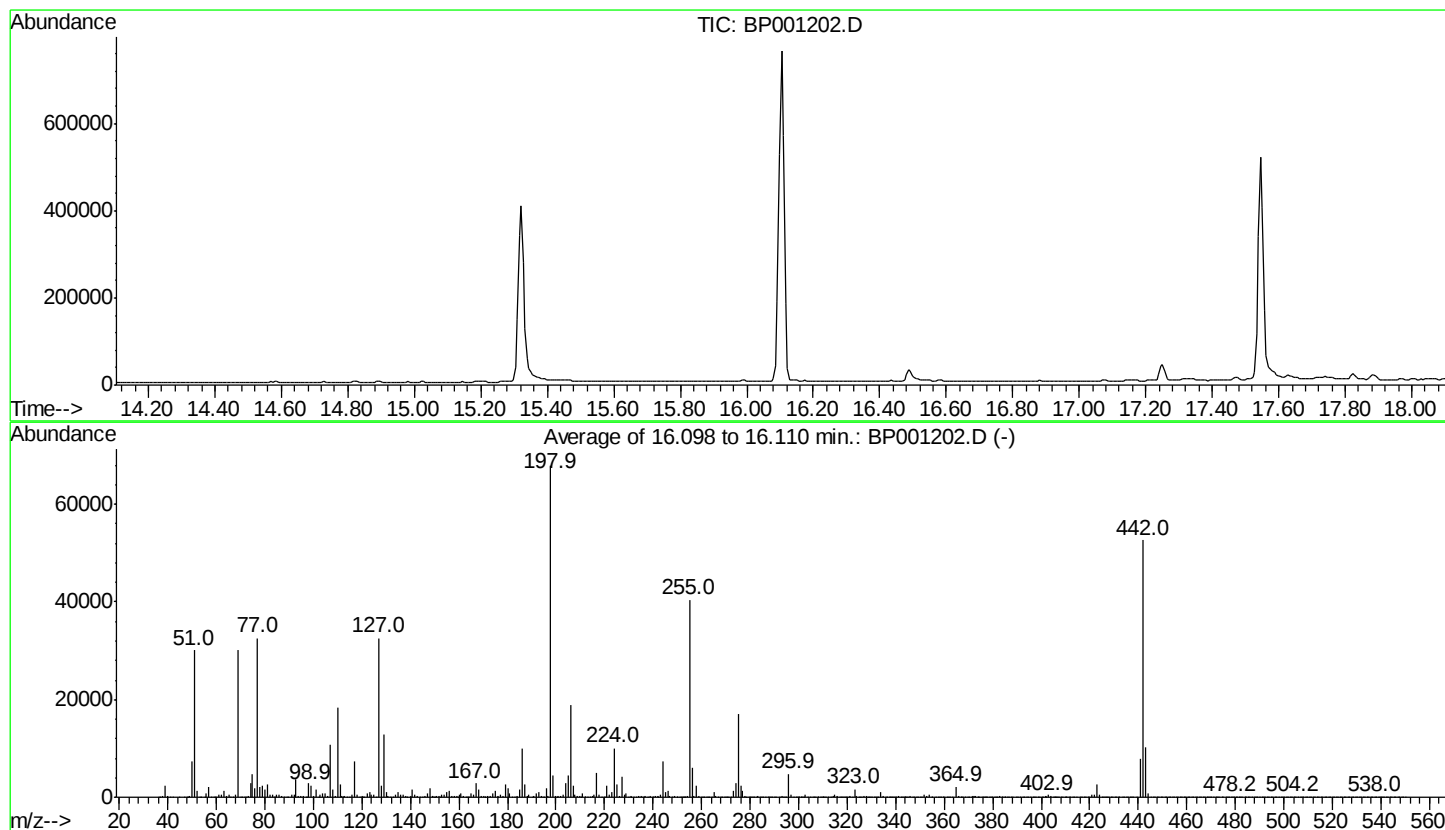

AutoFind: Scans 2382, 2383, 2384; Background Corrected with Scan 2375

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.4	30131	PASS
68	69	0.00	2	1.7	514	PASS
69	198	0.00	100	44.3	30094	PASS
70	69	0.00	2	0.5	137	PASS
127	198	10	80	48.0	32636	PASS
197	198	0.00	2	0.3	177	PASS
198	198	100	100	100.0	67928	PASS
199	198	5	9	6.6	4509	PASS
275	198	10	60	25.0	16978	PASS
365	198	1	100	3.1	2102	PASS
441	198	0.01	100	11.6	7874	PASS
442	198	50	100	77.6	52685	PASS
443	442	15	24	19.5	10262	PASS