
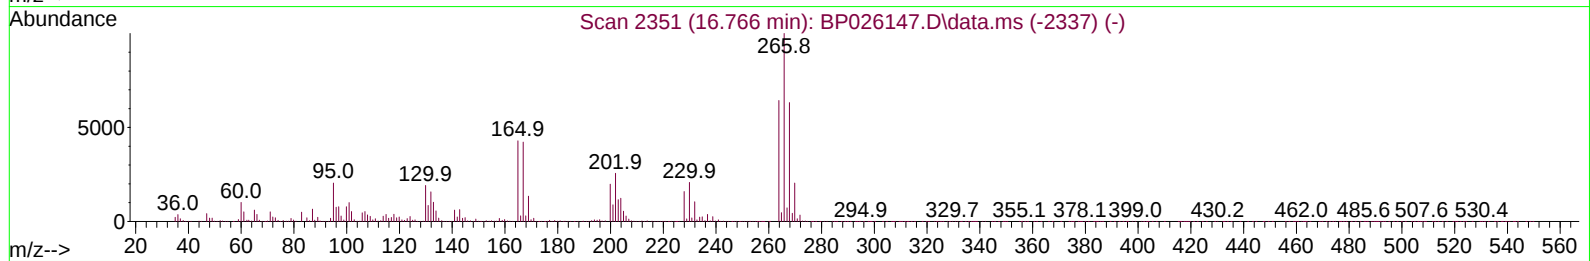
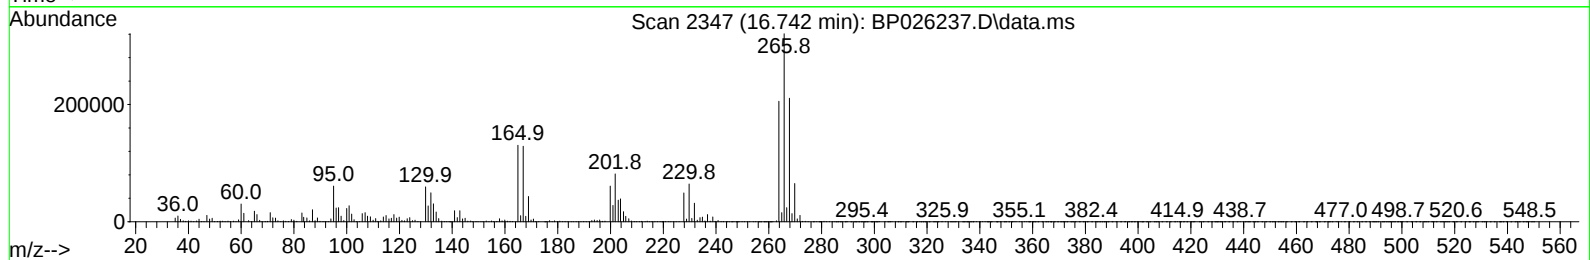


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120525\
Data File : BP026237.D
Acq On : 05 Dec 2025 13:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 14:23:25 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

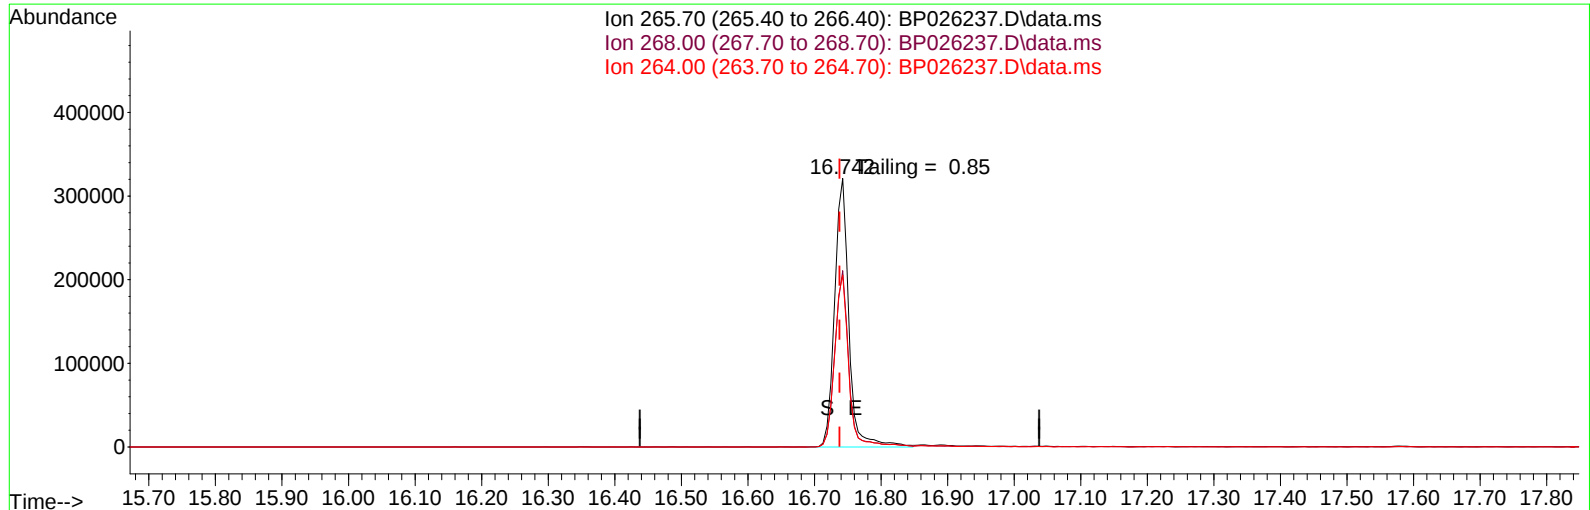

TIC: BP026237.D\data.ms

(70) Pentachlorophenol (C)




16.742min (+ 0.005) 103335.46 ng

response 479322

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	65.68
264.00	62.70	64.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120525\
Data File : BP026237.D
Acq On : 05 Dec 2025 13:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 14:23:25 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

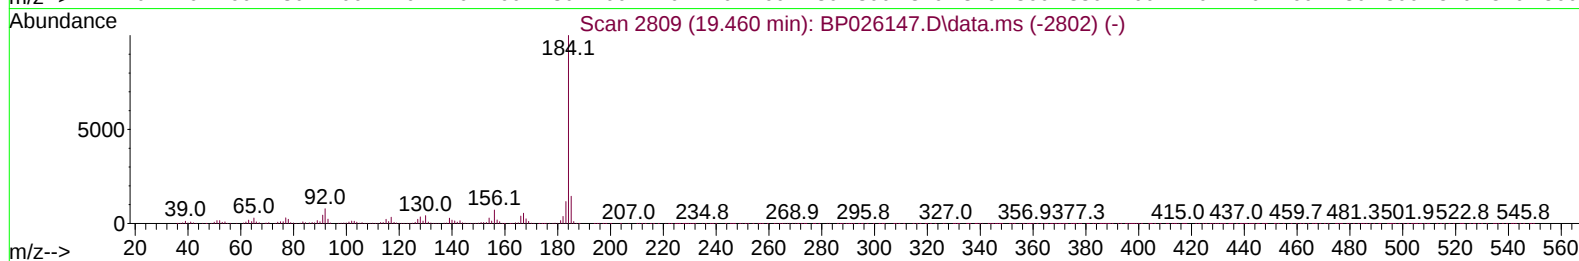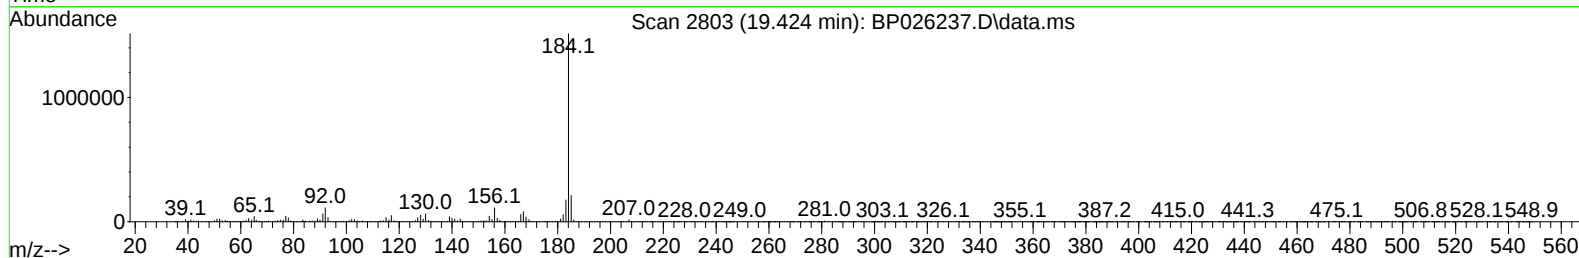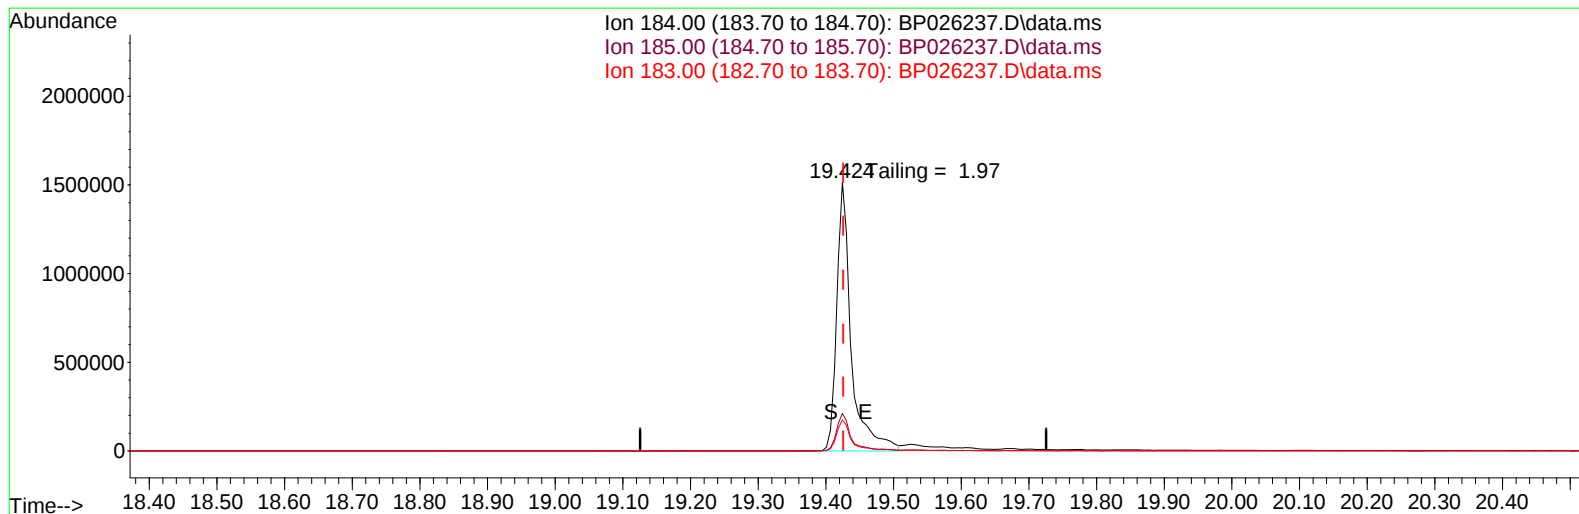

TIC: BP026237.D\data.ms

(77) Benzidine

19.424min (-0.001) 39177.70 ng

response 2267840

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.00
183.00	11.30	11.57
0.00	0.00	0.00