


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120525\
Data File : BP026238.D
Acq On : 05 Dec 2025 13:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 05 14:52:44 2025

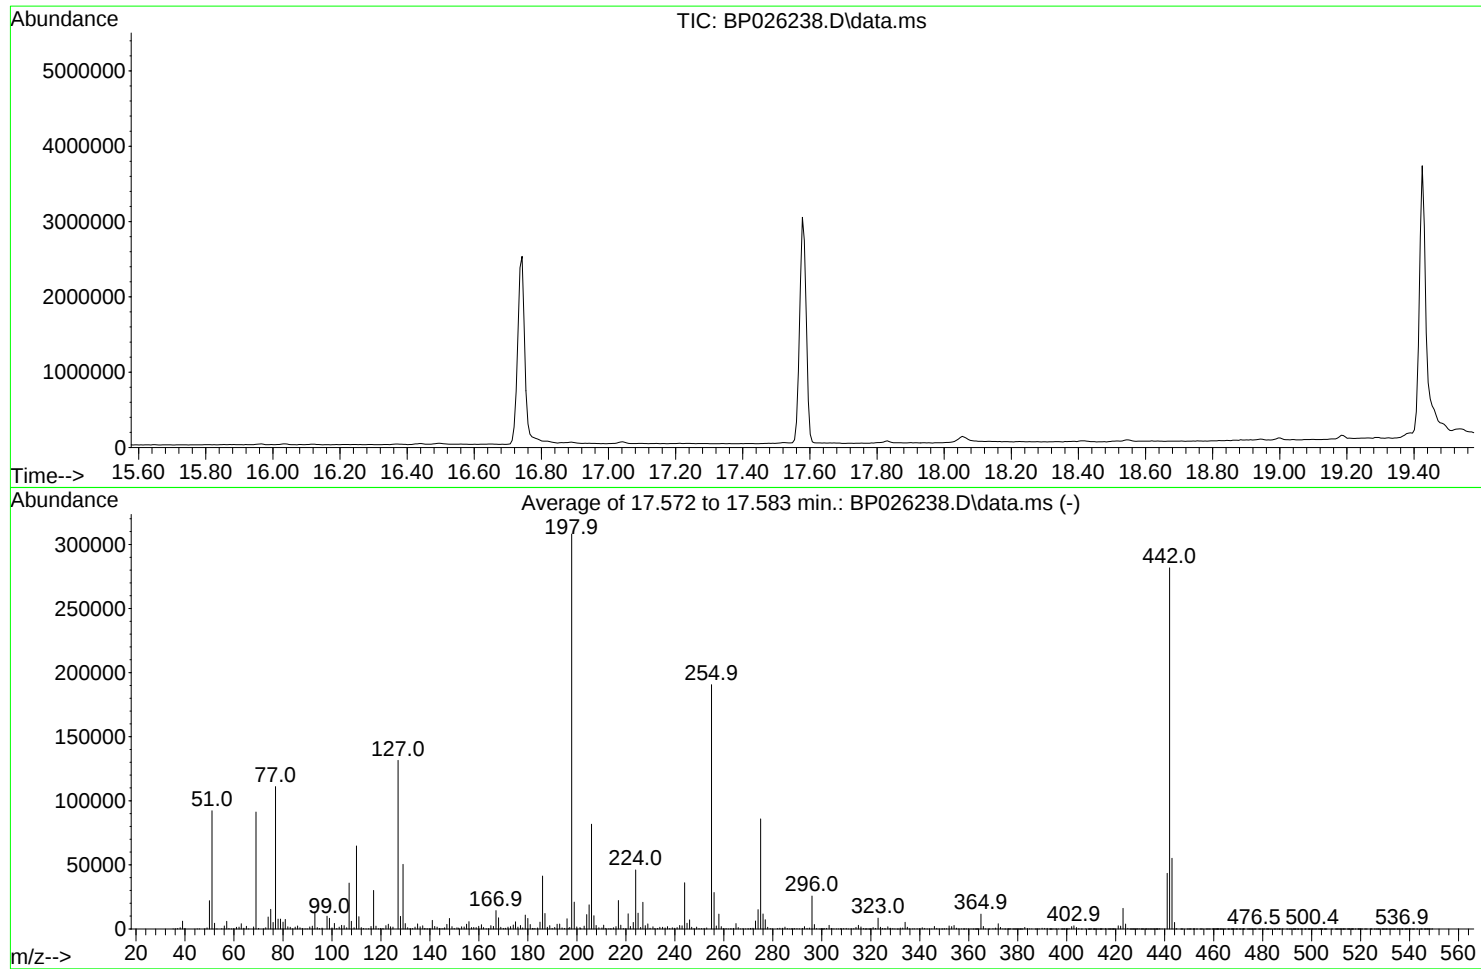




AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	1573	PASS
69	69	100	100	100.0	91164	PASS
70	69	0.00	2	0.5	413	PASS
197	198	0.00	2	0.4	1187	PASS
198	198	100	100	100.0	308073	PASS
199	198	5	9	6.8	20884	PASS
365	198	1	100	3.7	11543	PASS
441	443	0.01	150	78.7	43384	PASS
442	442	100	100	100.0	281728	PASS
443	442	15	24	19.6	55094	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120525\
Data File : BP026238.D
Acq On : 05 Dec 2025 13:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 05 14:23:25 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

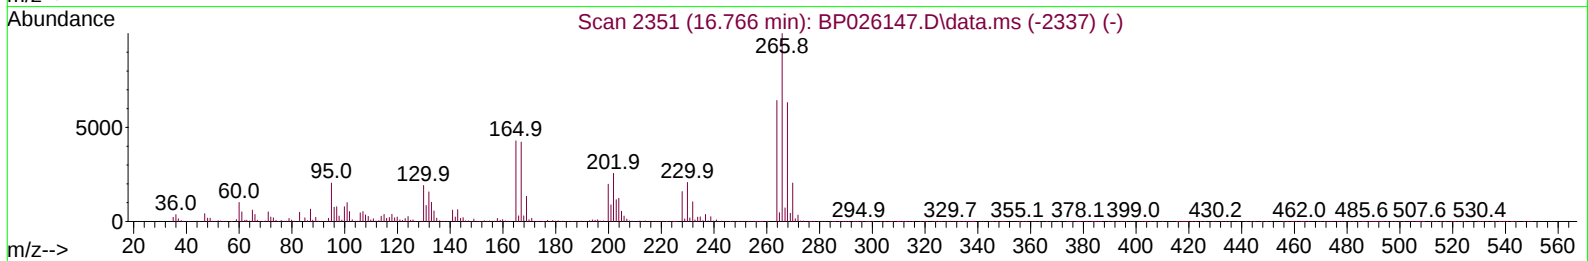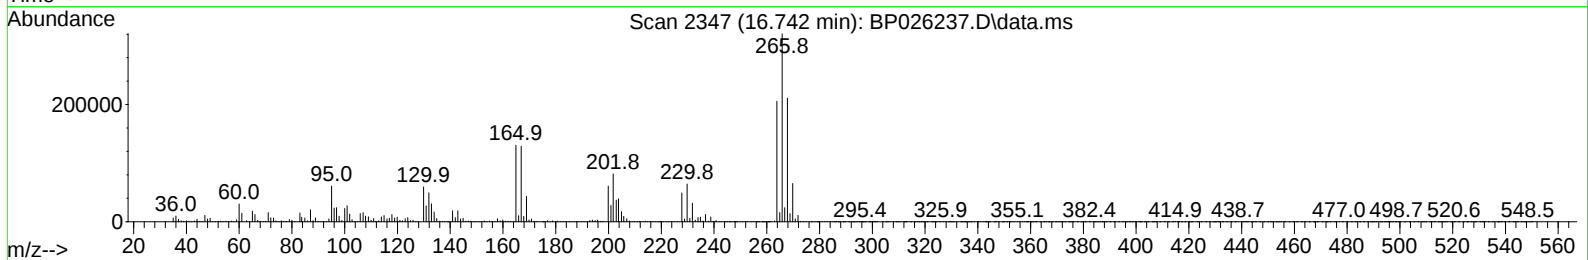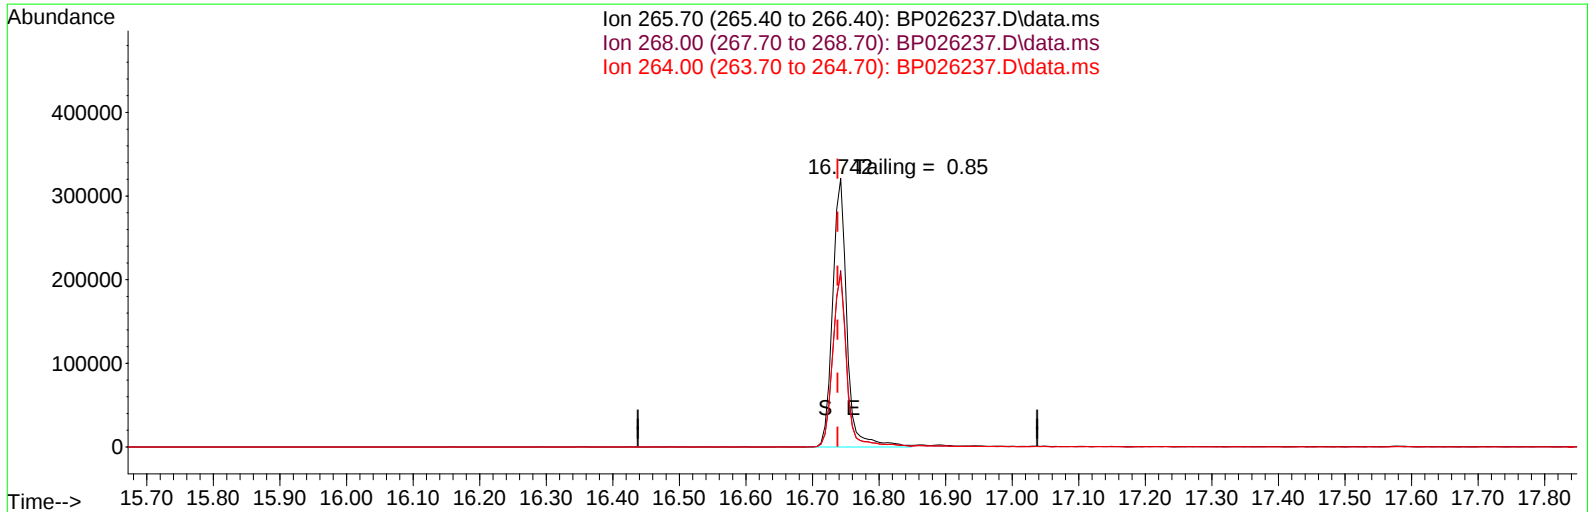

TIC: BP026237.D\data.ms

(70) Pentachlorophenol (C)

16.742min (+ 0.005) 103335.46 ng




response 479322

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	65.68
264.00	62.70	64.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120525\
Data File : BP026238.D
Acq On : 05 Dec 2025 13:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 05 14:23:25 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

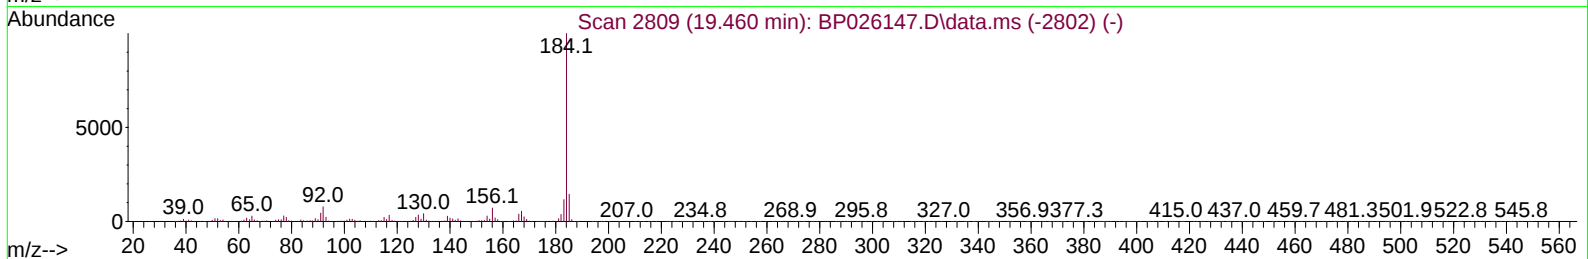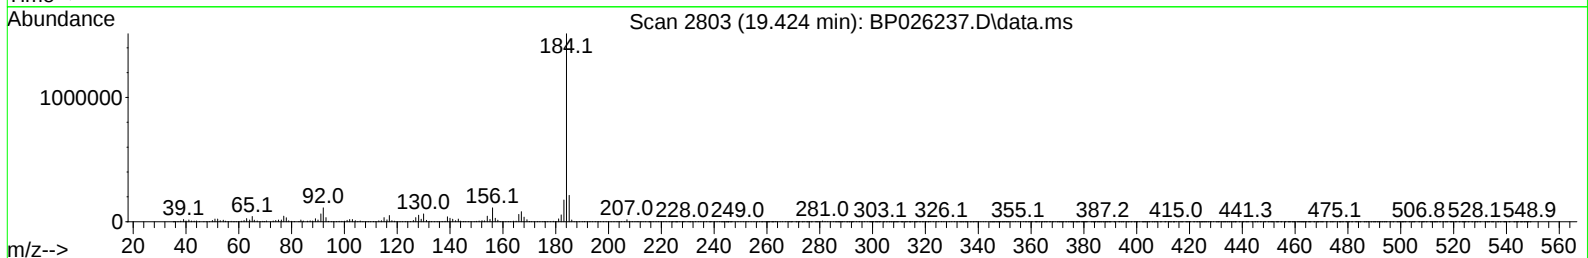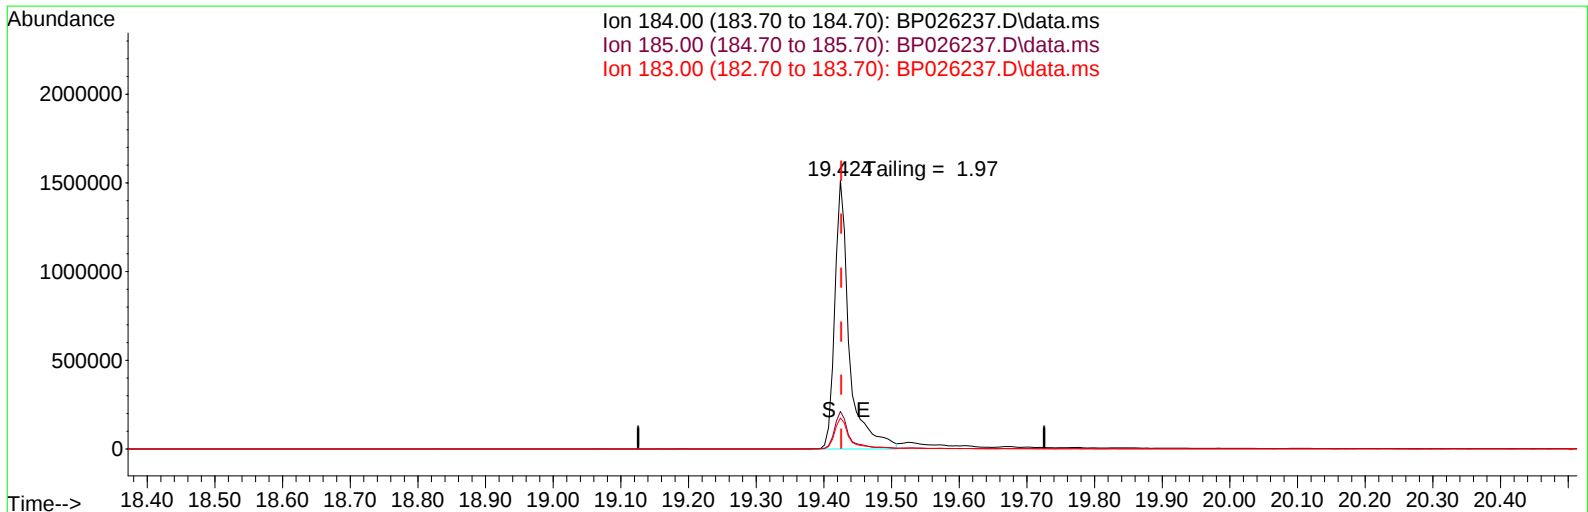

TIC: BP026237.D\data.ms

(77) Benzidine

19.424min (-0.001) 39177.70 ng

response 2267840

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.00
183.00	11.30	11.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/5/2025	BNA_P	BP026238.D
Compound Name	Response	Retention Time
DDT	1342620	20.73
DDD	14969	20.271
DDE	4845	19.736
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19814	1362434	1.45

Instrument :
BNA_P
ClientSampleId :
DFTPP