

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP120619\
 Data File : BP001244.D
 Acq On : 06 Dec 2019 22:21
 Operator : JU
 Sample : K6147-04 2X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Dec 07 00:42:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 05 12:34:47 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.31	152	81626	20.00	ng	0.00
21) Naphthalene-d8	10.35	136	303653	20.00	ng	0.00
39) Acenaphthene-d10	13.20	164	171085	20.00	ng	0.00
64) Phenanthrene-d10	15.60	188	320385	20.00	ng	0.00
76) Chrysene-d12	19.25	240	253033	20.00	ng	-0.01
87) Perylene-d12	21.02	264	257274	20.00	ng	0.00

System Monitoring Compounds						
5) 2-Fluorophenol	6.21	112	201631	40.98	ng	0.00
7) Phenol-d6	7.75	99	275551	42.04	ng	-0.01
23) Nitrobenzene-d5	9.19	82	186878	26.70	ng	-0.01
42) 2,4,6-Tribromophenol	14.49	330	72120	43.98	ng	-0.01
45) 2-Fluorobiphenyl	12.12	172	320166	27.39	ng	-0.01
79) Terphenyl-d14	17.88	244	356587	26.07	ng	-0.01


Target Compounds				Qvalue		
9) Benzaldehyde	7.60	77	3762	Below Cal		98
17) 2-Methylphenol	8.73	107	38336	8.210 ng		99
19) n-Nitroso-di-n-propylamine	9.19	70	28206	5.964 ng	#	79
31) Naphthalene	10.37	128	155106	10.001 ng		99
33) 4-Chloroaniline	10.37	127	21073	3.131 ng	#	29
37) 2-Methylnaphthalene	11.51	142	37847	3.576 ng		96
50) Dimethylphthalate	12.79	163	36742	2.871 ng		98
52) Acenaphthene	13.25	154	31730	3.332 ng		94
54) 2,4-Dinitrophenol	13.33	184	12	7.119 ng	#	1
55) Dibenzofuran	13.54	168	44487	3.109 ng		98
56) 4-Nitrophenol	13.54	139	19791	9.077 ng	#	1
58) Fluorene	14.10	166	36351	3.170 ng		99
65) 4,6-Dinitro-2-methylphenol	14.22	198	10	6.283 ng	#	1
71) Phenanthrene	15.63	178	174632	10.368 ng		99
72) Anthracene	15.72	178	48930	2.947 ng		98
75) Fluoranthene	17.35	202	113469	6.363 ng		99
78) Pyrene	17.65	202	91726	4.603 ng	#	95
81) Benzo(a)anthracene	19.23	228	44282	2.524 ng	#	91
83) Chrysene	19.27	228	44494	2.832 ng	#	85
84) Bis(2-ethylhexyl)phthalate	19.29	149	152630	12.060 ng	#	96
88) Benzo(b)fluoranthene	20.53	252	57405	3.653 ng	#	77
89) Benzo(k)fluoranthene	20.53	252	57405	3.793 ng	#	77
90) Benzo(a)pyrene	20.94	252	30384	2.099 ng	#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP120619\
Data File : BP001244.D
Acq On : 06 Dec 2019 22:21
Operator : JU
Sample : K6147-04 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Dec 07 00:42:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 05 12:34:47 2019
Response via : Initial Calibration

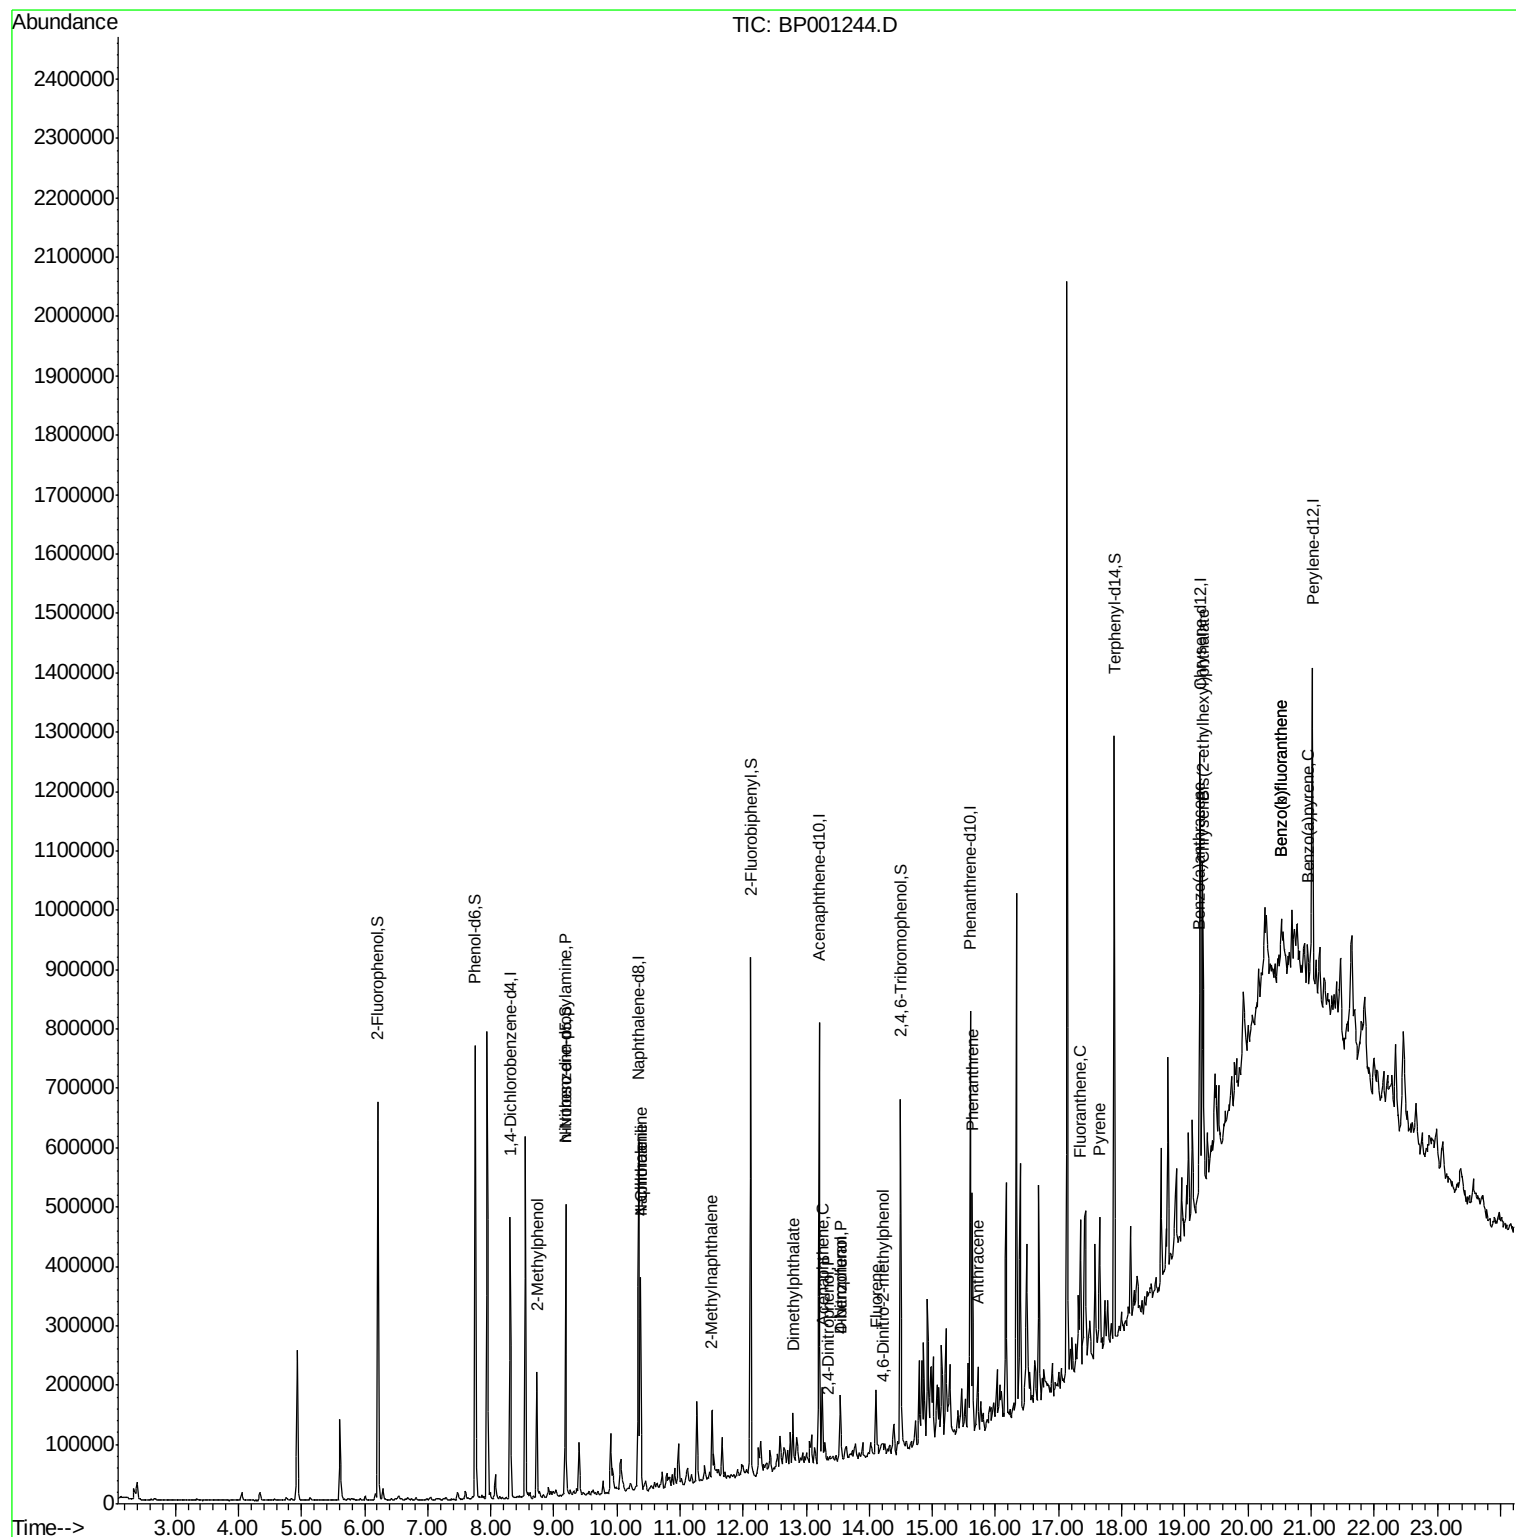



#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.31 min Scan# 1058

Delta R.T. -0.00 min

Lab File: BP001244.D

Acq: 06 Dec 2019 22:21

Instrument :

BNA_P

ClientSampled :


Tot Ion:152 Resp: 81626

Ion Ratio Lower Upper

152 100

150 152.2 127.3 190.9




115 66.6 56.0 84.0



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

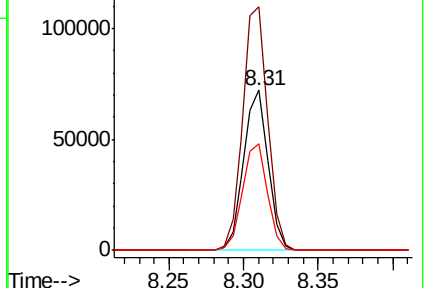

#5

2-Fluorophenol

Concen: 40.982 ng

RT: 6.21 min Scan# 701

Delta R.T. -0.00 min

Lab File: BP001244.D

Acq: 06 Dec 2019 22:21


Tgt Ion:112 Resp: 201631

Ion Ratio Lower Upper

112 100

64 72.3 56.8 85.2



63 43.0 32.2 48.2




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BP0

Ion 63.00 (62.70 to 63.70): BP0

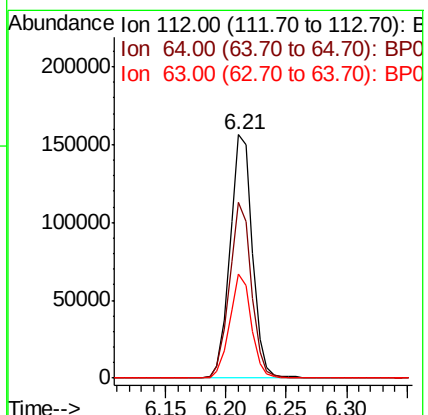

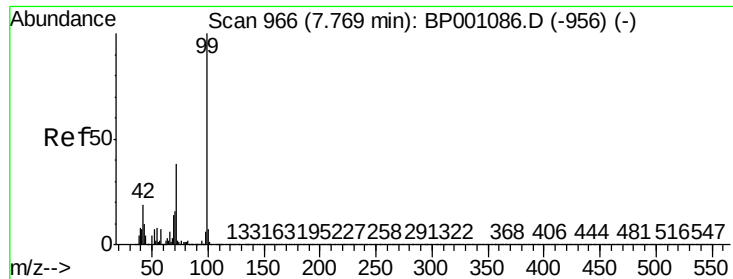

#7

Phenol-d6

Concen: 42.039 ng

RT: 7.75 min Scan# 963

Delta R.T. -0.01 min

Lab File: BP001244.D

Acq: 06 Dec 2019 22:21

Instrument :

BNA_P

ClientSampleId :


Tot Ion: 99 Resp: 275551

Ion Ratio Lower Upper

99 100

42 24.6 17.6 26.4




71 46.2 33.8 50.8

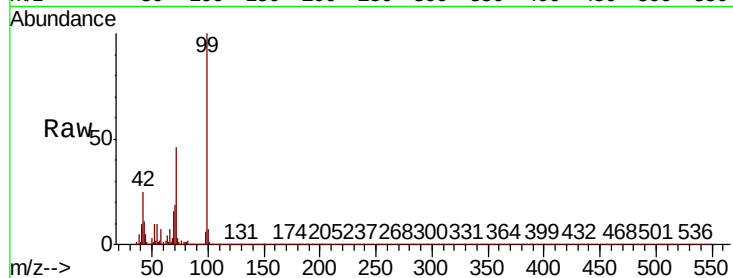

Abundance Ion 99.00 (98.70 to 99.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 71.00 (70.70 to 71.70): BP0

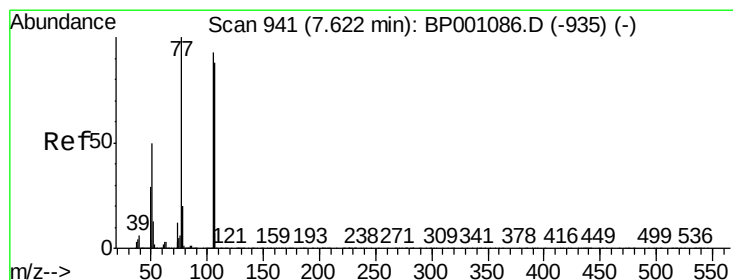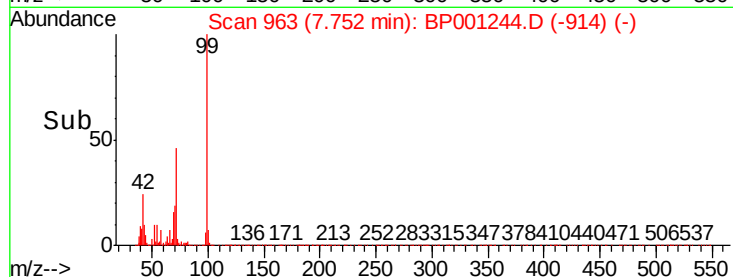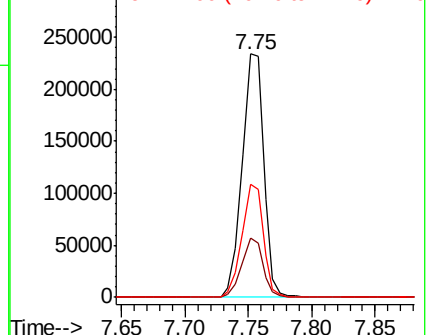

#9

Benzaldehyde

Concen: Below Cal

RT: 7.60 min Scan# 938

Delta R.T. -0.01 min

Lab File: BP001244.D

Acq: 06 Dec 2019 22:21


Tgt Ion: 77 Resp: 3762

Ion Ratio Lower Upper

77 100

105 92.5 69.7 109.7



106 85.4 67.1 107.1

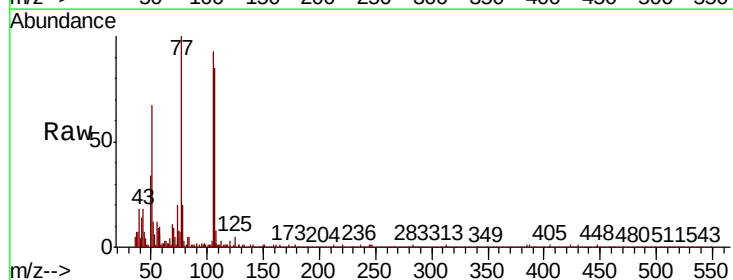


Abundance Ion 77.00 (76.70 to 77.70): BP0

Ion 105.00 (104.70 to 105.70): E

Ion 106.00 (105.70 to 106.70): E

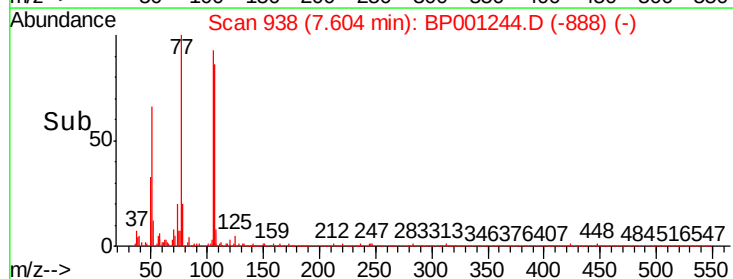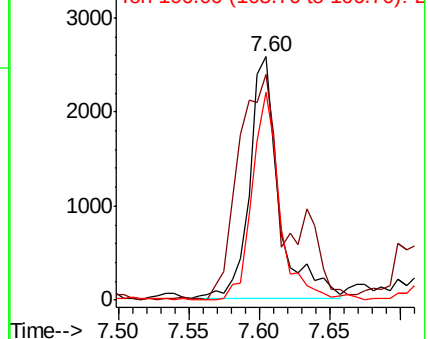







#17
2-Methylphenol
Concen: 8.210 ng
RT: 8.73 min Scan# 1129
Delta R.T. -0.01 min
Lab File: BP001244.D
Acq: 06 Dec 2019 22:21

Instrument :
BNA_P
ClientSampled :

Tot Ion:	107	Resp:	38336
Ion	Ratio	Lower	Upper
107	100		
108	110.9	88.8	133.2
77	59.0	46.3	69.5
79	59.1	46.6	70.0

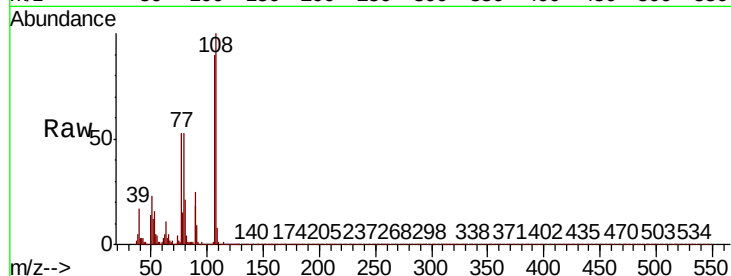


Abundance Ion 107.00 (106.70 to 107.70): E
Ion 108.00 (107.70 to 108.70): E
Ion 77.00 (76.70 to 77.70): BP0
Ion 79.00 (78.70 to 79.70): BP0


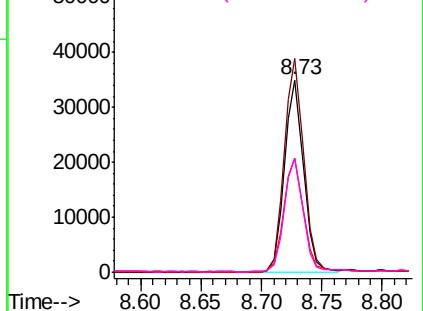



#19
n-Nitroso-di-n-propylamine
Concen: 5.964 ng
RT: 9.19 min Scan# 1207
Delta R.T. 0.21 min
Lab File: BP001244.D
Acq: 06 Dec 2019 22:21

Tgt Ion:	70	Resp:	28206
Ion	Ratio	Lower	Upper
70	100		
42	50.9	50.6	76.0
101	0.1	7.1	10.7#
130	1.2	13.6	20.4#



Abundance Ion 70.00 (69.70 to 70.70): BP0
Ion 42.00 (41.70 to 42.70): BP0
Ion 101.00 (100.70 to 101.70): E
Ion 130.00 (129.70 to 130.70): E




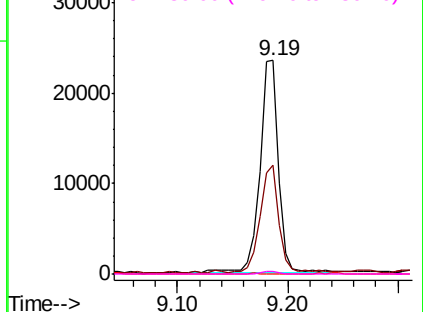




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.35 min Scan# 1404
Delta R.T. -0.01 min
Lab File: BP001244.D
Acq: 06 Dec 2019 22:21




Instrument :
BNA_P
ClientSampleId :


Tot Ion:136	Resp:	303653
Ion Ratio	Lower	Upper
136	100	
137	10.4	8.4 12.6
54	10.0	7.4 11.0
68	5.4	4.6 7.0

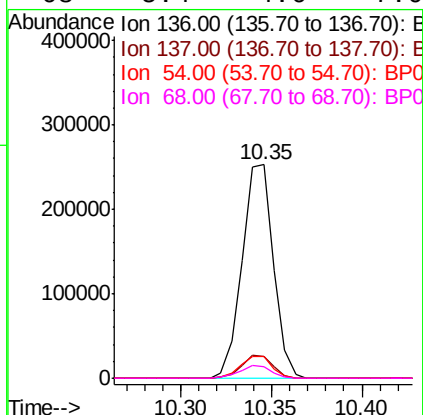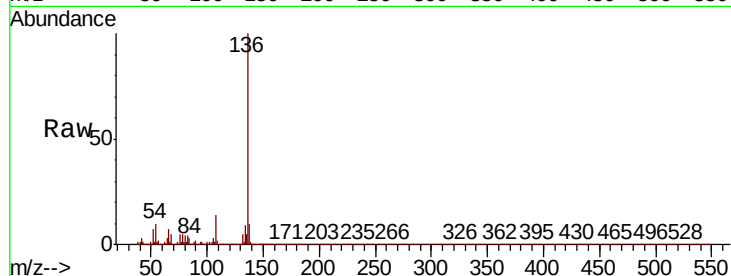

#23
Nitrobenzene-d5
Concen: 26.701 ng
RT: 9.19 min Scan# 1207
Delta R.T. -0.01 min
Lab File: BP001244.D
Acq: 06 Dec 2019 22:21

Tgt Ion: 82	Resp:	186878
Ion Ratio	Lower	Upper
82	100	
128	34.3	27.5 41.3
54	57.2	45.7 68.5


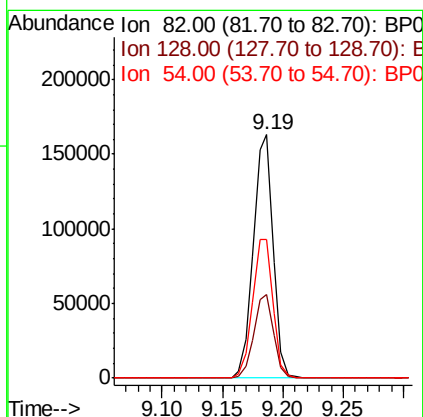






#31
Naphthalene
Concen: 10.001 ng
RT: 10.37 min Scan# 1409
Delta R.T. -0.01 min
Lab File: BP001244.D
Acq: 06 Dec 2019 22:21




Instrument :
BNA_P
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
128	100		
129	11.4	8.3	12.5
127	13.4	10.6	16.0

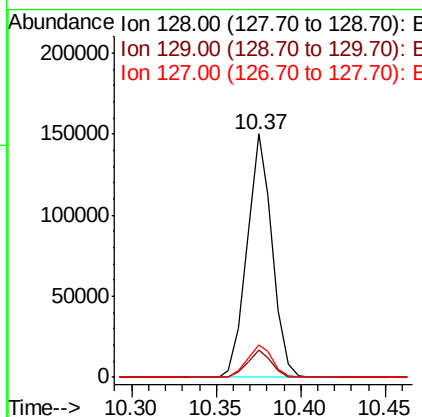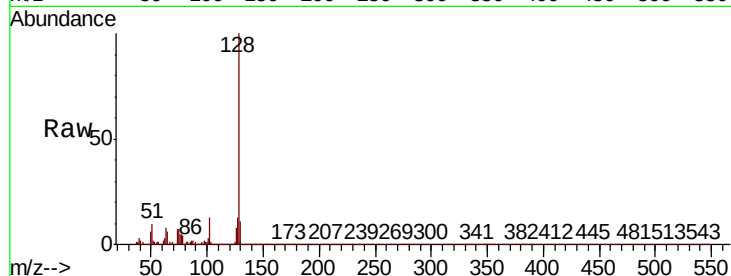

#33
4-Chloroaniline
Concen: 3.131 ng
RT: 10.37 min Scan# 1409
Delta R.T. -0.10 min
Lab File: BP001244.D
Acq: 06 Dec 2019 22:21

Tgt Ion	Ratio	Lower	Upper
127	100		
129	85.2	25.6	38.4#
65	0.0	33.6	50.4#
92	0.3	19.8	29.6#



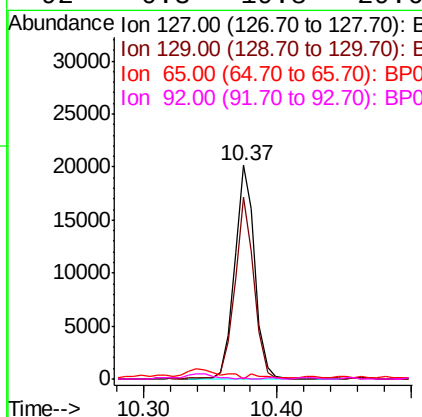



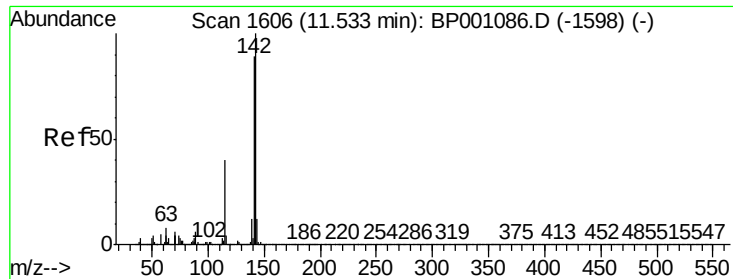

#37
 2-Methylnaphthalene
 Concen: 3.576 ng
 RT: 11.51 min Scan# 1602
 Delta R.T. -0.01 min
 Lab File: BP001244.D
 Acq: 06 Dec 2019 22:21




Instrument :
 BNA_P
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
142	100		
141	85.0	71.6	107.4
115	46.0	36.0	54.0

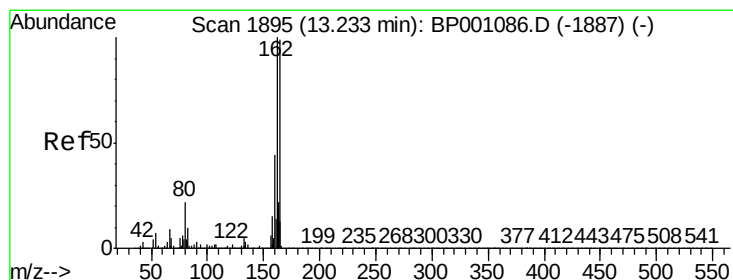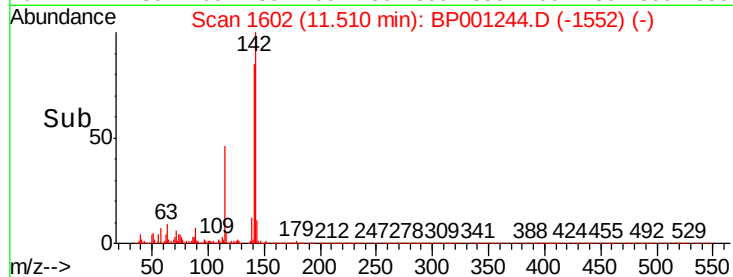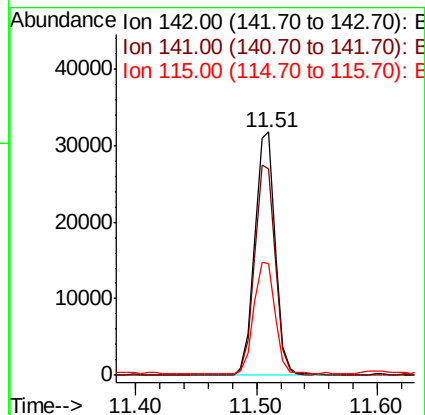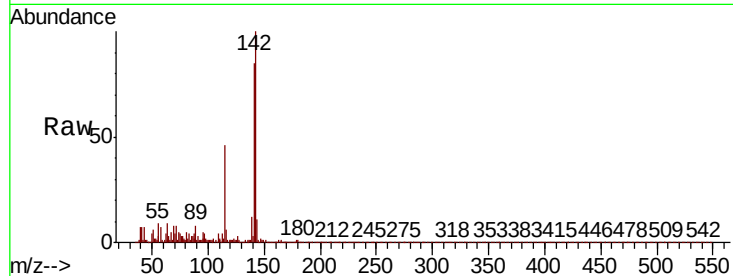

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 13.20 min Scan# 1890
 Delta R.T. -0.01 min
 Lab File: BP001244.D
 Acq: 06 Dec 2019 22:21

Tgt Ion	Ratio	Lower	Upper
164	100		
162	103.7	80.7	121.1
160	46.5	36.3	54.5

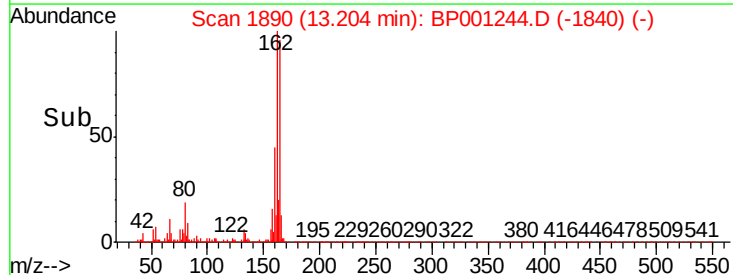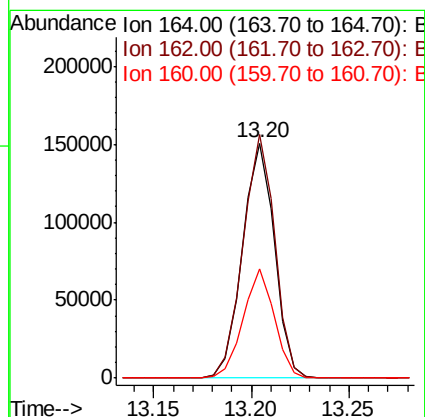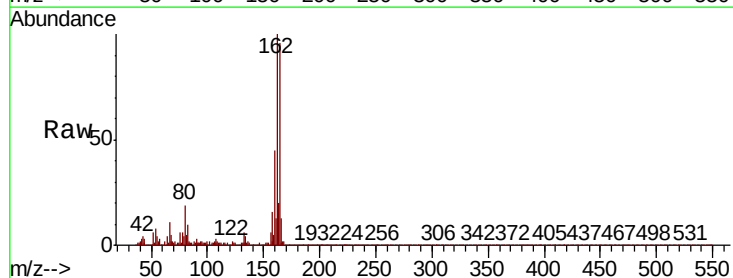


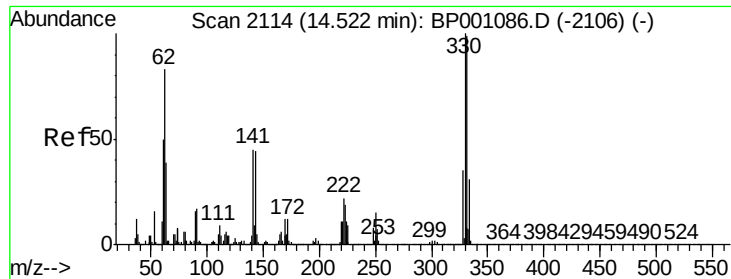

#42
2,4,6-Tribromophenol
Concen: 43.980 ng
RT: 14.49 min Scan# 2109
Delta R.T. -0.01 min
Lab File: BP001244.D
Acq: 06 Dec 2019 22:21

Instrument :
BNA_P
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.8	79.1	118.7
141	46.7	35.9	53.9



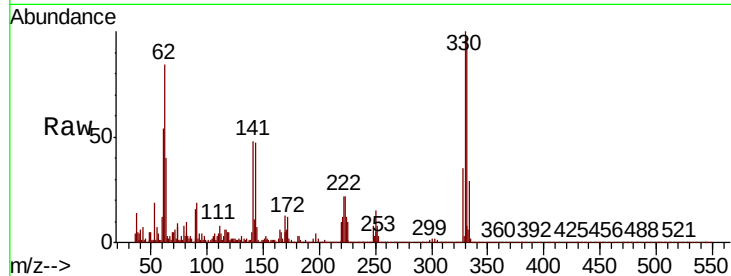


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

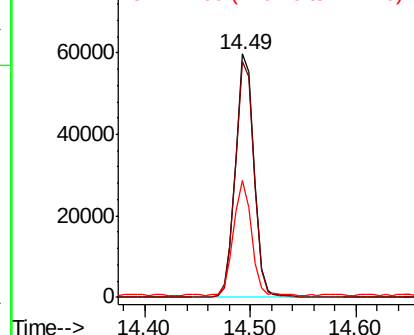

#45
2-Fluorobiphenyl
Concen: 27.389 ng
RT: 12.12 min Scan# 1706
Delta R.T. -0.01 min
Lab File: BP001244.D
Acq: 06 Dec 2019 22:21

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.2	28.7	43.1
170	23.2	19.2	28.8






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

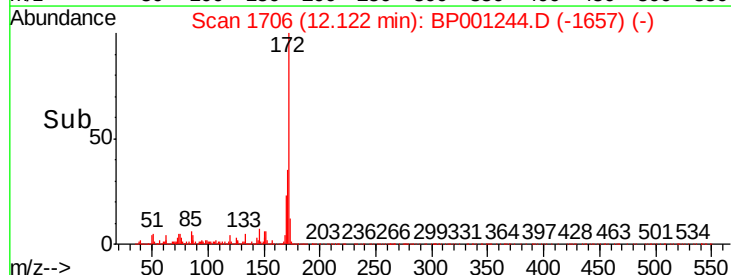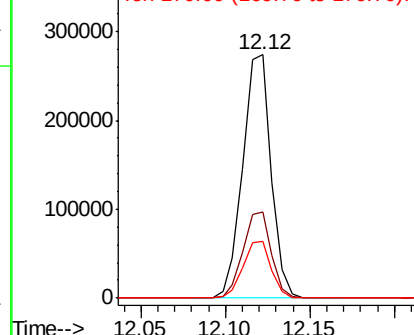



#50

Dimethylphthalate

Concen: 2.871 ng

RT: 12.79 min Scan# 1819

Delta R.T. -0.02 min

Lab File: BP001244.D

Acq: 06 Dec 2019 22:21

Instrument :

BNA_P

ClientSampleId :


Tot Ion:163 Resp: 36742

Ion Ratio Lower Upper

163 100

194 4.6 3.1 4.7




164 11.0 8.2 12.4



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

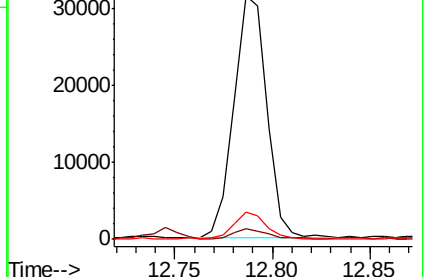

#52

Acenaphthene

Concen: 3.332 ng

RT: 13.25 min Scan# 1898

Delta R.T. -0.02 min

Lab File: BP001244.D

Acq: 06 Dec 2019 22:21


Tgt Ion:154 Resp: 31730

Ion Ratio Lower Upper

154 100

153 107.2 90.3 135.5



152 49.1 42.9 64.3




Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E




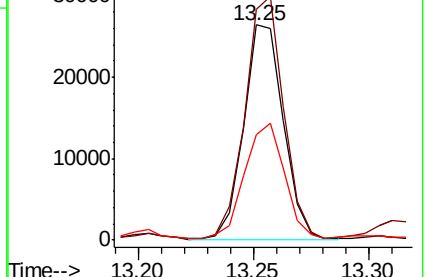


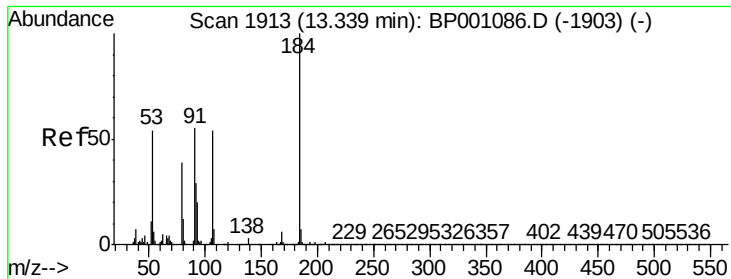

#54
2,4-Dinitrophenol
Concen: 7.119 ng
RT: 13.33 min Scan# 1911
Delta R.T. 0.01 min
Lab File: BP001244.D
Acq: 06 Dec 2019 22:21




Instrument :
BNA_P
ClientSampleId :


Tot Ion:184 Resp: 12
Ion Ratio Lower Upper
184 100
63 1013.0 69.4 104.0#
154 521.7 57.4 86.2#

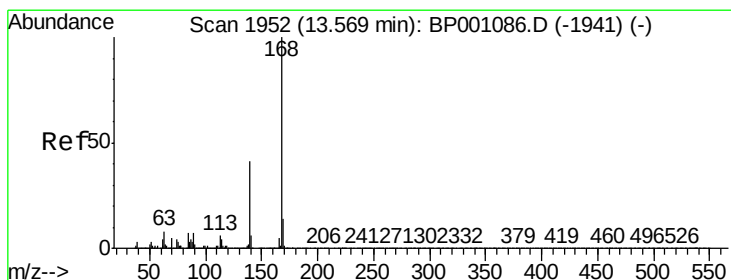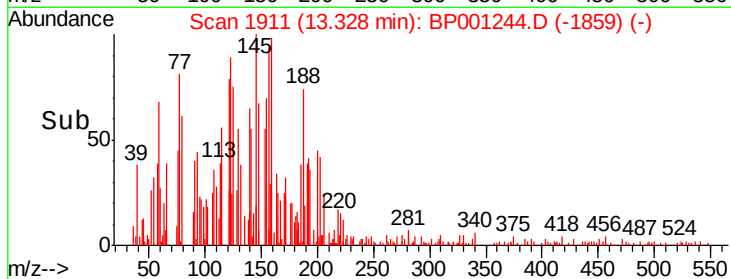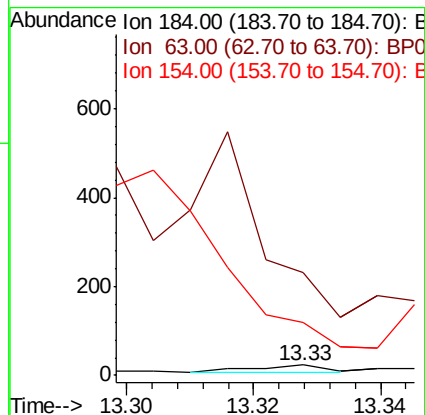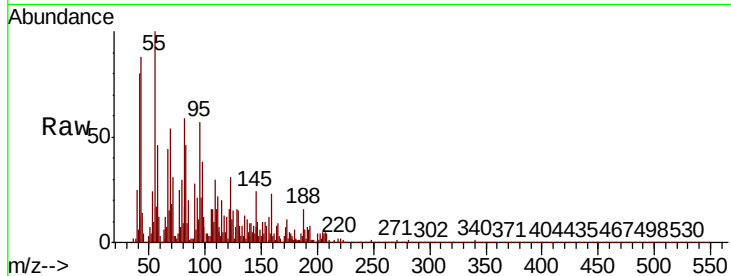

#55
Dibenzofuran
Concen: 3.109 ng
RT: 13.54 min Scan# 1947
Delta R.T. -0.01 min
Lab File: BP001244.D
Acq: 06 Dec 2019 22:21

Tgt Ion:168 Resp: 44487
Ion Ratio Lower Upper
168 100
139 43.5 34.5 51.7
169 15.2 10.8 16.2

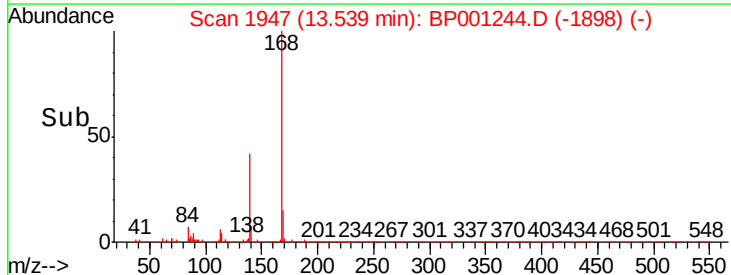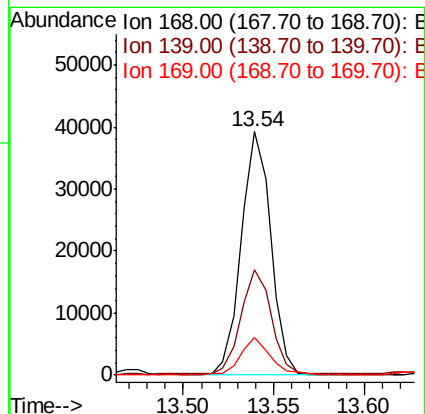

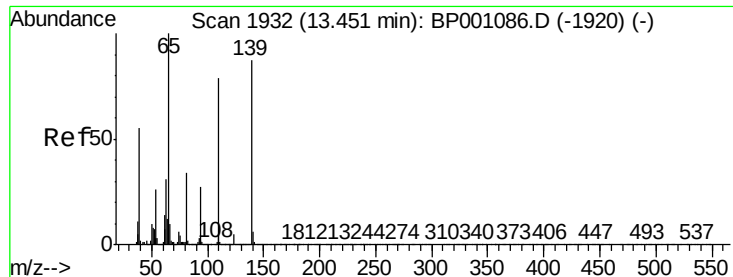

#56

4-Nitrophenol

Concen: 9.077 ng

RT: 13.54 min Scan# 1947

Delta R.T. 0.10 min

Lab File: BP001244.D





Acq: 06 Dec 2019 22:21

Instrument :

BNA_P

ClientSampleId :

Tot Ion	Ratio	Lower	Upper
139	100		
109	9.4	87.8	127.8#
65	6.0	111.9	151.9#

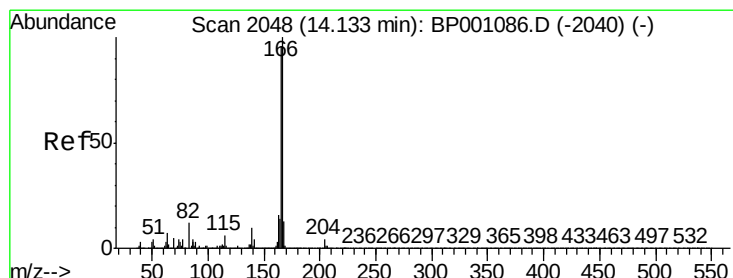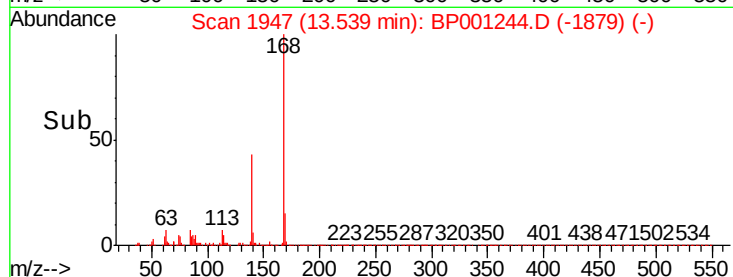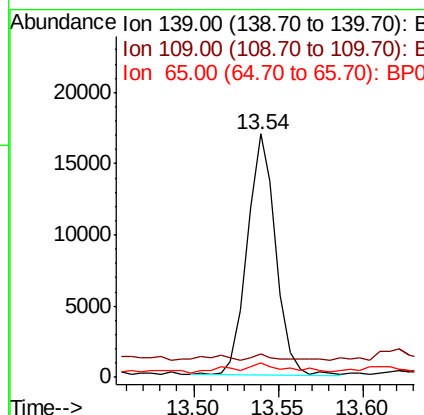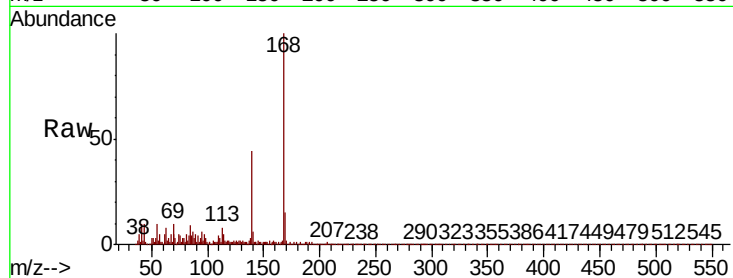

#58

Fluorene

Concen: 3.170 ng




RT: 14.10 min Scan# 2043


Delta R.T. -0.01 min

Lab File: BP001244.D

Acq: 06 Dec 2019 22:21

Tgt Ion	Ratio	Lower	Upper
166	100		
165	98.5	77.8	116.8
167	13.1	10.5	15.7

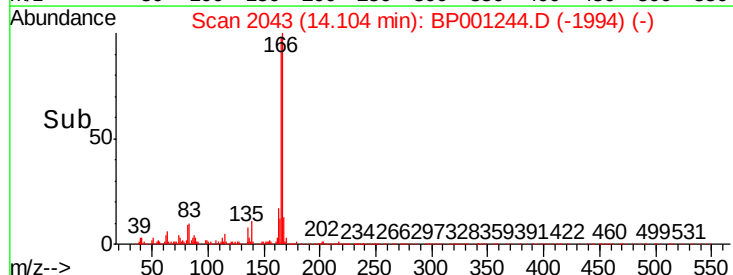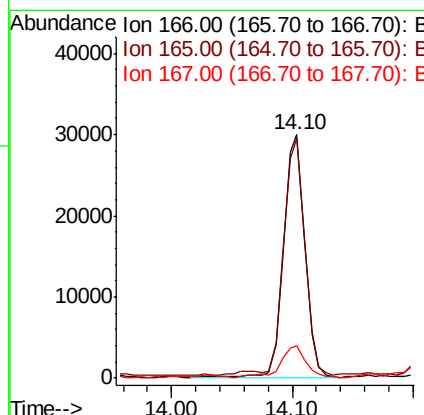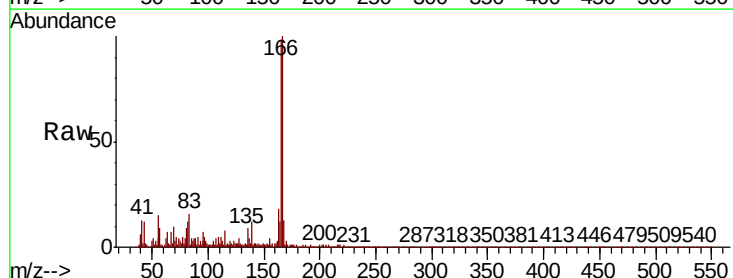







#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 15.60 min Scan# 2298
Delta R.T. -0.01 min
Lab File: BP001244.D
Acq: 06 Dec 2019 22:21

Instrument :
BNA_P
ClientSampleId :

Tot Ion:188 Resp: 320385
Ion Ratio Lower Upper
188 100
94 8.2 7.1 10.7
80 9.0 7.8 11.6




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BP0
Ion 80.00 (79.70 to 80.70): BP0


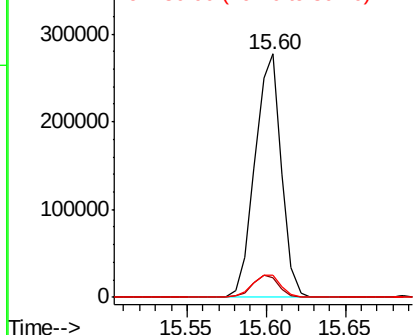



#65
4,6-Dinitro-2-methylphenol
Concen: 6.283 ng
RT: 14.22 min Scan# 2062
Delta R.T. 0.01 min
Lab File: BP001244.D
Acq: 06 Dec 2019 22:21

Tgt Ion:198 Resp: 10
Ion Ratio Lower Upper
198 100
51 1504.3 36.2 76.2#
105 4400.0 30.2 70.2#



Abundance Ion 198.00 (197.70 to 198.70): E
Ion 51.00 (50.70 to 51.70): BP0
Ion 105.00 (104.70 to 105.70): E



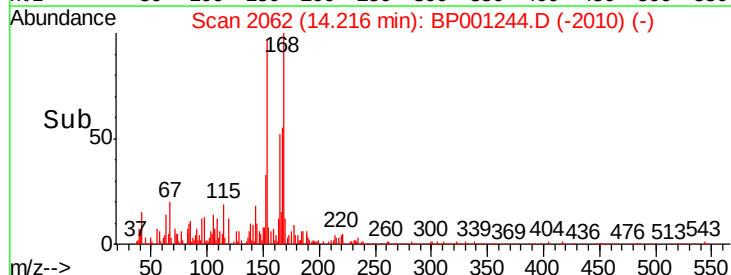
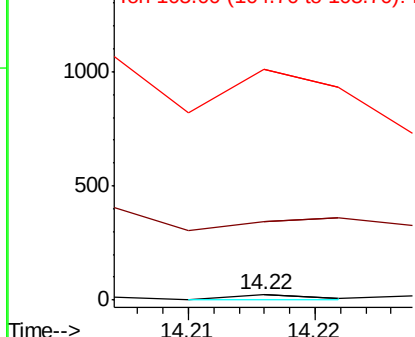




#71
Phenanthrene
Concen: 10.368 ng
RT: 15.63 min Scan# 2303
Delta R.T. -0.01 min
Lab File: BP001244.D
Acq: 06 Dec 2019 22:21




Instrument :
BNA_P
ClientSampleId :


Tot Ion:178 Resp: 174632
Ion Ratio Lower Upper
178 100
176 19.3 15.7 23.5
179 16.0 12.4 18.6

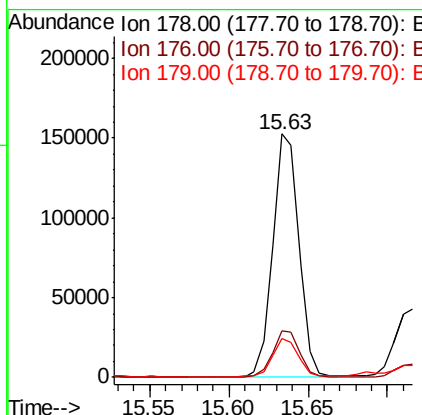

#72
Anthracene
Concen: 2.947 ng
RT: 15.72 min Scan# 2317
Delta R.T. -0.01 min
Lab File: BP001244.D
Acq: 06 Dec 2019 22:21

Tgt Ion:178 Resp: 48930
Ion Ratio Lower Upper
178 100
176 18.6 15.1 22.7
179 17.2 12.7 19.1

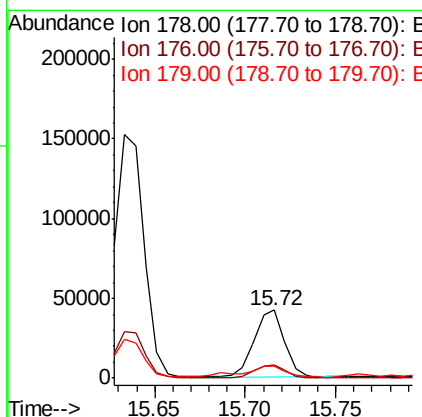



#75

Fluoranthene

Concen: 6.363 ng

RT: 17.35 min Scan# 2594

Delta R.T. -0.01 min

Lab File: BP001244.D


Acq: 06 Dec 2019 22:21

Instrument :

BNA_P

ClientSampled :

Tot Ion:	202	Resp:	113469
Ion Ratio	Lower	Upper	
202	100		
101	10.3	0.0	30.0
203	17.8	0.0	37.1






Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

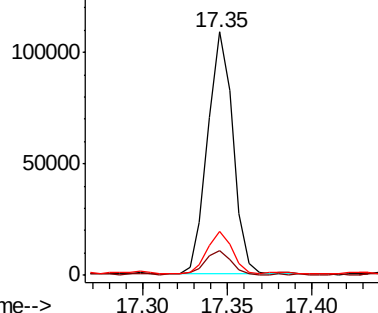

#76

Chrysene-d12

Concen: 20.000 ng


RT: 19.25 min Scan# 2917

Delta R.T. -0.01 min

Lab File: BP001244.D

Acq: 06 Dec 2019 22:21

Tgt Ion:	240	Resp:	253033
Ion Ratio	Lower	Upper	
240	100		
120	9.5	7.0	10.6
236	26.7	21.7	32.5






Abundance

Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

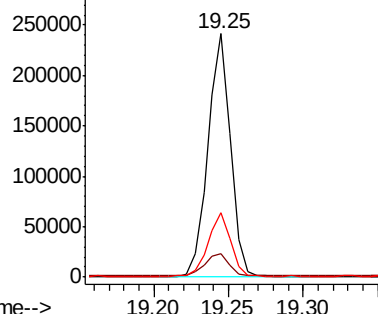

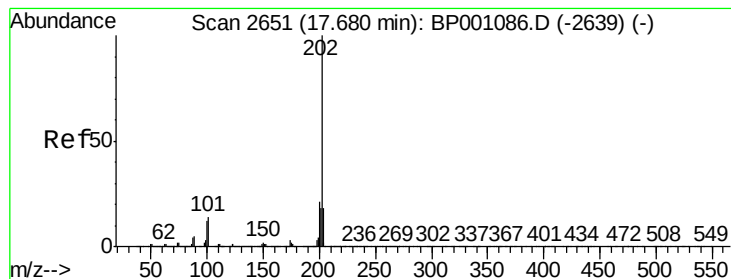

#78

Pvrene

Concen: 4.603 ng

RT: 17.65 min Scan# 2646

Delta R.T. -0.01 min

Lab File: BP001244.D





Acq: 06 Dec 2019 22:21

Instrument :

BNA_P

ClientSampleId :

Tot Ion:	202	Resp:	91726
Ion	Ratio	Lower	Upper
202	100		
200	22.9	17.3	25.9
203	21.0	13.8	20.8#

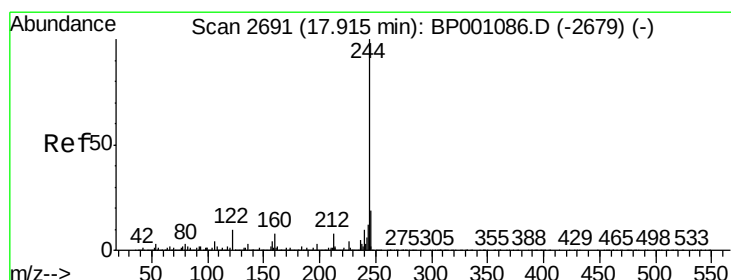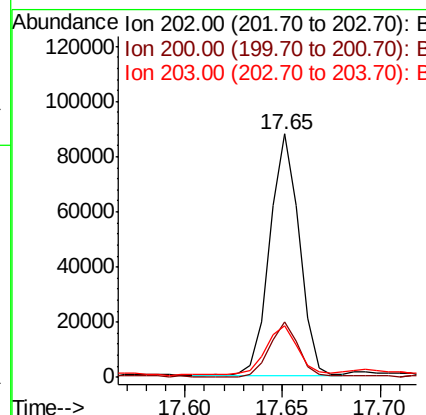

#79

Terphenyl-d14

Concen: 26.072 ng




RT: 17.88 min Scan# 2685


Delta R.T. -0.01 min

Lab File: BP001244.D

Acq: 06 Dec 2019 22:21

Tgt Ion:	244	Resp:	356587
Ion	Ratio	Lower	Upper
244	100		
212	8.4	6.6	9.8
122	11.0	9.2	13.8



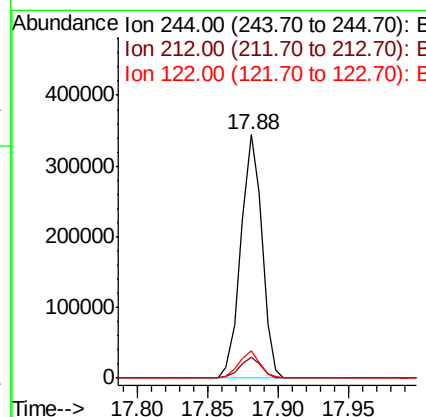
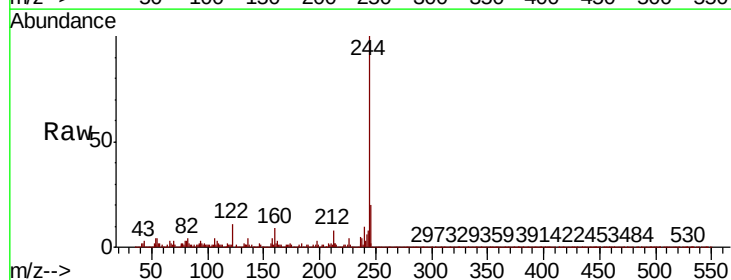


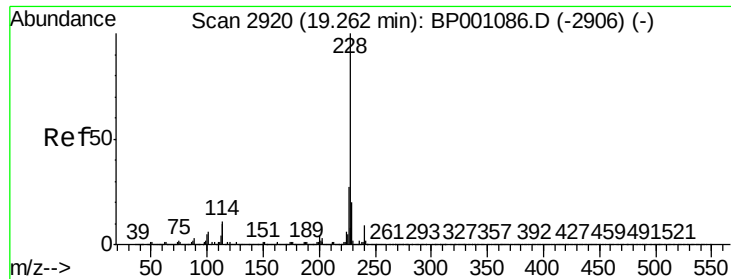

#81
Benzo(a)anthracene
Concen: 2.524 ng
RT: 19.23 min Scan# 2914
Delta R.T. -0.01 min
Lab File: BP001244.D
Acq: 06 Dec 2019 22:21




Instrument :
BNA_P
ClientSampleId :


Tot Ion:228 Resp: 44282
Ion Ratio Lower Upper
228 100
226 30.9 21.7 32.5
229 25.1 15.8 23.6#

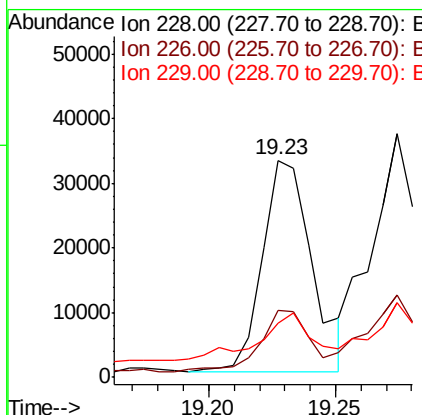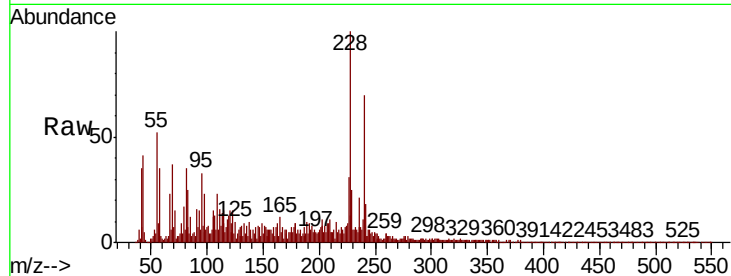

#83
Chrysene
Concen: 2.832 ng
RT: 19.27 min Scan# 2922
Delta R.T. -0.01 min
Lab File: BP001244.D
Acq: 06 Dec 2019 22:21

Tgt Ion:228 Resp: 44494
Ion Ratio Lower Upper
228 100
226 33.7 23.7 35.5
229 30.6 15.2 22.8#

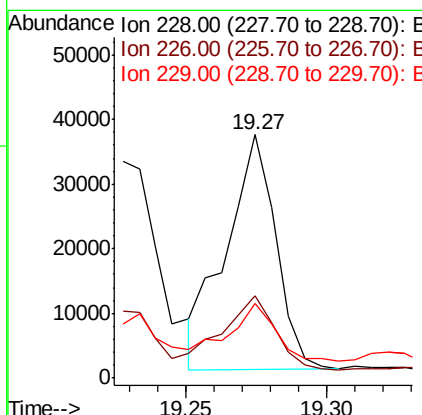



#84

Bis(2-ethylhexyl)phthalate

Concen: 12.060 ng

RT: 19.29 min Scan# 2924

Delta R.T. -0.01 min

Lab File: BP001244.D

Acq: 06 Dec 2019 22:21

Instrument :

BNA_P

ClientSampleId :


Tot Ion:149 Resp: 152630

Ion Ratio Lower Upper

149 100

167 28.3 20.8 31.2




279 4.4 2.8 4.2#



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

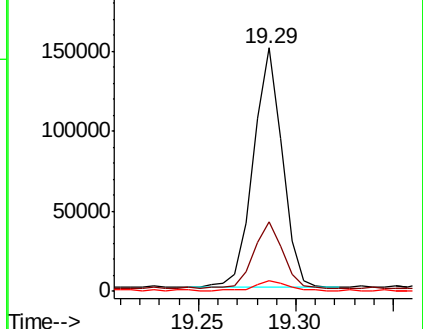

#87

Perylene-d12

Concen: 20.000 ng

RT: 21.02 min Scan# 3219

Delta R.T. -0.01 min

Lab File: BP001244.D

Acq: 06 Dec 2019 22:21


Tgt Ion:264 Resp: 257274

Ion Ratio Lower Upper

264 100

260 24.6 19.4 29.0



265 22.2 17.1 25.7




Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

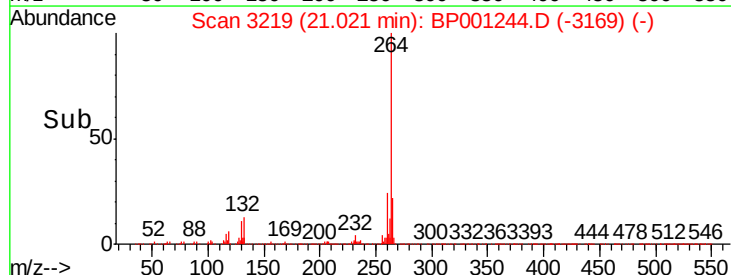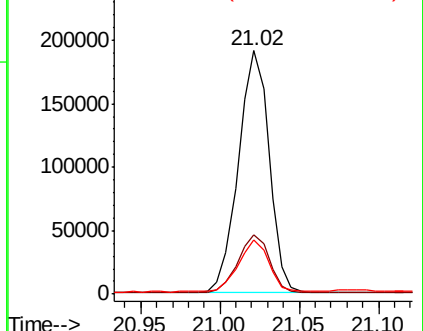



#88

Benzo(b)fluoranthene

Concen: 3.653 ng

RT: 20.53 min Scan# 3135

Delta R.T. -0.02 min

Lab File: BP001244.D

Acq: 06 Dec 2019 22:21

Instrument :

BNA_P

ClientSampleId :





Tot Ion:252 Resp: 57405

Ion Ratio Lower Upper

252 100

253 27.7 17.0 25.6#

125 25.1 6.6 9.8#

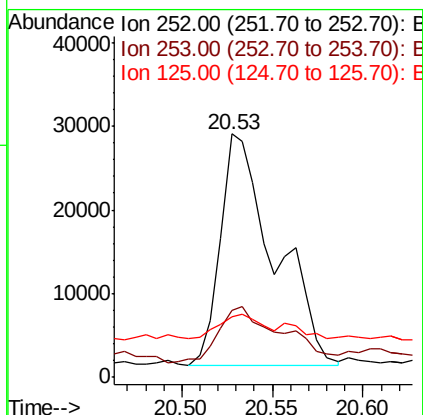

#89

Benzo(k)fluoranthene

Concen: 3.793 ng

RT: 20.53 min Scan# 3135

Delta R.T. -0.05 min

Lab File: BP001244.D

Acq: 06 Dec 2019 22:21




Tgt Ion:252 Resp: 57405


Ion Ratio Lower Upper

252 100

253 27.7 17.2 25.8#

125 25.1 6.2 9.4#

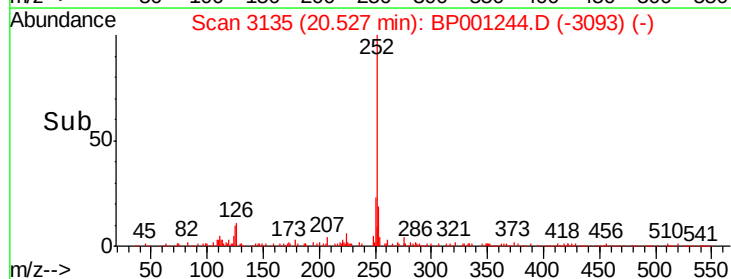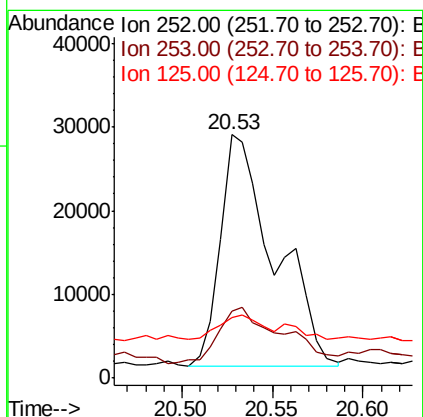

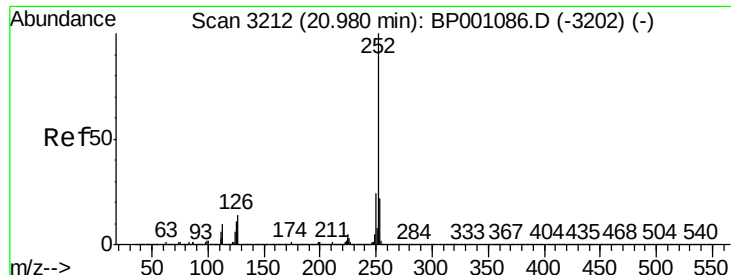

#90

Benzo(a)pyrene

Concen: 2.099 ng

RT: 20.94 min Scan# 3206

Delta R.T. -0.01 min

Lab File: BP001244.D

Acq: 06 Dec 2019 22:21

Instrument :

BNA_P

ClientSampleId :


Tot Ion: 252 Resp: 30384

Ion Ratio Lower Upper

252 100

253 32.3 16.8 25.2#

125 28.9 7.8 11.6#

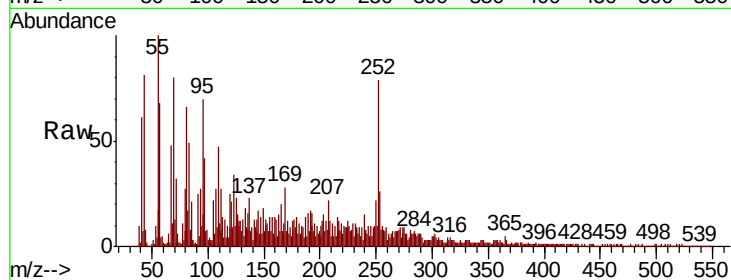

Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

