
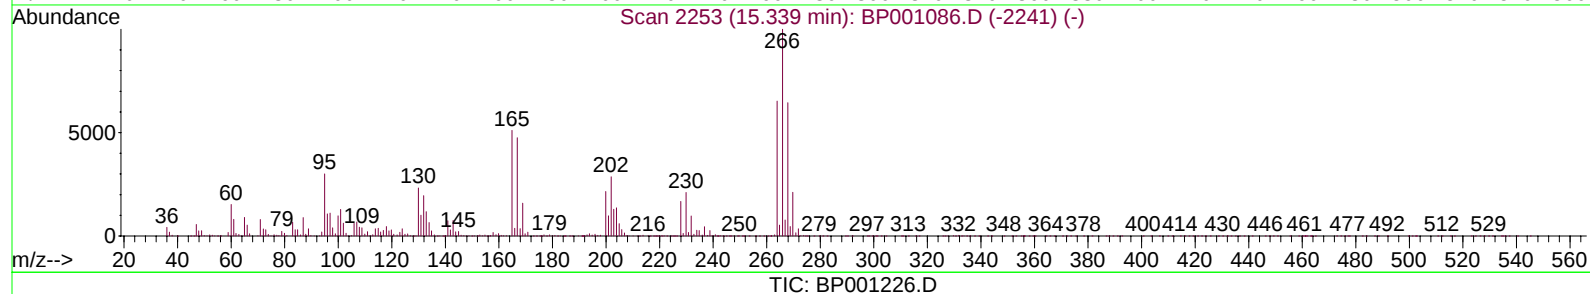
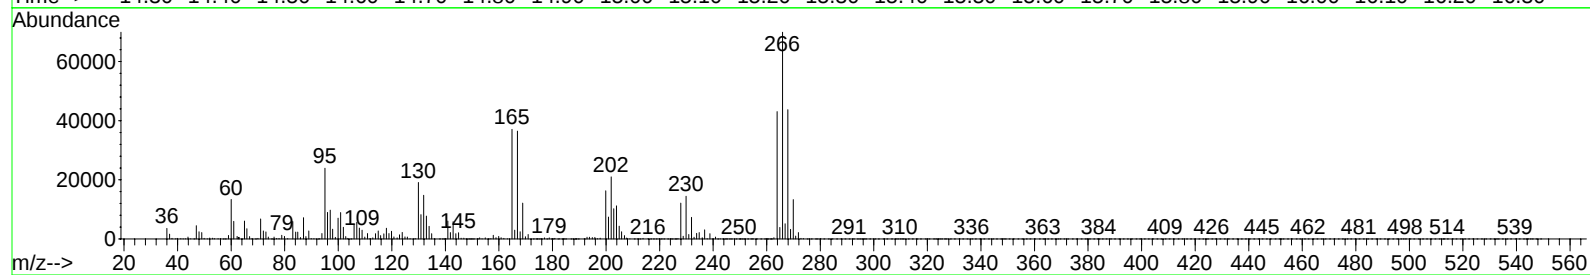


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP120619\
Data File : BP001226.D
Acq On : 06 Dec 2019 12:41
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 16:45:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 05 12:34:47 2019
Response via : Initial Calibration

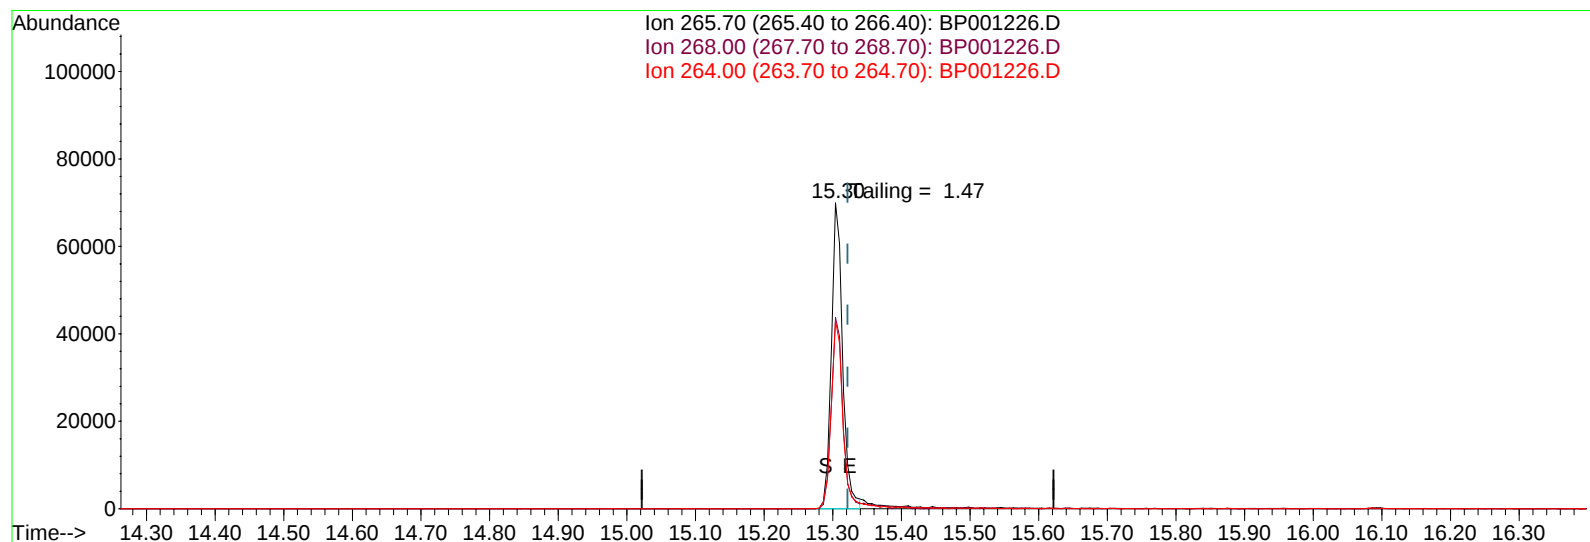

(70) Pentachlorophenol (C)




15.304min (-0.018) 2659394.50ng

response 82718

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	62.53
264.00	62.40	61.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP120619\
Data File : BP001226.D
Acq On : 06 Dec 2019 12:41
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 16:45:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 05 12:34:47 2019
Response via : Initial Calibration

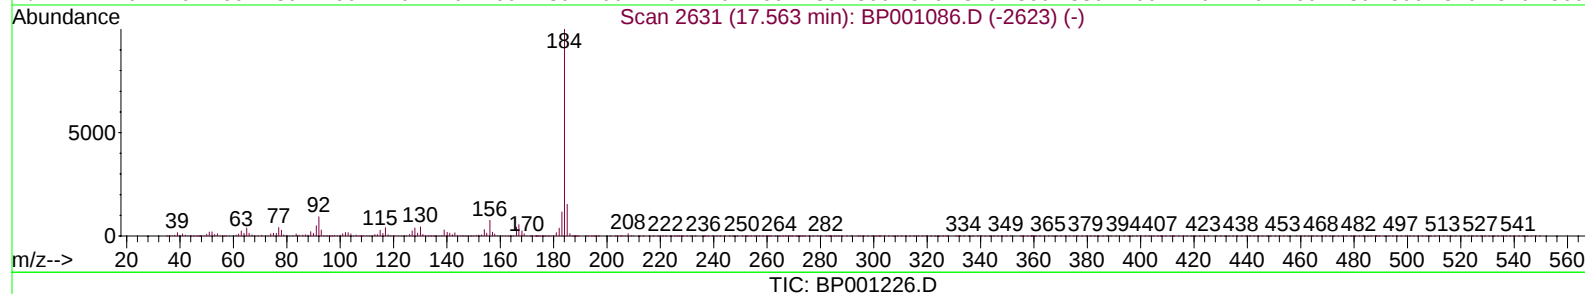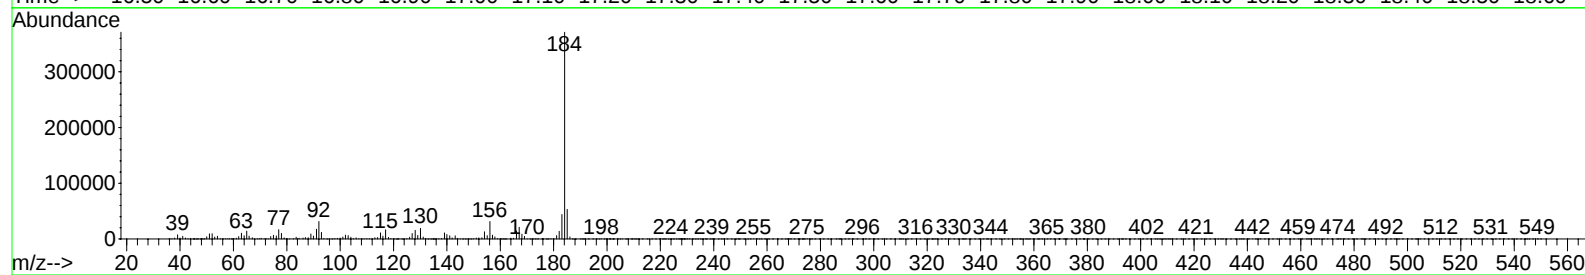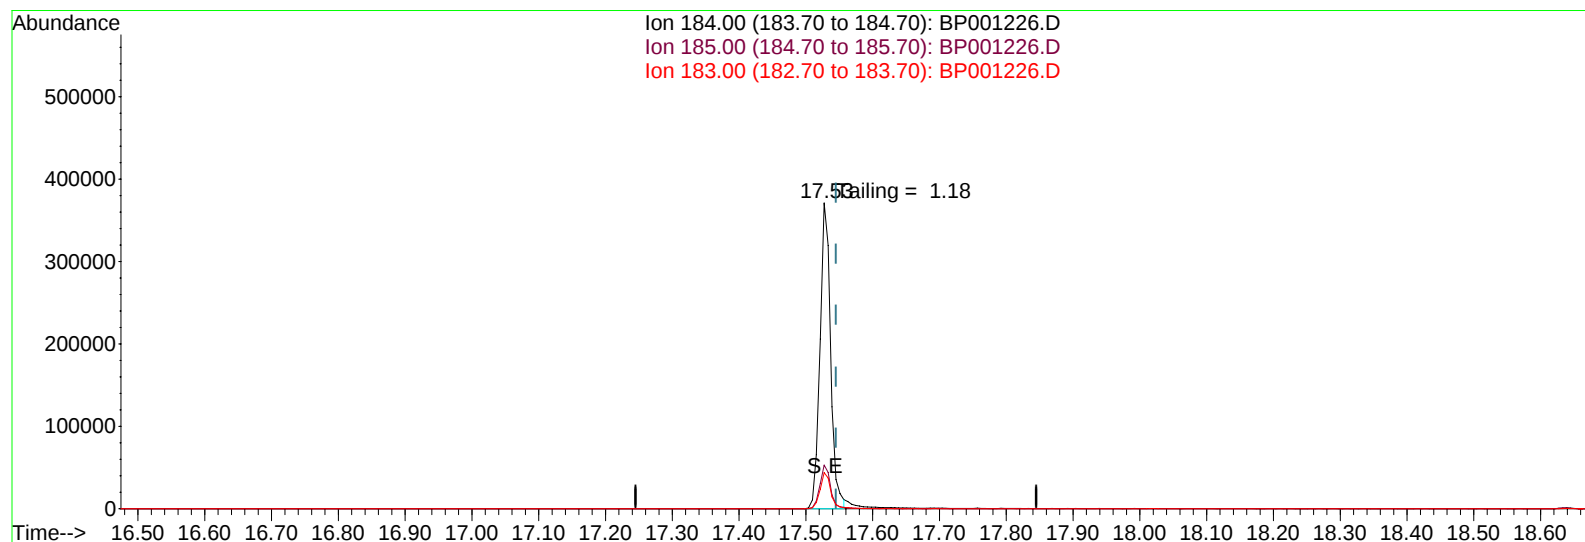

(77) Benzidine

17.527min (-0.018) 1372281.31ng

response 425175

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.30
183.00	11.20	11.85
0.00	0.00	0.00